

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
 Data File : VU052089.D
 Acq On : 23 Nov 2022 15:10
 Operator : JC/MD
 Sample : VU1123WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK142

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.392	12	16	30	rVB2	6103	9237	1.09%	0.138%
2	1.597	72	80	102	rVB	118681	143336	16.90%	2.145%
3	1.777	125	136	146	rBV6	8423	16943	2.00%	0.254%
4	1.913	169	178	200	rBV	95254	136536	16.10%	2.043%
5	2.565	369	381	398	rBV	184081	297225	35.04%	4.448%
6	3.048	519	531	543	rBV2	18202	34384	4.05%	0.515%
7	4.617	1003	1019	1044	rBV	135777	336674	39.69%	5.038%
8	5.060	1141	1157	1179	rBV	163726	360508	42.50%	5.395%
9	5.723	1343	1363	1400	rBV2	320198	848250	100.00%	12.694%
10	6.247	1512	1526	1546	rBV	255466	494419	58.29%	7.399%
11	6.543	1604	1618	1630	rVB4	8407	16688	1.97%	0.250%
12	6.687	1648	1663	1692	rBV	206658	402289	47.43%	6.020%
13	7.565	1924	1936	1955	rBV2	89591	159456	18.80%	2.386%
14	7.896	2025	2039	2075	rBV	351192	616461	72.67%	9.225%
15	8.179	2110	2127	2142	rBV2	56506	96271	11.35%	1.441%
16	8.633	2255	2268	2308	rBV	446259	838545	98.86%	12.548%
17	9.417	2498	2512	2530	rBV	371951	631007	74.39%	9.443%
18	10.755	2916	2928	2944	rBV	167255	267291	31.51%	4.000%
19	11.809	3244	3256	3291	rBV	295979	479105	56.48%	7.170%
20	12.192	3362	3375	3395	rBV	296738	497870	58.69%	7.450%




Sum of corrected areas: 6682495

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
Data File : VU052089.D
Acq On : 23 Nov 2022 15:10
Operator : JC/MD
Sample : VU1123WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK142

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

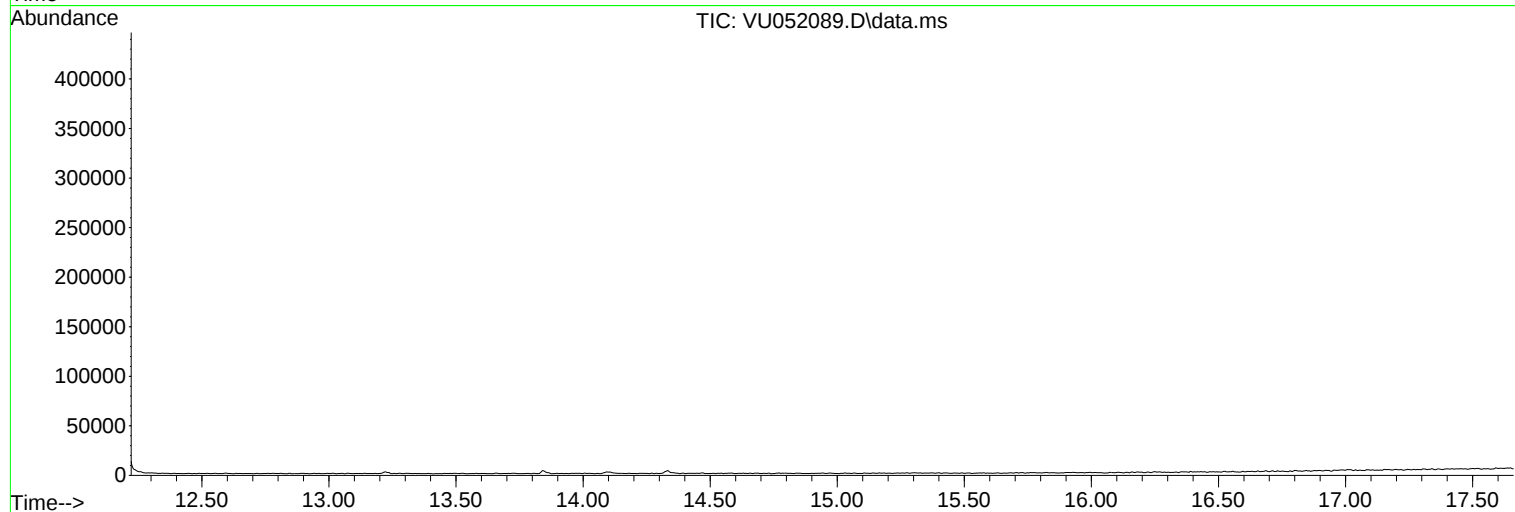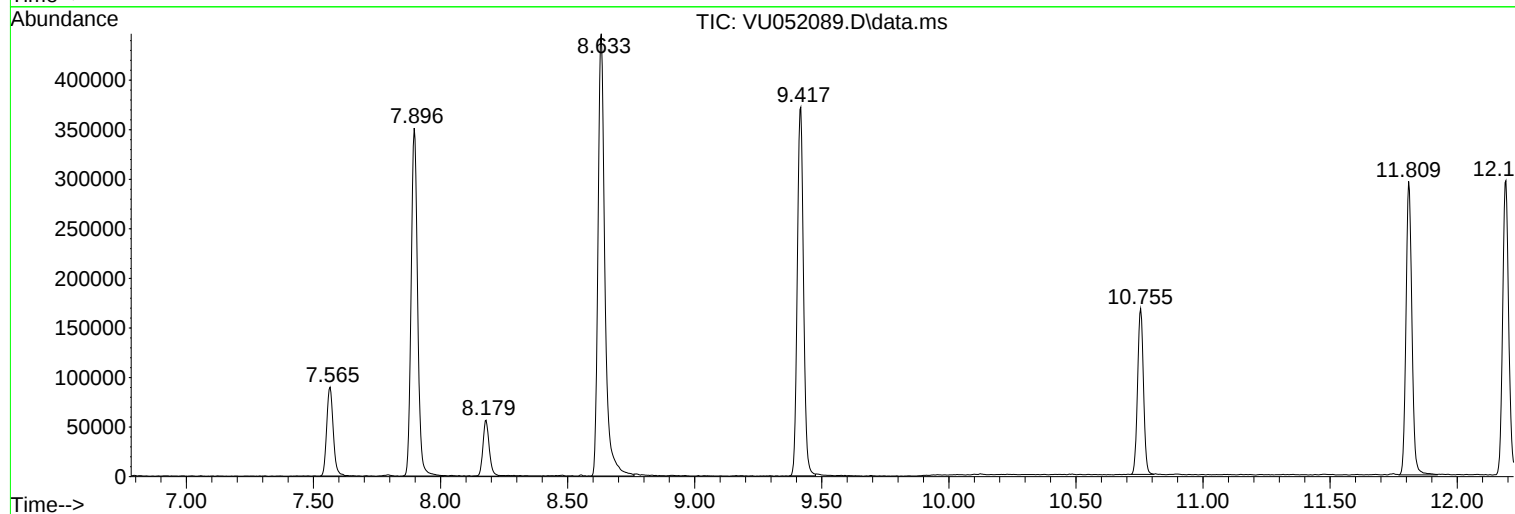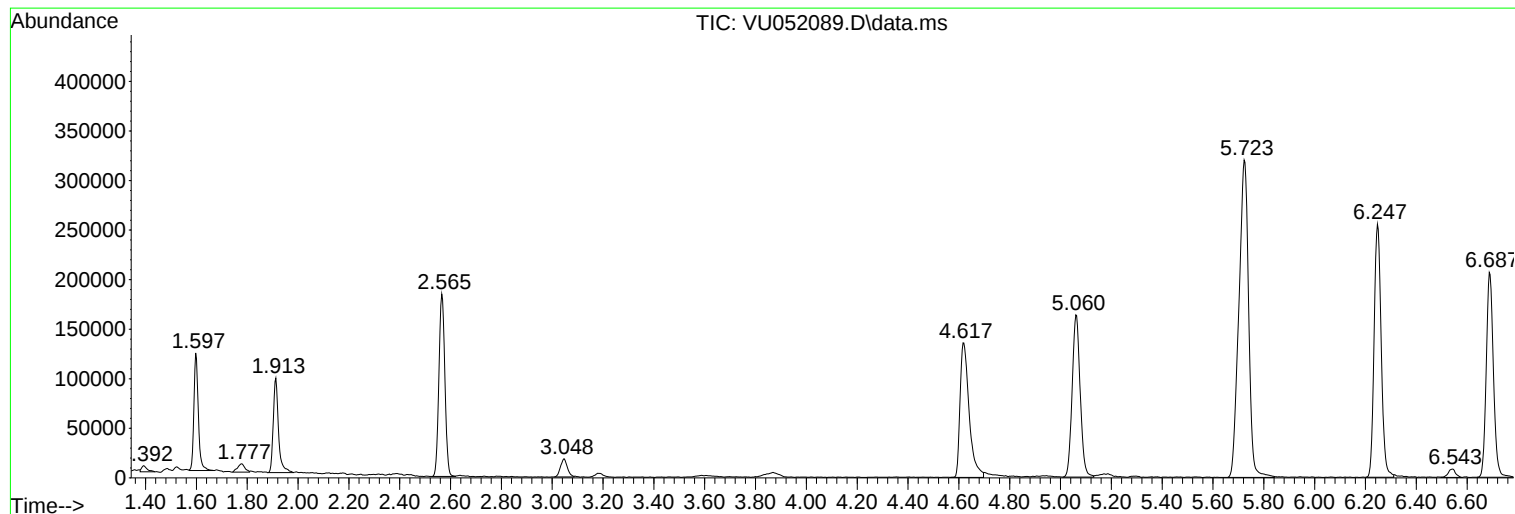

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
Data File : VU052089.D
Acq On : 23 Nov 2022 15:10
Operator : JC/MD
Sample : VU1123WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK142

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
Data File : VU052089.D
Acq On : 23 Nov 2022 15:10
Operator : JC/MD
Sample : VU1123WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK142

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc