

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
 Data File : VU052091.D
 Acq On : 23 Nov 2022 16:08
 Operator : JC/MD
 Sample : N5685-14
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052091.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.466	32	39	51	rBV	9619	21076	2.36%	0.299%
2	1.601	73	81	94	rBV	119450	138928	15.57%	1.972%
3	1.771	126	134	145	rVB5	9347	16380	1.84%	0.233%
4	1.912	169	178	194	rBV	98229	141274	15.83%	2.006%
5	2.565	370	381	397	rBV	184583	298993	33.50%	4.245%
6	3.044	519	530	548	rBV2	14243	29024	3.25%	0.412%
7	4.617	1007	1019	1049	rBV	142972	350356	39.25%	4.974%
8	5.060	1140	1157	1185	rBV	172672	393307	44.07%	5.584%
9	5.726	1339	1364	1386	rBV2	341283	892544	100.00%	12.671%
10	6.247	1509	1526	1547	rBV	271078	525904	58.92%	7.466%
11	6.542	1605	1618	1630	rBV4	9547	18291	2.05%	0.260%
12	6.687	1649	1663	1696	rBV	213460	427873	47.94%	6.075%
13	7.565	1924	1936	1956	rBV	95524	171083	19.17%	2.429%
14	7.896	2026	2039	2059	rBV	371833	655014	73.39%	9.299%
15	8.179	2114	2127	2143	rBV	60198	101753	11.40%	1.445%
16	8.632	2255	2268	2314	rBV	463018	880189	98.62%	12.496%
17	9.417	2498	2512	2538	rBV	395056	673560	75.47%	9.563%
18	10.755	2916	2928	2949	rBV	175236	280701	31.45%	3.985%
19	11.809	3244	3256	3278	rBV	309474	498075	55.80%	7.071%
20	12.192	3362	3375	3396	rBV	321888	529417	59.32%	7.516%




Sum of corrected areas: 7043742

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
Data File : VU052091.D
Acq On : 23 Nov 2022 16:08
Operator : JC/MD
Sample : N5685-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

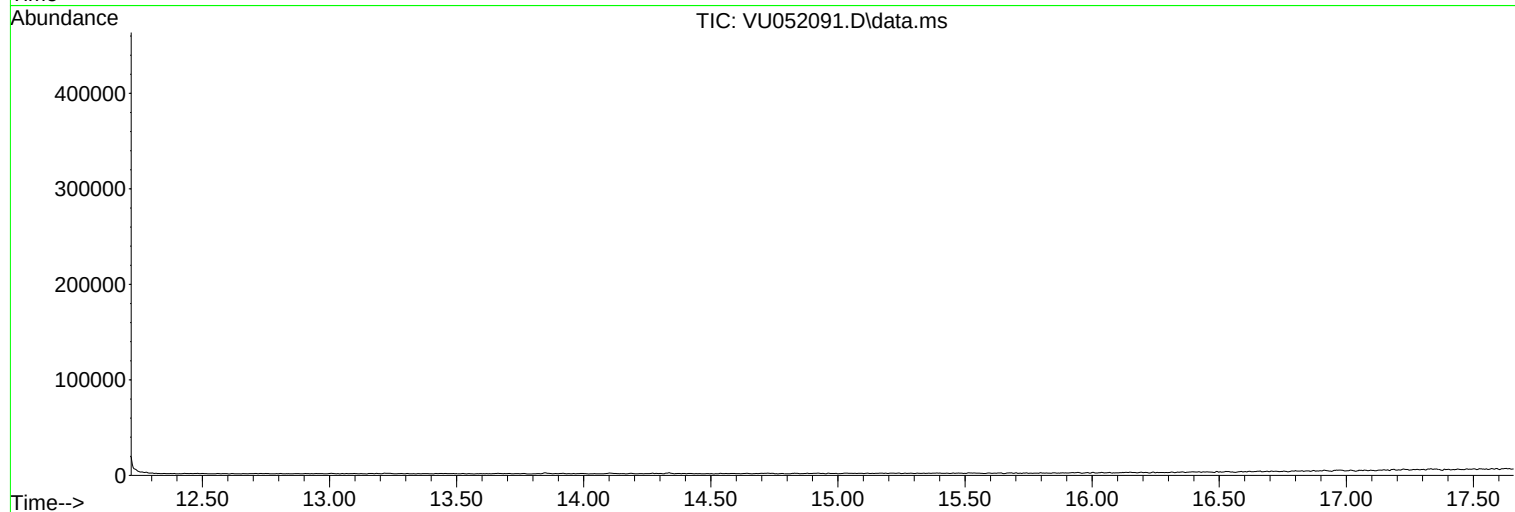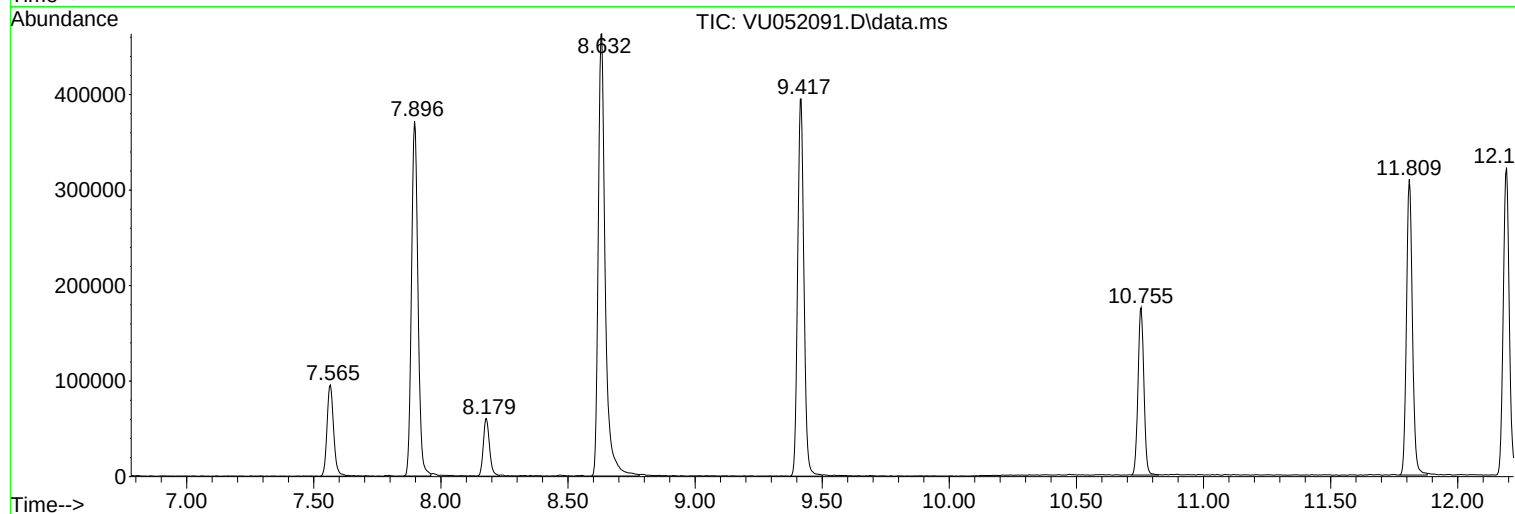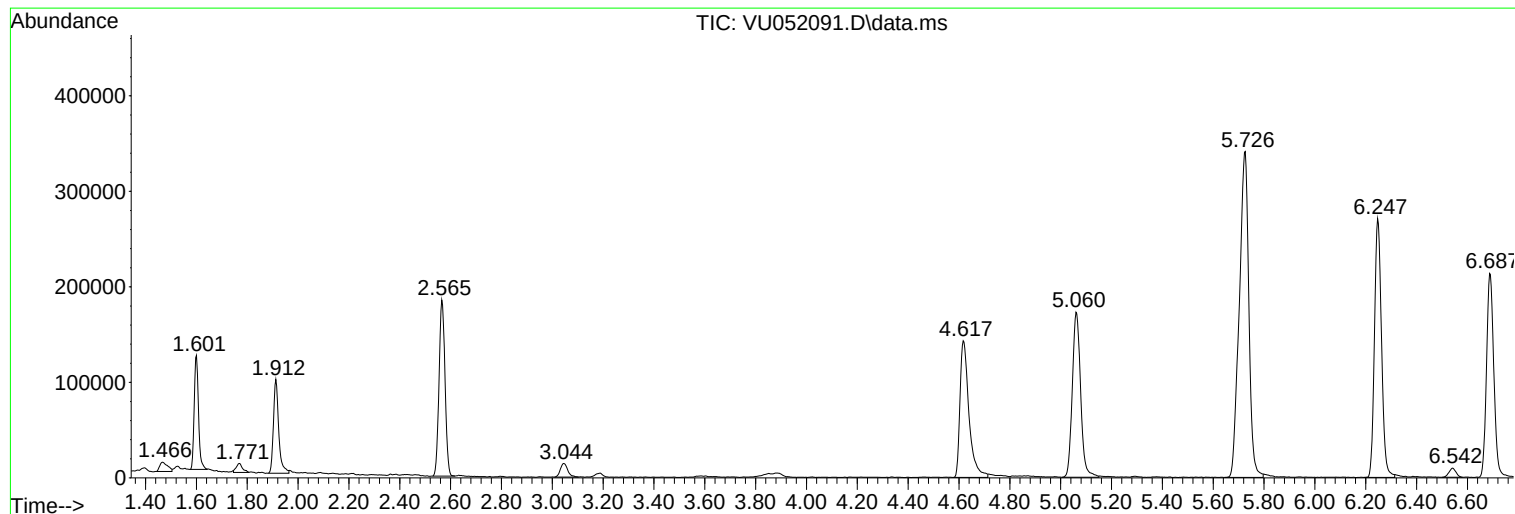

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
Data File : VU052091.D
Acq On : 23 Nov 2022 16:08
Operator : JC/MD
Sample : N5685-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
Data File : VU052091.D
Acq On : 23 Nov 2022 16:08
Operator : JC/MD
Sample : N5685-14
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc