

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
 Data File : VU052125.D
 Acq On : 24 Nov 2022 08:24
 Operator : JC/MD
 Sample : N5760-02DL 25X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COL17DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052125.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	33	42	52	rBV	10875	24480	2.55%	0.315%
2	1.601	74	81	97	rVB	103593	123976	12.94%	1.593%
3	1.774	126	135	141	rVB5	9637	13999	1.46%	0.180%
4	1.912	169	178	199	rVB	83110	117858	12.30%	1.514%
5	2.568	369	382	397	rBV	158394	257718	26.90%	3.311%
6	3.044	516	530	544	rBV	31130	59540	6.21%	0.765%
7	3.183	558	573	596	rVB	69315	156970	16.38%	2.017%
8	4.617	1003	1019	1057	rBV	164400	490681	51.21%	6.304%
9	5.060	1141	1157	1176	rBV	155089	342450	35.74%	4.400%
10	5.723	1343	1363	1392	rBV2	301387	798103	83.30%	10.254%
11	6.247	1513	1526	1547	rBV	249080	477086	49.79%	6.130%
12	6.539	1603	1617	1650	rBV	509343	958159	100.00%	12.310%
13	6.687	1650	1663	1680	rBV	202151	385891	40.27%	4.958%
14	7.565	1923	1936	1954	rBV	84196	149267	15.58%	1.918%
15	7.896	2026	2039	2052	rBV	321833	563209	58.78%	7.236%
16	7.967	2052	2061	2080	rVB2	53744	98312	10.26%	1.263%
17	8.179	2113	2127	2148	rBV	51497	89879	9.38%	1.155%
18	8.629	2255	2267	2300	rBV	457216	862094	89.97%	11.076%
19	9.414	2498	2511	2531	rBV	363911	614038	64.09%	7.889%
20	10.755	2915	2928	2947	rBV	168310	269999	28.18%	3.469%
21	11.809	3241	3256	3275	rBV	286271	452478	47.22%	5.813%
22	12.192	3362	3375	3397	rBV	284428	477246	49.81%	6.132%




Sum of corrected areas: 7783433

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
Data File : VU052125.D
Acq On : 24 Nov 2022 08:24
Operator : JC/MD
Sample : N5760-02DL 25X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COL17DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

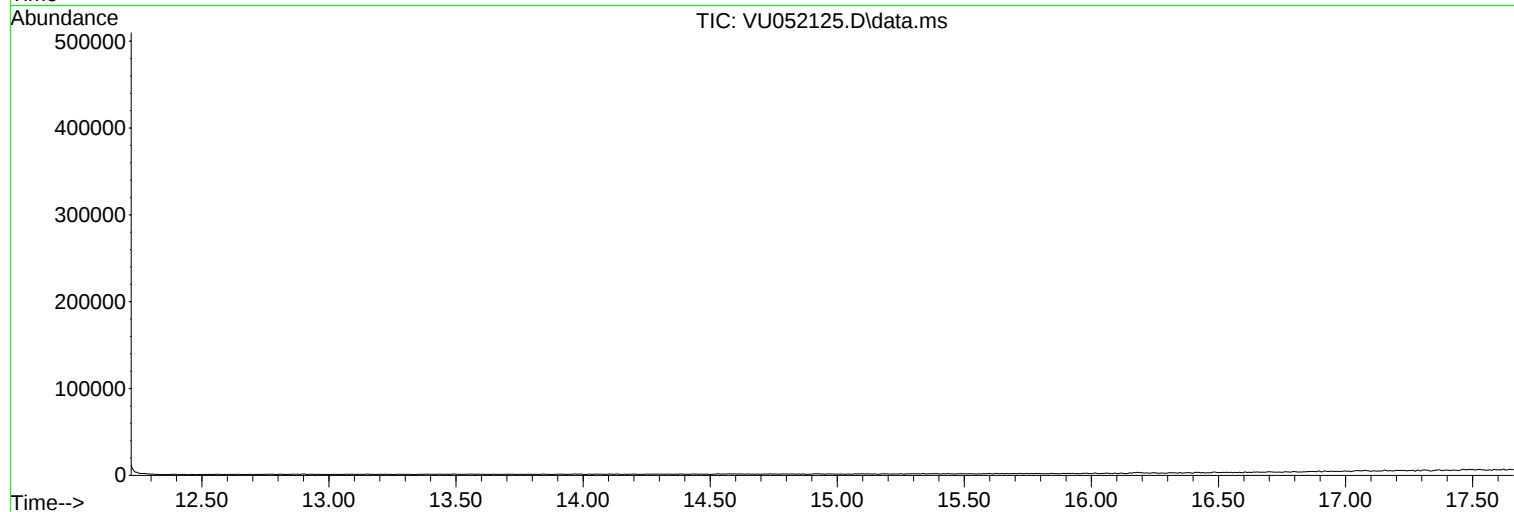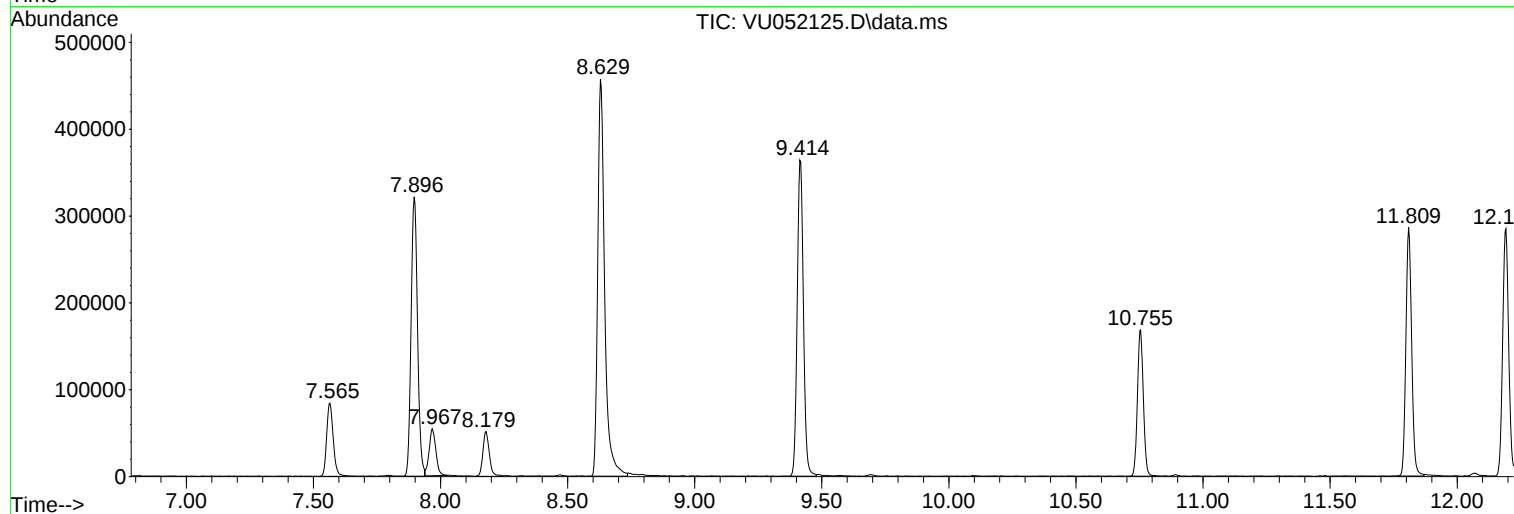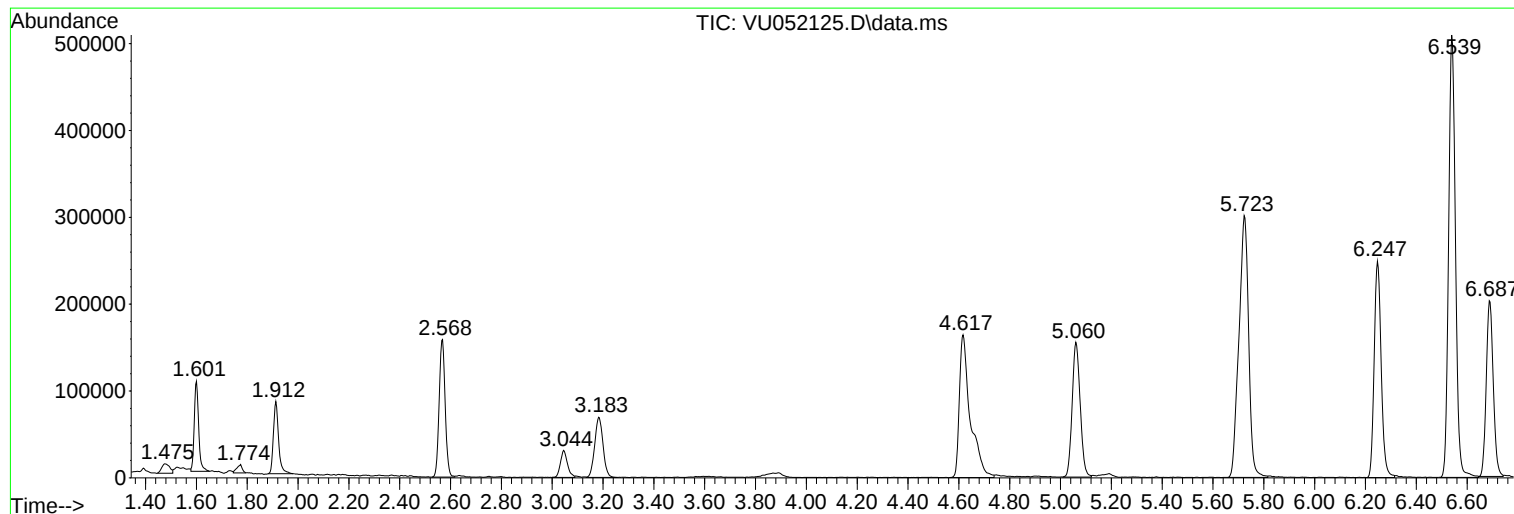

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
Data File : VU052125.D
Acq On : 24 Nov 2022 08:24
Operator : JC/MD
Sample : N5760-02DL 25X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L17DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
Data File : VU052125.D
Acq On : 24 Nov 2022 08:24
Operator : JC/MD
Sample : N5760-02DL 25X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COL17DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc