

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
 Data File : VU052128.D
 Acq On : 24 Nov 2022 09:46
 Operator : JC/MD
 Sample : N5760-06DL 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L21DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052128.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	102	rVB	107409	135816	15.66%	1.775%
2	1.774	125	135	136	rBV6	13271	13688	1.58%	0.179%
3	1.906	168	176	193	rBV	82884	122395	14.11%	1.600%
4	2.565	368	381	395	rBV	168702	275767	31.79%	3.604%
5	3.044	517	530	543	rBV2	25540	49772	5.74%	0.651%
6	3.182	557	573	595	rBV	81732	190075	21.91%	2.484%
7	3.899	767	796	817	rVB	6463	29966	3.45%	0.392%
8	4.616	1004	1019	1055	rBV	152702	440100	50.74%	5.752%
9	5.060	1141	1157	1178	rBV	162939	364487	42.02%	4.764%
10	5.722	1342	1363	1390	rBV2	314082	824225	95.02%	10.772%
11	6.247	1513	1526	1547	rBV	277209	531196	61.24%	6.943%
12	6.539	1603	1617	1640	rBV	307746	582180	67.12%	7.609%
13	6.690	1650	1664	1690	rBV	203188	399368	46.04%	5.220%
14	7.565	1923	1936	1958	rBV	86026	152739	17.61%	1.996%
15	7.896	2026	2039	2059	rBV	343646	598518	69.00%	7.822%
16	8.179	2116	2127	2149	rBV2	52019	90561	10.44%	1.184%
17	8.629	2254	2267	2294	rBV	470181	867422	100.00%	11.337%
18	9.414	2499	2511	2542	rBV	413144	686736	79.17%	8.975%
19	10.754	2912	2928	2948	rBV	171269	277419	31.98%	3.626%
20	11.809	3243	3256	3272	rBV	321342	507051	58.45%	6.627%
21	12.192	3359	3375	3398	rBV	305051	511820	59.00%	6.689%




Sum of corrected areas: 7651301

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
Data File : VU052128.D
Acq On : 24 Nov 2022 09:46
Operator : JC/MD
Sample : N5760-06DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COL21DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

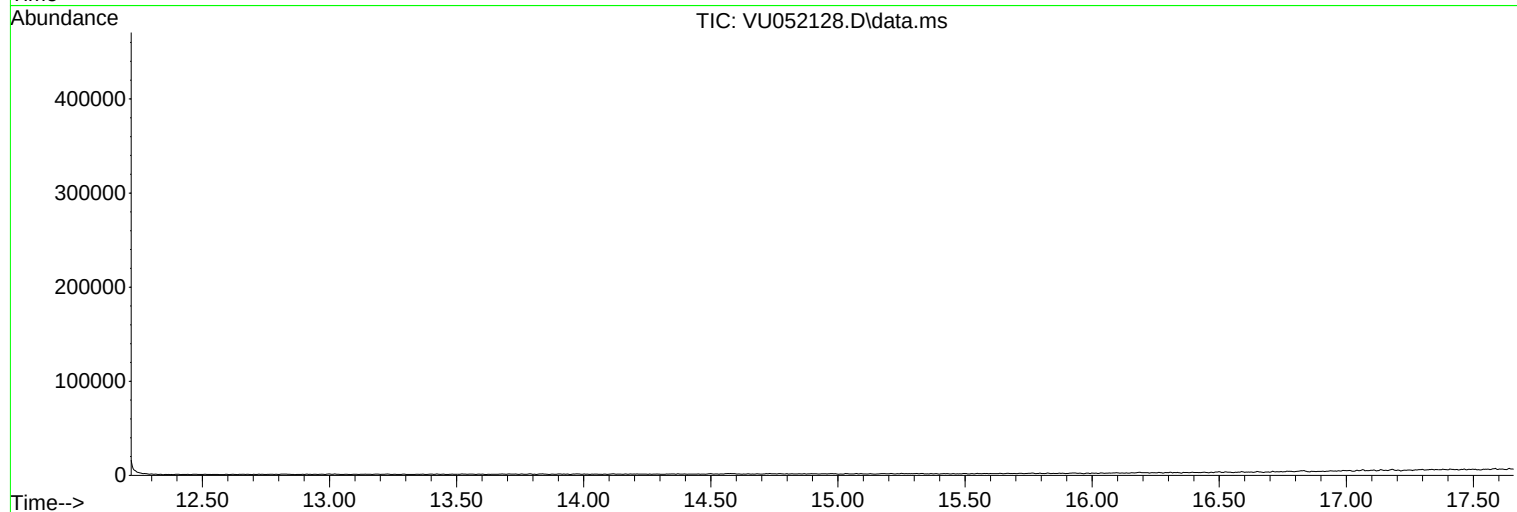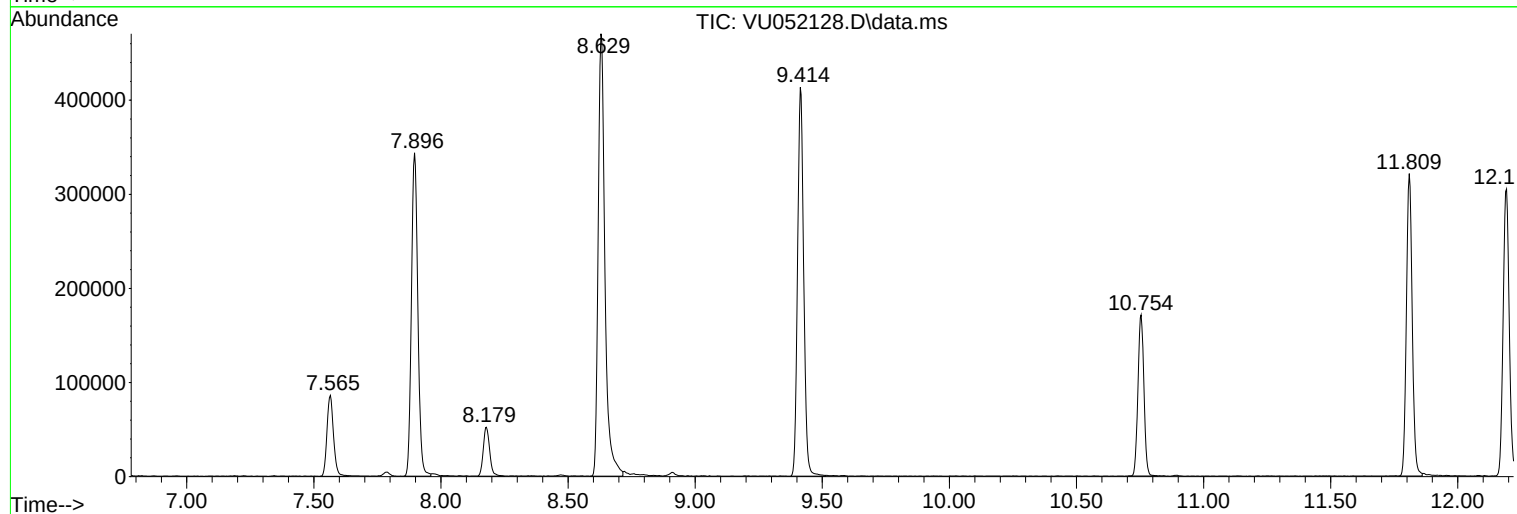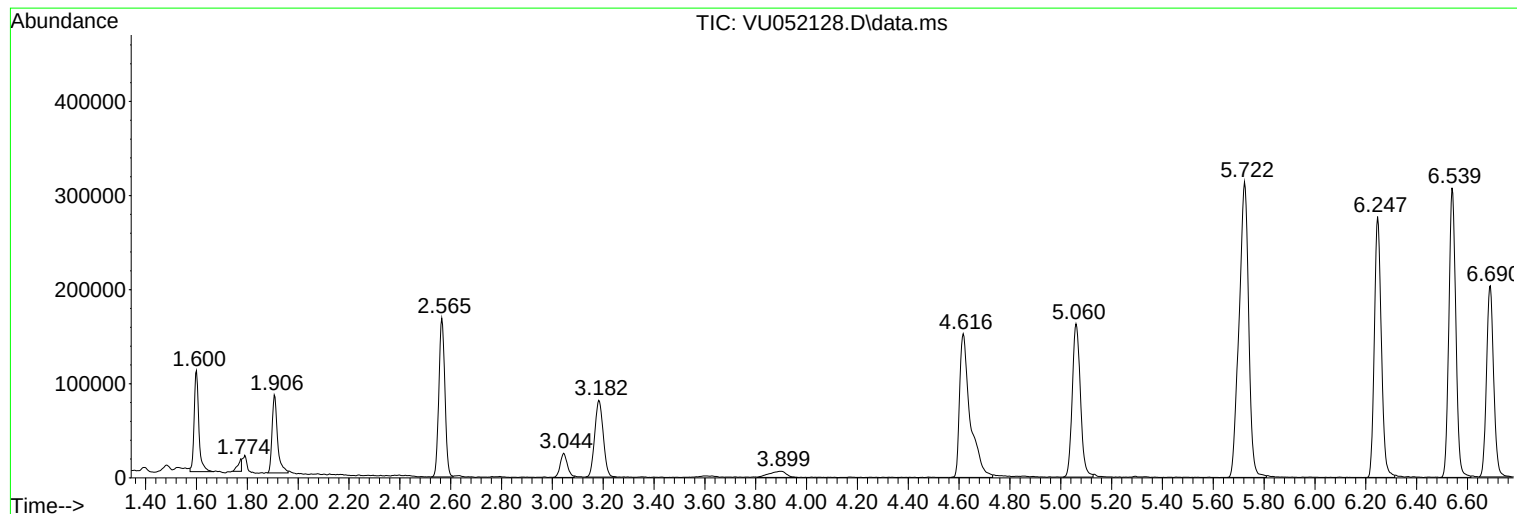

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
Data File : VU052128.D
Acq On : 24 Nov 2022 09:46
Operator : JC/MD
Sample : N5760-06DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L21DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
Data File : VU052128.D
Acq On : 24 Nov 2022 09:46
Operator : JC/MD
Sample : N5760-06DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L21DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc