

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
 Data File : VU052130.D
 Acq On : 24 Nov 2022 10:36
 Operator : JC/MD
 Sample : N5760-05DL 200X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COL20DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU052130.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	96	rVB	96736	114813	13.84%	1.564%
2	1.774	125	135	148	rVB6	9494	19000	2.29%	0.259%
3	1.912	169	178	194	rBV	82372	115953	13.98%	1.579%
4	2.565	369	381	396	rBV	152515	249288	30.05%	3.396%
5	3.044	518	530	548	rBV2	31779	62142	7.49%	0.846%
6	3.183	557	573	598	rVB2	66776	154301	18.60%	2.102%
7	4.617	1002	1019	1058	rBV2	160384	459998	55.45%	6.266%
8	5.060	1141	1157	1179	rBV	156251	346502	41.77%	4.720%
9	5.723	1342	1363	1391	rBV3	301444	797079	96.07%	10.857%
10	6.247	1512	1526	1560	rBV	267647	513051	61.84%	6.988%
11	6.539	1603	1617	1649	rBV2	308826	582853	70.25%	7.939%
12	6.687	1649	1663	1691	rVB	199813	391256	47.16%	5.329%
13	7.565	1923	1936	1953	rBV	81026	147276	17.75%	2.006%
14	7.896	2023	2039	2058	rBV	328150	572221	68.97%	7.794%
15	8.176	2114	2126	2139	rBV	52012	86502	10.43%	1.178%
16	8.629	2255	2267	2303	rBV	439254	829645	100.00%	11.300%
17	8.909	2345	2354	2372	rVB2	5146	9759	1.18%	0.133%
18	9.414	2498	2511	2534	rBV	395461	665604	80.23%	9.066%
19	10.751	2915	2927	2945	rBV	162329	263066	31.71%	3.583%
20	11.809	3242	3256	3280	rBV	299794	486872	58.68%	6.632%
21	12.189	3358	3374	3392	rBV	286255	474499	57.19%	6.463%




Sum of corrected areas: 7341680

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
Data File : VU052130.D
Acq On : 24 Nov 2022 10:36
Operator : JC/MD
Sample : N5760-05DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COL20DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

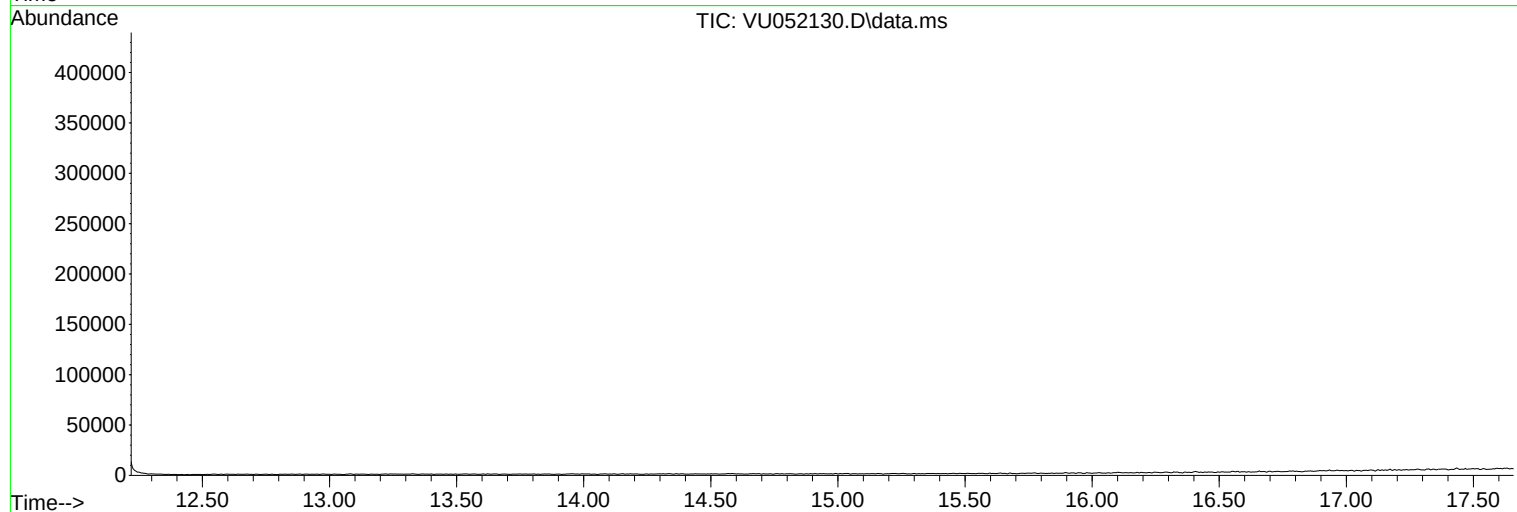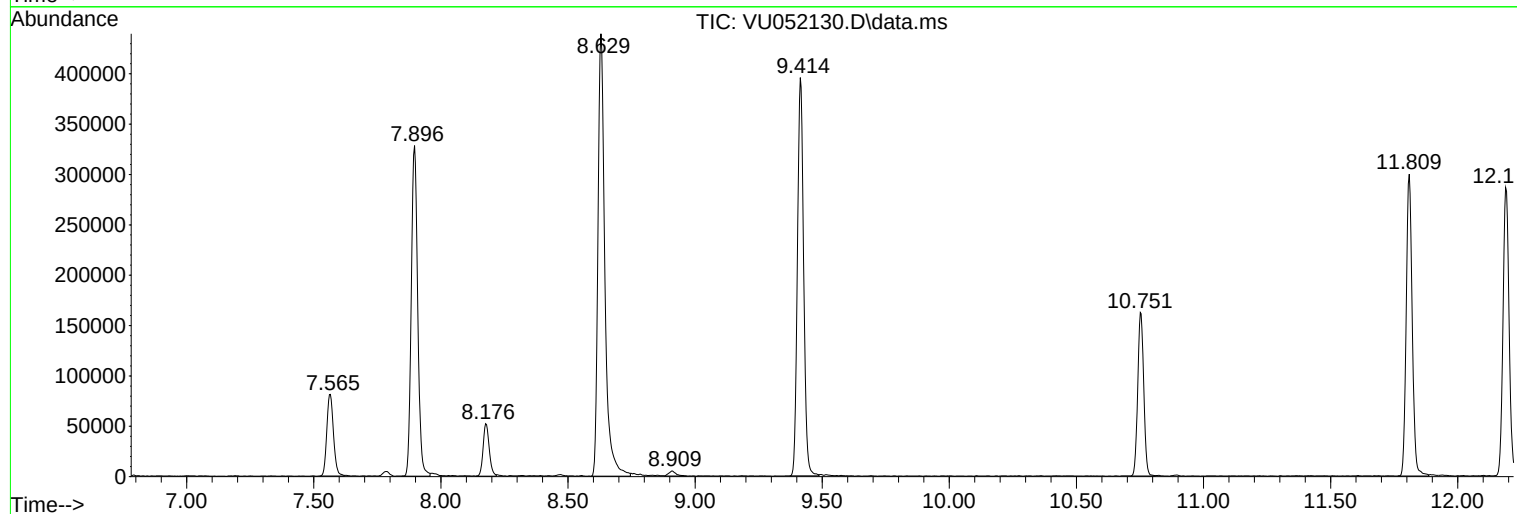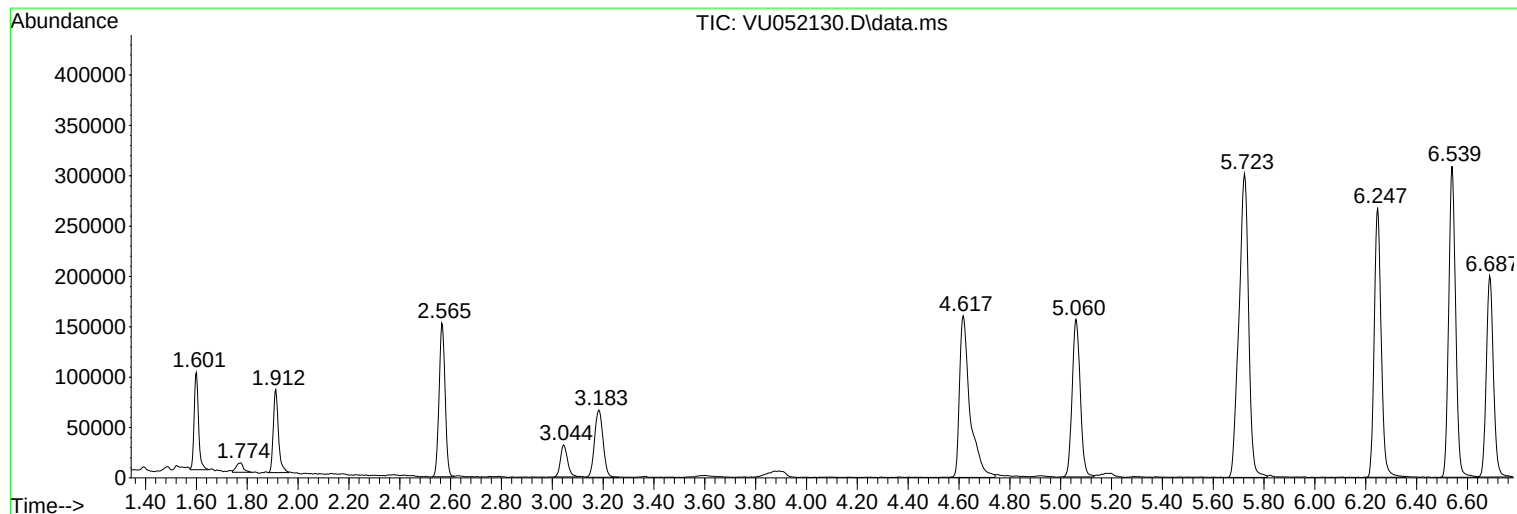

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
Data File : VU052130.D
Acq On : 24 Nov 2022 10:36
Operator : JC/MD
Sample : N5760-05DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L20DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
Data File : VU052130.D
Acq On : 24 Nov 2022 10:36
Operator : JC/MD
Sample : N5760-05DL 200X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L20DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc