
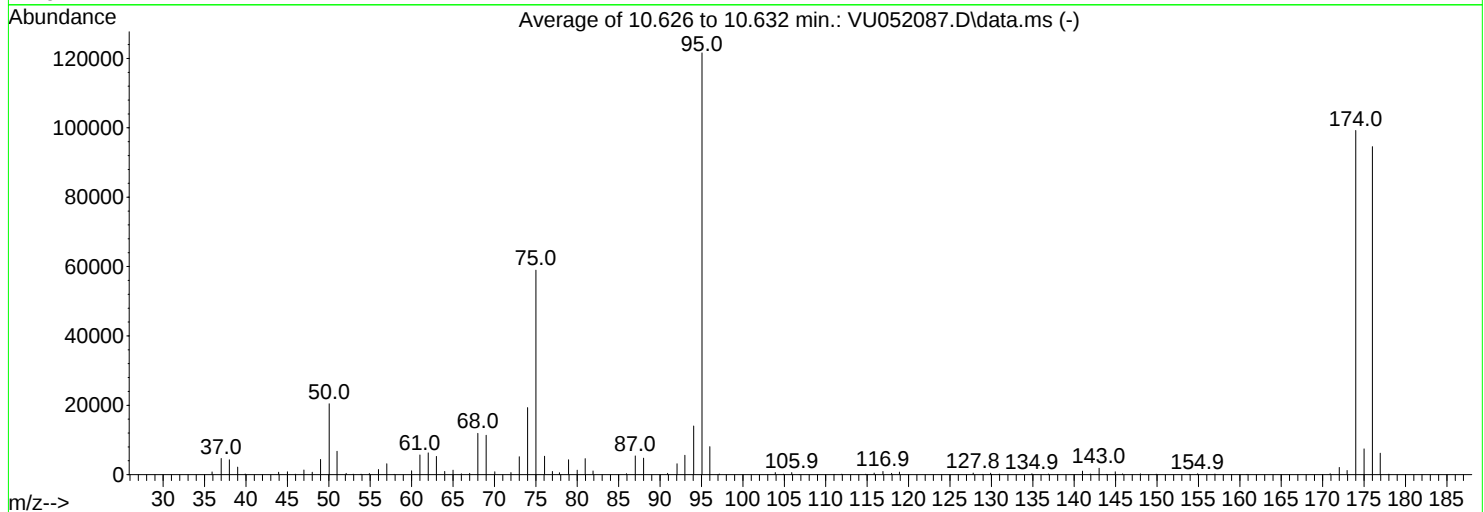


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112322\
 Data File : VU052087.D
 Acq On : 23 Nov 2022 13:04
 Operator : JC/MD
 Sample : BFB172
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB172

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111822WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Nov 24 05:20:45 2022

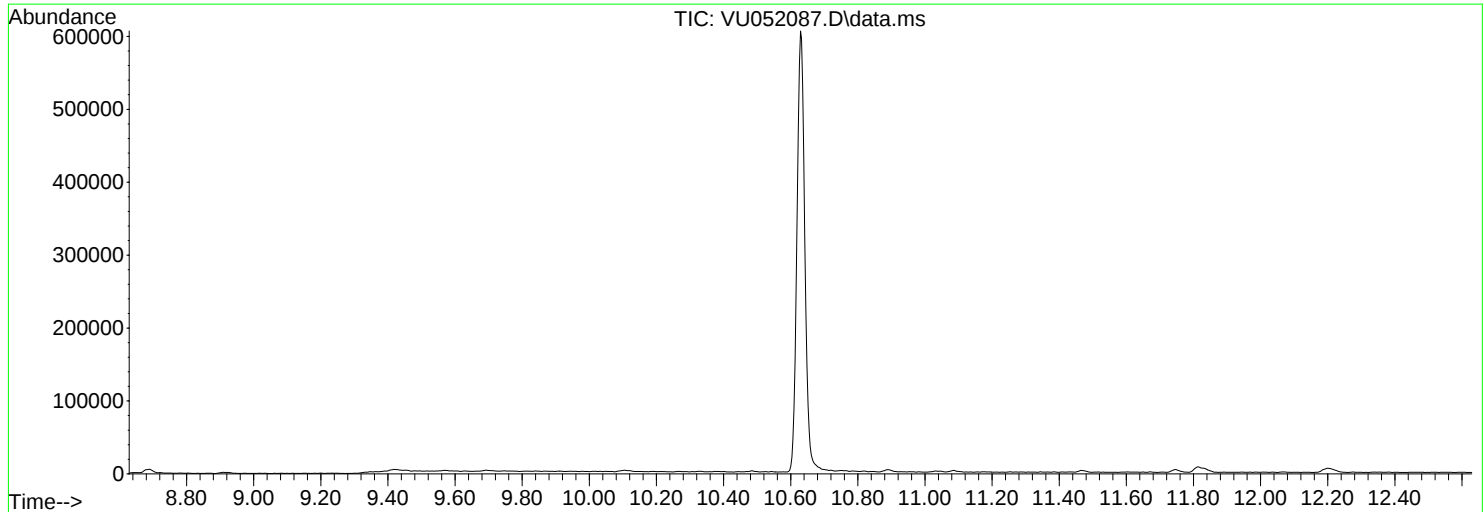

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.8	20445	PASS
75	95	30	80	48.5	58965	PASS
95	95	100	100	100.0	121621	PASS
96	95	5	9	6.6	8081	PASS
173	174	0.00	2	1.2	1201	PASS
174	95	50	120	81.6	99227	PASS
175	174	5	9	7.5	7455	PASS
176	174	95	101	95.3	94565	PASS
177	176	5	9	6.5	6171	PASS

m/z	Abundance
36.00	2227.0
37.00	4695.0
38.00	4897.0
39.00	2247.0
39.90	338.0
44.00	1116.0
45.00	867.0
45.90	153.0
47.00	1470.0
48.00	667.0
49.00	4425.0
50.00	20536.0
51.00	6867.0
52.10	362.0
53.00	154.0
53.90	133.0
54.90	353.0
56.00	1594.0
57.00	3095.0
60.00	1214.0
61.00	5607.0
62.00	6110.0
63.00	5384.0
64.00	874.0
65.00	1208.0
66.00	266.0
67.00	377.0
68.00	11824.0
69.00	11175.0
70.10	752.0
72.00	641.0
73.00	5280.0
74.00	19496.0
75.00	58648.0
76.10	5189.0
77.00	877.0
77.80	416.0
79.00	4206.0
80.00	1284.0
81.00	4769.0
81.90	1039.0
85.90	246.0
87.00	5445.0
88.00	4703.0
90.90	412.0
92.10	3043.0
93.00	5398.0
94.10	13839.0
95.10	122256.0
96.00	8158.0
97.10	203.0
103.90	666.0
104.90	120.0
105.90	652.0
106.80	110.0
111.00	156.0
112.00	100.0
114.90	167.0
115.90	517.0
116.90	866.0
117.90	354.0
118.90	888.0
127.80	481.0
128.90	147.0
129.90	477.0
131.00	244.0
134.90	264.0
136.90	159.0
141.00	1107.0
141.90	140.0
143.00	1821.0
143.90	190.0
144.90	841.0
145.80	228.0
148.00	227.0
149.90	132.0
154.90	361.0
157.00	207.0
159.00	117.0
160.90	122.0
170.90	238.0
172.00	2198.0
173.00	1204.0
174.00	102704.0
175.00	7717.0
176.00	97976.0
176.90	6189.0
178.00	141.0

Instrument :
MSVOA_U
ClientSampleId :
BFB172

m/z	Abundance
35.90	1570.0
38.00	486.0
39.90	177.0
43.90	466.0

Instrument :
MSVOA_U
ClientSampleId :
BFB172

m/z	Abundance
36.00	2427.0
37.00	4476.0
38.00	4575.0
39.00	2080.0
39.90	393.0
44.00	1163.0
45.00	784.0
46.00	171.0
47.00	1146.0
48.00	746.0
49.00	4222.0
50.10	19560.0
51.00	6371.0
52.10	355.0
52.90	147.0
53.90	118.0
54.90	282.0
56.00	1351.0
57.00	3092.0
57.90	153.0
60.00	964.0
61.00	5650.0
62.00	6255.0
63.00	4979.0
64.00	974.0
65.00	1360.0
66.00	203.0
67.00	307.0
68.00	11593.0
69.00	11230.0
70.00	876.0
72.00	582.0
73.00	4922.0
74.00	18480.0
75.00	57408.0
76.00	5164.0
77.00	896.0
77.90	661.0
78.90	4285.0
80.00	1279.0
80.90	4288.0
81.90	1080.0
86.00	285.0
87.00	5310.0
88.00	4733.0
90.90	350.0
92.00	3175.0
93.00	5643.0
94.00	13682.0
95.10	117112.0
96.00	7742.0
97.20	164.0
103.90	479.0
104.90	122.0
105.90	514.0
111.90	132.0
114.80	124.0
115.80	397.0
116.90	993.0
118.00	371.0
118.90	618.0
127.80	426.0
129.90	333.0
130.90	124.0
134.90	247.0
136.90	174.0
141.00	890.0
141.90	206.0
143.00	1780.0
145.00	797.0
145.90	183.0
148.00	210.0
149.90	113.0
153.90	168.0
154.90	220.0
157.00	172.0
170.90	305.0
172.00	1923.0
172.90	1151.0
174.00	93200.0
175.00	7008.0
176.00	87768.0
177.00	5936.0
178.00	167.0

Instrument :
MSVOA_U
ClientSampleId :
BFB172

m/z	Abundance
36.00	2425.0
37.00	4822.0
38.00	4837.0
39.00	2257.0
39.90	379.0
44.00	1217.0
45.00	836.0
46.00	157.0
47.00	1423.0
48.00	733.0
49.00	4480.0
50.00	21240.0
51.00	6913.0
52.10	407.0
53.00	175.0
53.90	137.0
54.90	344.0
56.00	1528.0
57.00	3288.0
57.90	131.0
60.00	1136.0
61.00	5825.0
62.00	6528.0
63.00	5363.0
64.00	994.0
65.00	1335.0
66.00	256.0
67.00	366.0
68.00	12346.0
69.00	11664.0
70.00	851.0
72.00	598.0
73.00	5366.0
74.00	20008.0
75.00	60840.0
76.00	5539.0
77.00	945.0
77.80	534.0
78.90	4433.0
80.00	1329.0
81.00	4777.0
81.90	1085.0
85.90	262.0
87.00	5388.0
88.00	4805.0
90.90	407.0
92.10	3212.0
93.00	5751.0
94.00	14542.0
95.00	125496.0
96.00	8343.0
97.10	190.0
103.90	596.0
104.90	120.0
105.90	592.0
111.00	147.0
111.90	133.0
114.90	151.0
115.80	522.0
116.90	957.0
117.90	389.0
118.90	748.0
127.80	520.0
128.90	125.0
129.90	433.0
131.00	186.0
134.90	301.0
136.90	178.0
141.00	1050.0
142.00	188.0
143.00	1898.0
143.90	151.0
144.90	830.0
145.90	247.0
148.00	232.0
149.90	117.0
153.90	117.0
154.90	291.0
157.00	198.0
160.80	102.0
170.90	293.0
172.00	2164.0
173.00	1249.0
174.00	101776.0
175.00	7639.0
176.00	97952.0
177.00	6387.0
178.00	169.0

Instrument :
MSVOA_U
ClientSampleId :
BFB172