


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU112420\
 Data File : VU041408.D
 Acq On : 24 Nov 2020 08:47
 Operator : SY/MD
 Sample : BFB18
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB18

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112320WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Nov 25 07:37:29 2020

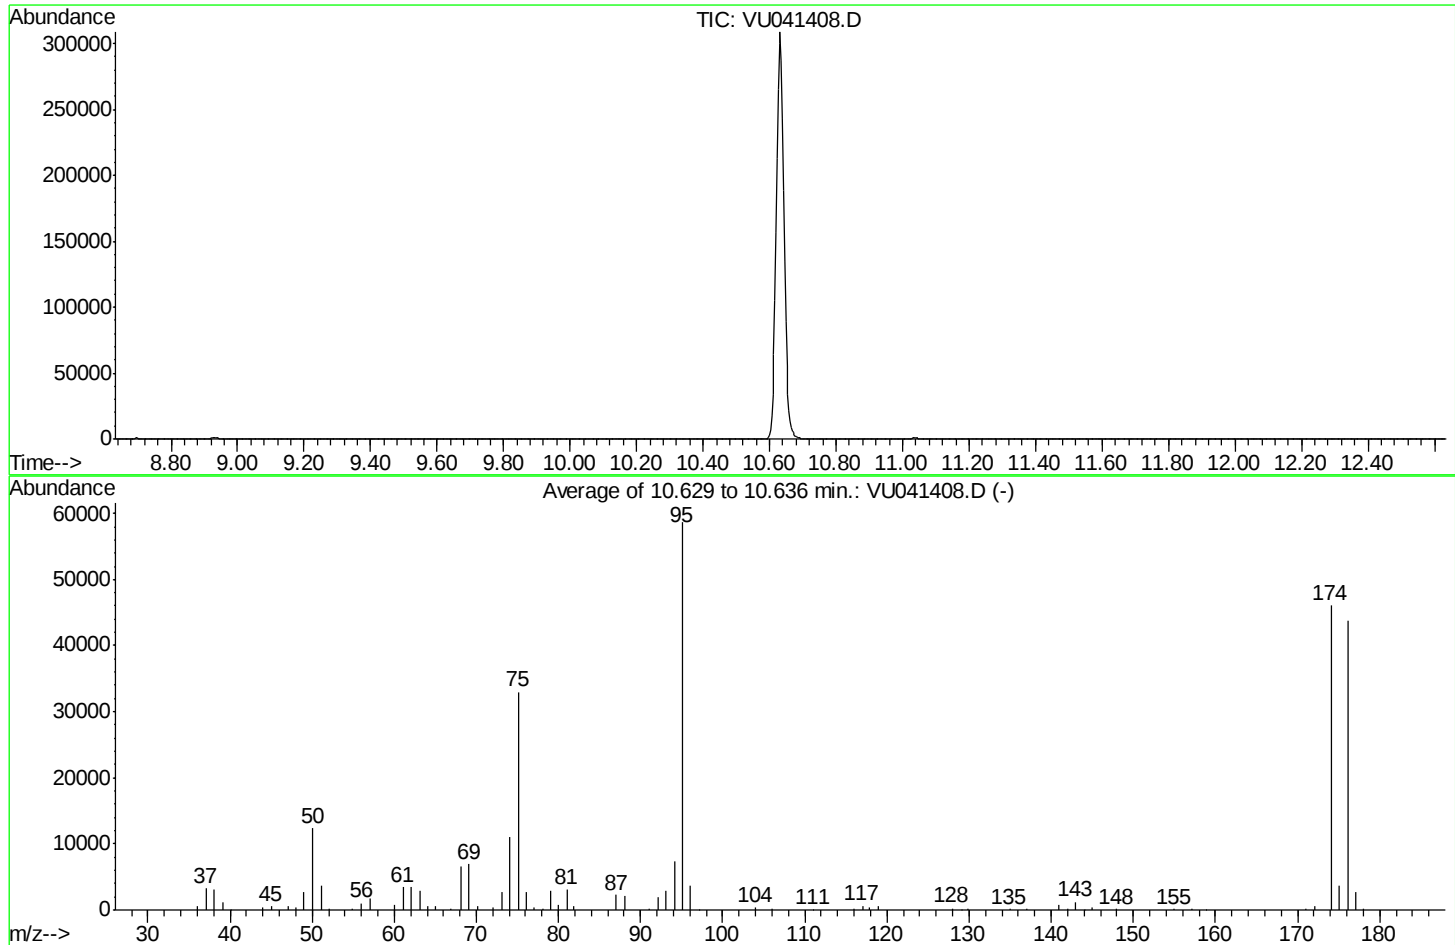

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	12314	PASS
75	95	30	80	56.3	33010	PASS
95	95	100	100	100.0	58648	PASS
96	95	5	9	6.4	3756	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.6	46082	PASS
175	174	5	9	7.8	3604	PASS
176	174	95	101	95.2	43850	PASS
177	176	5	9	6.4	2799	PASS

m/z	Abundance
36.10	665.0
37.10	3246.0
38.10	3221.0
39.10	1230.0
40.10	139.0
44.00	454.0
45.00	532.0
47.10	566.0
48.00	451.0
49.00	2702.0
50.10	12534.0
51.10	3848.0
52.00	156.0
55.00	215.0
56.00	952.0
57.10	1844.0
60.00	765.0
61.10	3486.0
62.10	3519.0
63.10	3058.0
64.00	629.0
65.00	568.0
66.90	187.0
68.10	6579.0
69.10	6926.0
70.10	518.0
72.00	311.0
73.10	2716.0
74.10	11126.0
75.10	33728.0
76.10	2961.0
77.00	330.0
78.10	202.0
79.00	3102.0
80.00	757.0
81.00	3020.0
81.90	671.0
87.10	2423.0
88.00	2132.0
90.90	245.0
92.10	1758.0
93.10	2884.0
94.10	7354.0
95.10	59144.0
96.10	3823.0
104.00	300.0
106.00	308.0
116.00	237.0
117.00	645.0
117.90	299.0
119.00	557.0
127.90	244.0
129.00	104.0
129.90	191.0
135.00	130.0
137.00	118.0
141.00	783.0
141.90	142.0
143.00	1252.0
144.00	114.0
145.00	429.0
148.00	154.0
155.00	176.0
157.10	118.0
158.90	104.0
171.00	186.0
172.10	621.0
174.10	45656.0
175.10	3564.0
176.10	43520.0
177.10	2824.0
178.00	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

m/z	Abundance
36.00	640.0
37.10	3378.0
38.10	3244.0
39.10	1225.0
40.00	119.0
44.00	464.0
45.00	537.0
47.10	603.0
48.00	445.0
49.00	2677.0
50.10	12735.0
51.10	3876.0
52.00	162.0
54.90	196.0
56.00	1023.0
57.10	1826.0
60.00	769.0
61.10	3529.0
62.00	3522.0
63.10	3086.0
64.00	607.0
65.10	556.0
66.90	168.0
68.10	6741.0
69.10	7226.0
70.10	560.0
72.00	321.0
73.10	2734.0
74.10	11364.0
75.10	34192.0
76.10	2828.0
77.00	387.0
78.00	245.0
79.00	3033.0
80.00	794.0
81.00	3231.0
81.90	703.0
87.10	2364.0
88.10	2292.0
91.00	220.0
92.10	1903.0
93.10	3054.0
94.10	7623.0
95.10	60472.0
96.10	3841.0
97.00	107.0
104.00	311.0
105.90	289.0
111.00	113.0
116.00	273.0
117.00	605.0
117.90	358.0
119.00	560.0
128.00	237.0
129.00	104.0
129.90	241.0
134.90	142.0
136.90	112.0
141.00	836.0
141.90	137.0
143.00	1249.0
144.00	106.0
145.00	444.0
148.00	143.0
155.00	169.0
157.10	118.0
171.00	243.0
172.10	686.0
174.10	47712.0
175.10	3726.0
176.10	45256.0
177.10	2903.0
178.00	121.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

m/z	Abundance
36.00	616.0
37.10	3154.0
38.10	2981.0
39.10	1099.0
44.00	437.0
45.00	487.0
47.10	613.0
47.90	414.0
49.00	2533.0
50.10	11673.0
51.10	3444.0
52.10	125.0
54.90	188.0
56.00	991.0
57.00	1675.0
60.00	705.0
61.10	3272.0
62.10	3225.0
63.10	2774.0
64.00	578.0
65.10	571.0
67.00	145.0
68.10	6277.0
69.10	6608.0
70.10	532.0
72.00	316.0
73.10	2612.0
74.10	10696.0
75.10	31112.0
76.10	2534.0
77.00	411.0
78.00	254.0
79.00	2639.0
80.00	793.0
81.00	3026.0
81.90	657.0
87.00	2044.0
88.10	2055.0
91.10	189.0
92.10	1917.0
93.10	2769.0
94.10	7257.0
95.10	56328.0
96.10	3604.0
97.10	112.0
104.00	296.0
105.90	283.0
111.00	105.0
116.00	291.0
117.00	533.0
117.90	366.0
119.00	504.0
128.00	244.0
129.90	275.0
134.90	113.0
136.90	122.0
141.00	768.0
142.00	122.0
143.00	1101.0
145.00	403.0
148.00	122.0
155.00	151.0
157.10	109.0
171.00	242.0
172.10	666.0
174.10	44880.0
175.10	3522.0
176.10	42776.0
177.10	2671.0
178.00	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18

m/z	Abundance
44.00	129.0

Instrument :
MSVOA_U
ClientSampleId :
BFB18