

Quantitation Report (QT/LSC Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
 Data File : VU045992.D
 Acq On : 24 Nov 2021 14:15
 Operator : SY/MD
 Sample : M4722-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 Client Sampled :
 C0G00

Quant Time: Nov 26 00:20:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 26 00:17:51 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/26/2021
 Supervised By : Semsettin Yesilyurt 11/29/2021

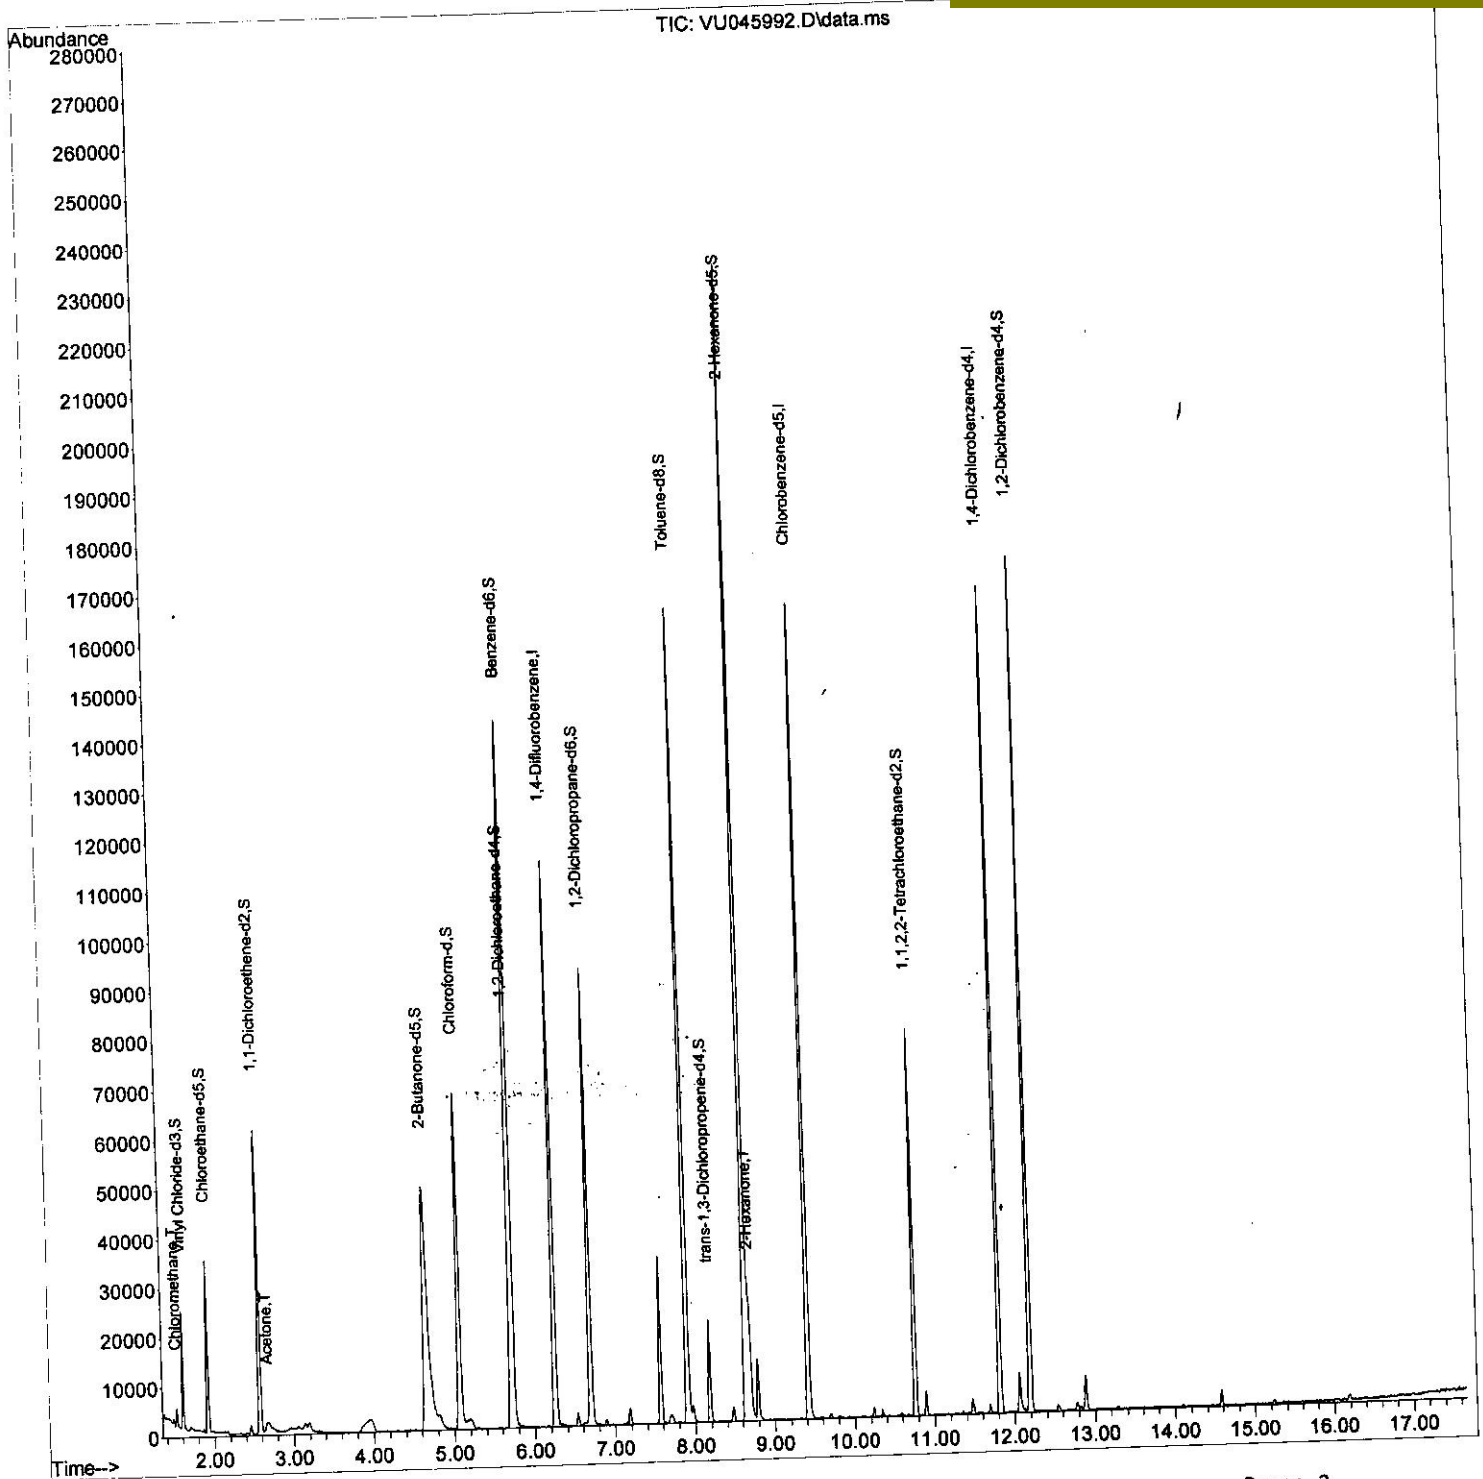

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
 Data File : VU045992.D
 Acq On : 24 Nov 2021 14:15
 Operator : SY/MD
 Sample : M4722-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampled :
 C0G00

Quant Time: Nov 26 00:20:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 26 00:17:51 2021
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/26/2021
 Supervised By :Semsettin Yesilyurt 11/29/2021

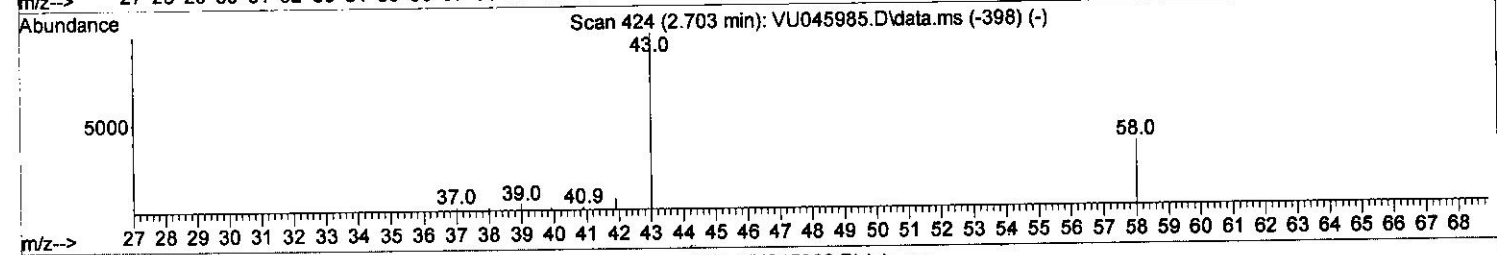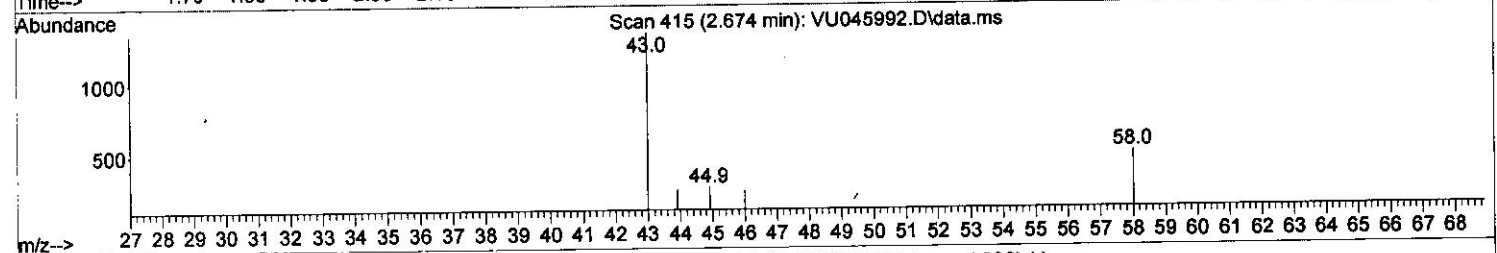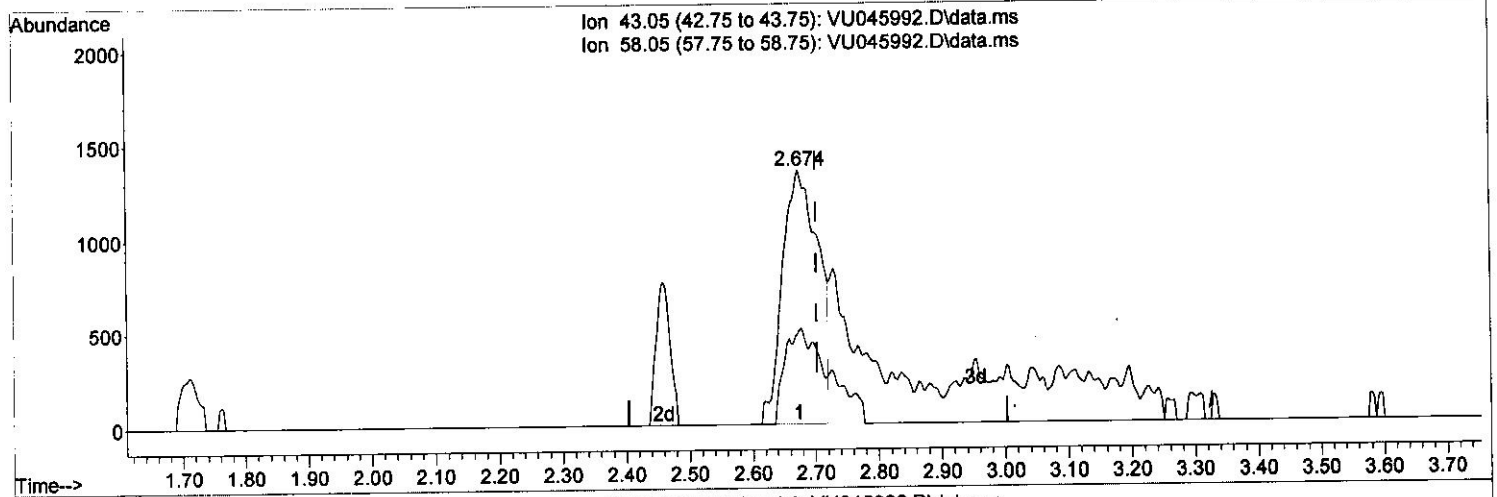

TIC: VU045992.D\data.ms

(13) Acetone (T)

2.674min (-0.029) 4.46 ug/L

response 5311

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	3.73
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
 Data File : VU045992.D
 Acq On : 24 Nov 2021 14:15
 Operator : SY/MD
 Sample : M4722-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampled :
 C0G00

Quant Time: Nov 26 00:20:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 26 00:17:51 2021
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/26/2021
 Supervised By :Semsettin Yesilyurt 11/29/2021

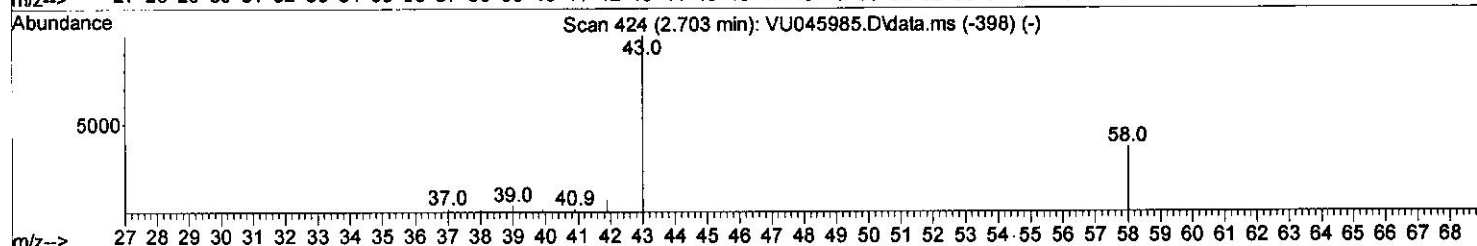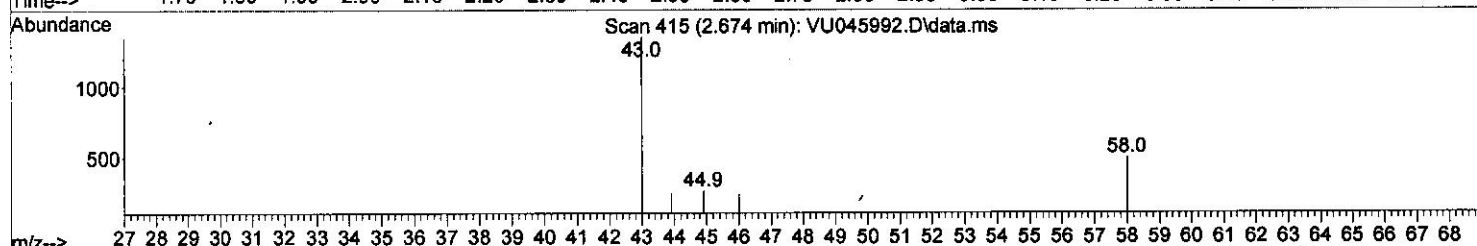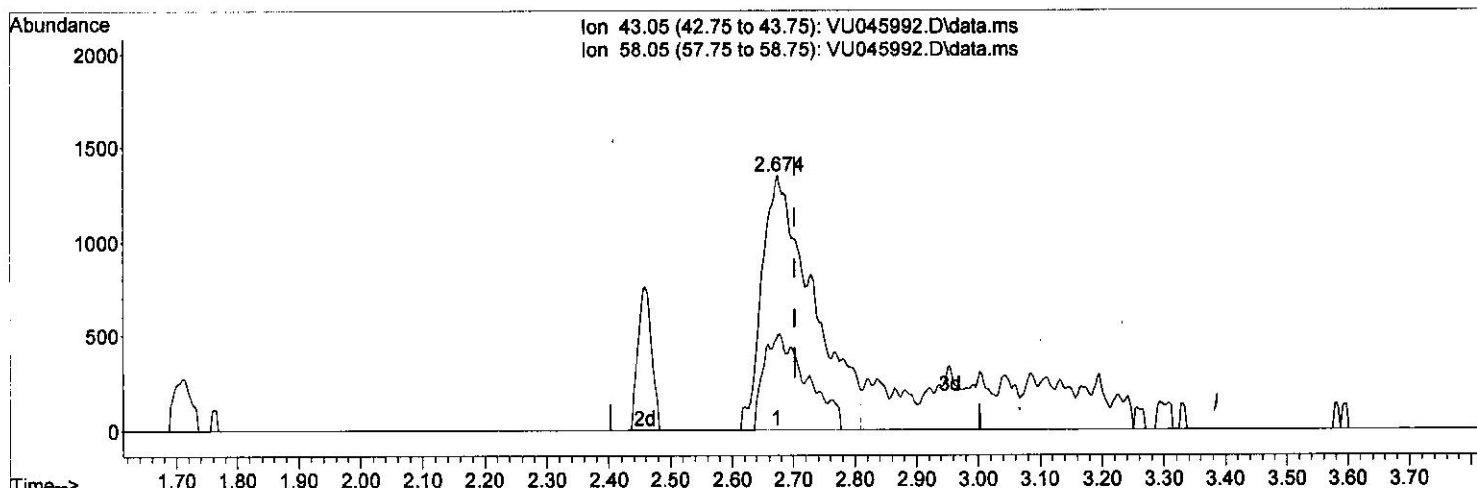

TIC: VU045992.D\data.ms

(13) Acetone (T)

2.674min (-0.029) 6.51 ug/L m } 29111

response 7754

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	2.55
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT/LSC Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
 Data File : VU045992.D
 Acq On : 24 Nov 2021 14:15
 Operator : SY/MD
 Sample : M4722-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 Client Sampled :
 C0G00

Quant Time: Nov 26 00:20:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 Qlast Update : Fri Nov 26 00:17:51 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/26/2021
 Supervised By : Semsettin Yesilyurt 11/29/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	95285	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	94090	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	44128	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	16378	2.169	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	43.400%	
7) Chloroethane-d5	1.919	69	25963	4.724	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	94.400%	
11) 1,1-Dichloroethene-d2	2.571	65	11274	3.561	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	71.200%	
20) 2-Butanone-d5	4.652	46	128109	63.323	ug/L	-0.01
Spiked Amount	50.000	Range 40 - 130	Recovery	=	126.640%	
24) Chloroform-d	5.070	84	63587	5.056	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	101.200%	
26) 1,2-Dichloroethane-d4	5.706	65	38955	5.279	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	105.600%	
32) Benzene-d6	5.732	84	134579	5.194	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	103.800%	
36) 1,2-Dichloropropane-d6	6.694	67	44498	5.449	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	109.000%	
41) Toluene-d8	7.899	98	113867	4.858	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	97.200%	
43) trans-1,3-Dichloroprop...	8.179	79	12498	3.770	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	75.400%	
46) 2-Hexanone-d5	8.636	63	88885	59.570	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	119.140%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	38619	5.598	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	112.000%	
66) 1,2-Dichlorobenzene-d4	12.195	152	44650	5.893	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	117.800%	
Target Compounds						
3) Chloromethane	1.520	50	2844	0.346	ug/L	98
13) Acetone	2.674	43	7754m	6.512	ug/L	
48) 2-Hexanone	8.693	43	13911	4.249	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

m D
 11/28/21