

Quantitation Report (QT/LSC Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
 Data File : VU045993.D
 Acq On : 24 Nov 2021 14:39
 Operator : SY/MD
 Sample : M4722-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 Client Sampled :
 C0G04

Quant Time: Nov 26 00:20:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 26 00:17:51 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/26/2021
 Supervised By : Semsettin Yesilyurt 11/29/2021

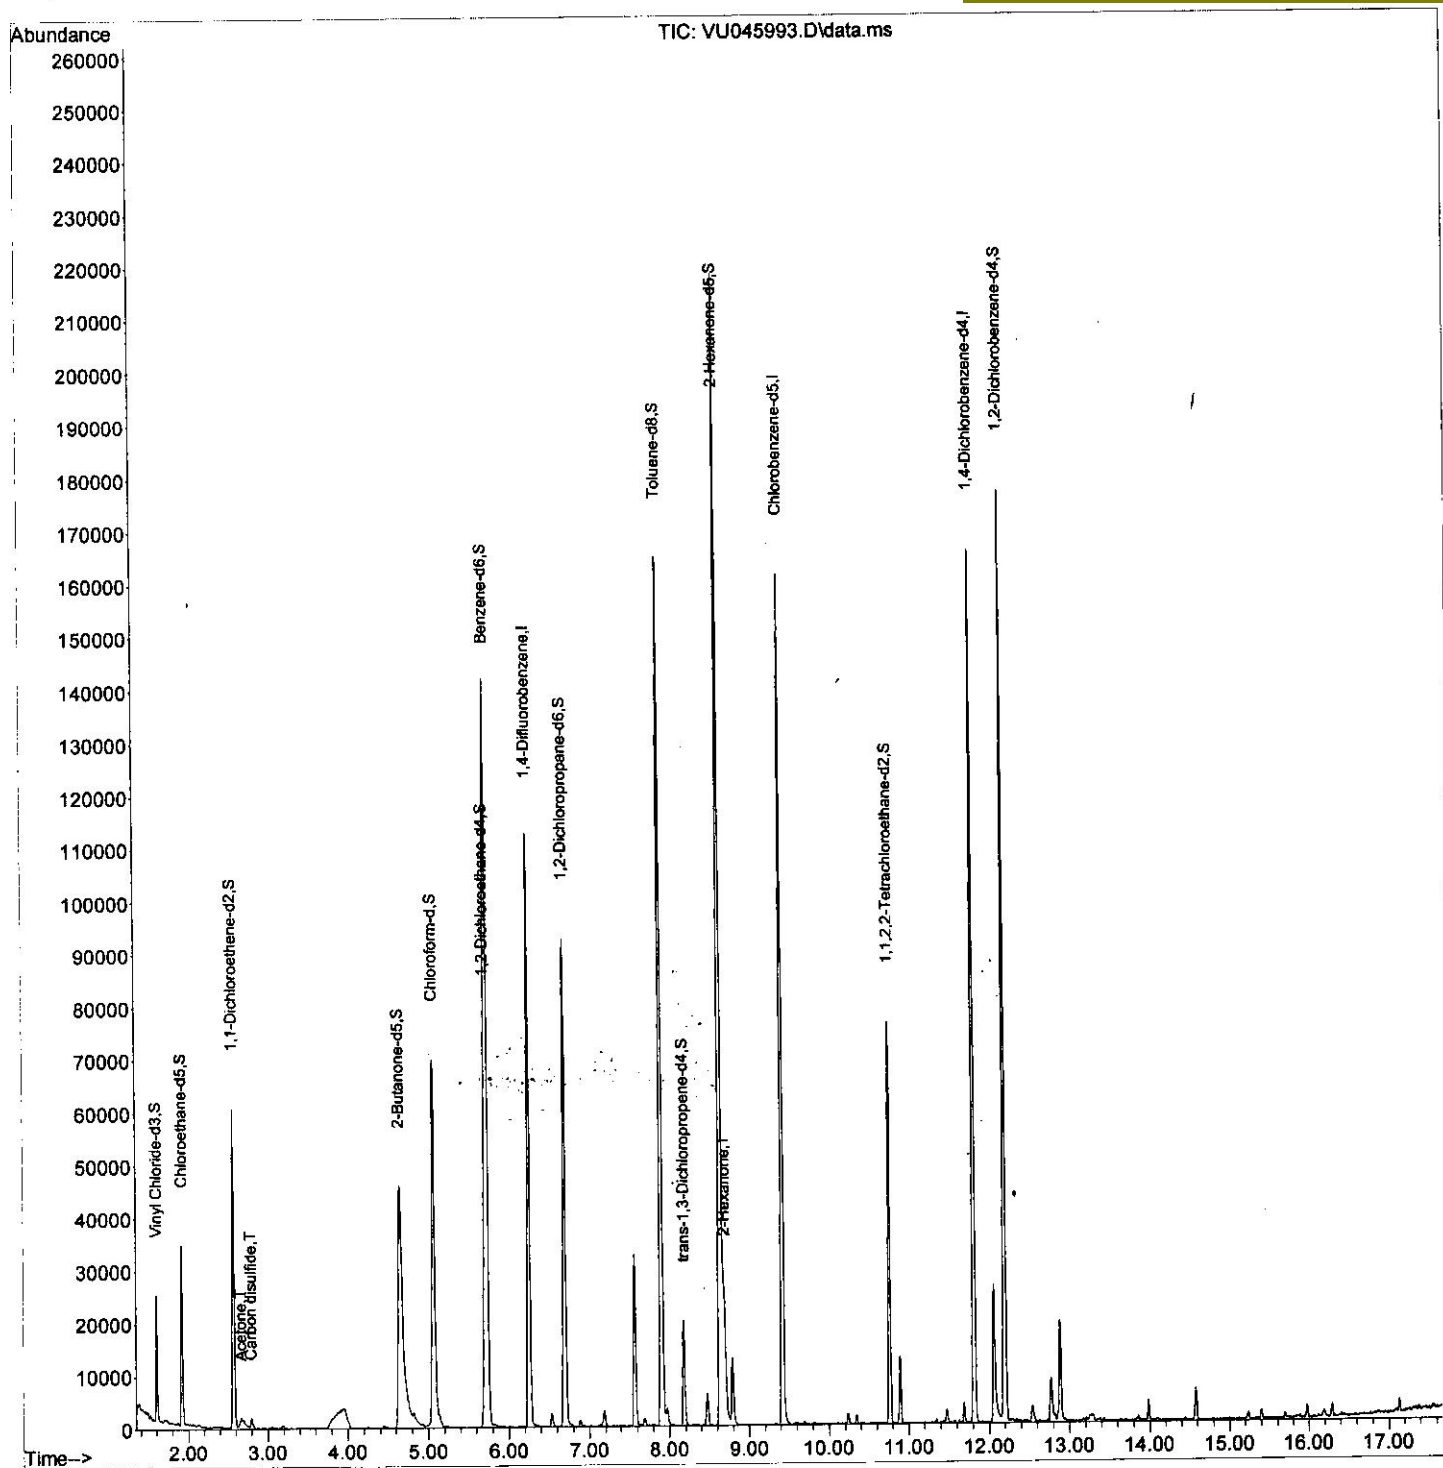

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
 Data File : VU045993.D
 Acq On : 24 Nov 2021 14:39
 Operator : SY/MD
 Sample : M4722-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampled :
 C0G04

Manual IntegrationsAPPROVED

Quant Time: Nov 26 00:20:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 26 00:17:51 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 11/26/2021
 Supervised By :Semsettin Yesilyurt 11/29/2021

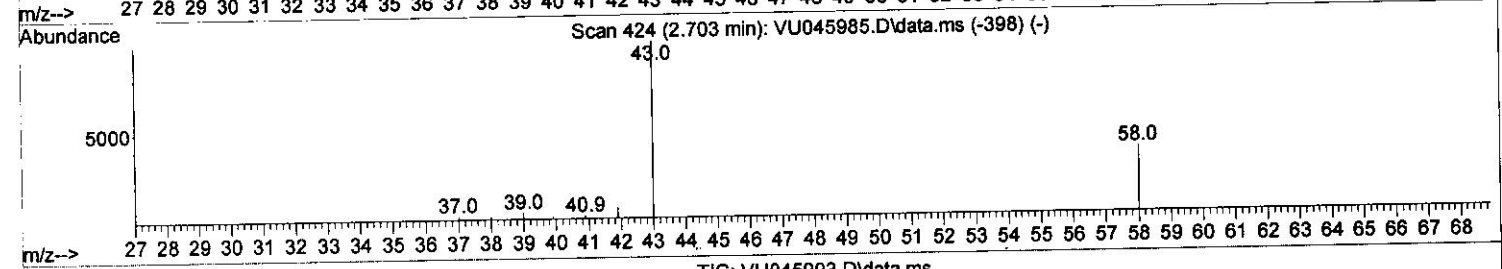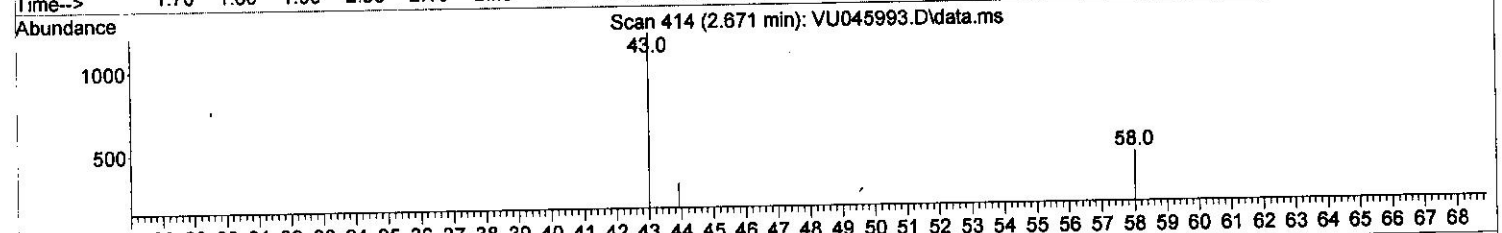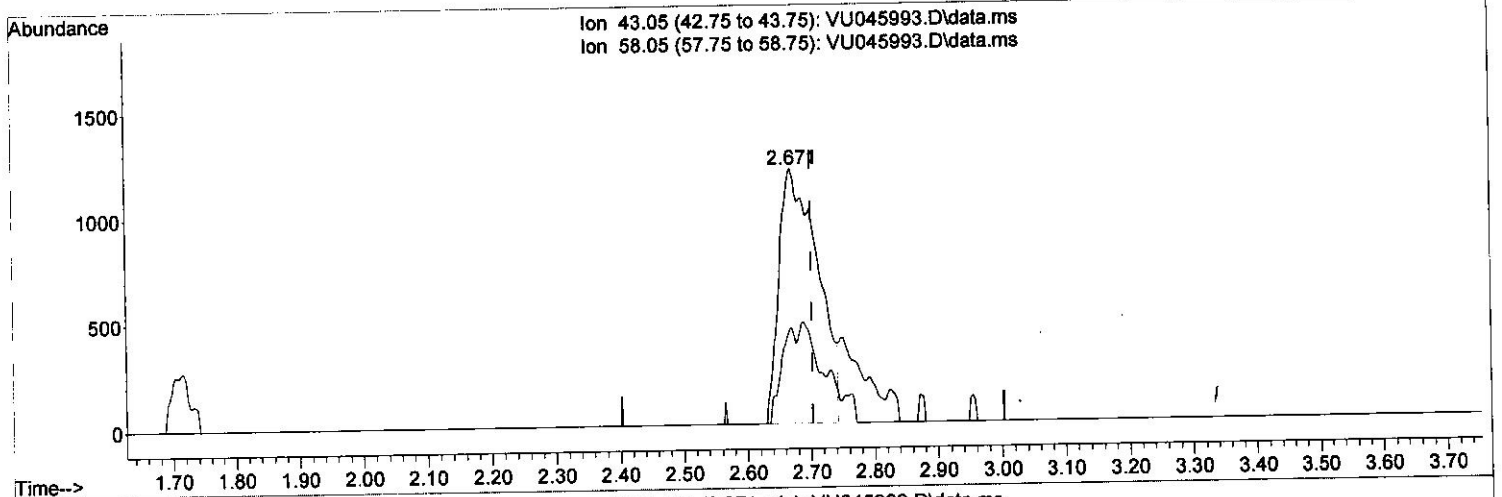

TIC: VU045993.D\data.ms

(13) Acetone (T)

2.671min (-0.032) 4.44 ug/L

response 5096

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	14.80
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
 Data File : VU045993.D
 Acq On : 24 Nov 2021 14:39
 Operator : SY/MD
 Sample : M4722-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 Client Sampled :
 C0G04

Quant Time: Nov 26 00:20:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 26 00:17:51 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/26/2021
 Supervised By : Semsettin Yesilyurt 11/29/2021

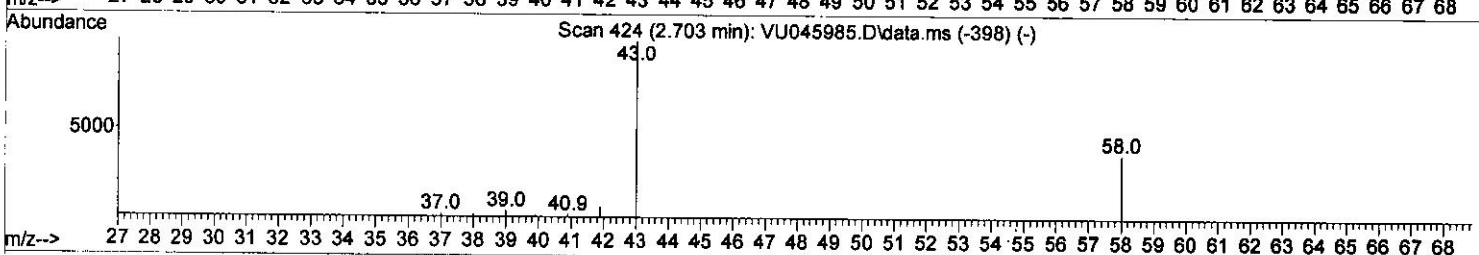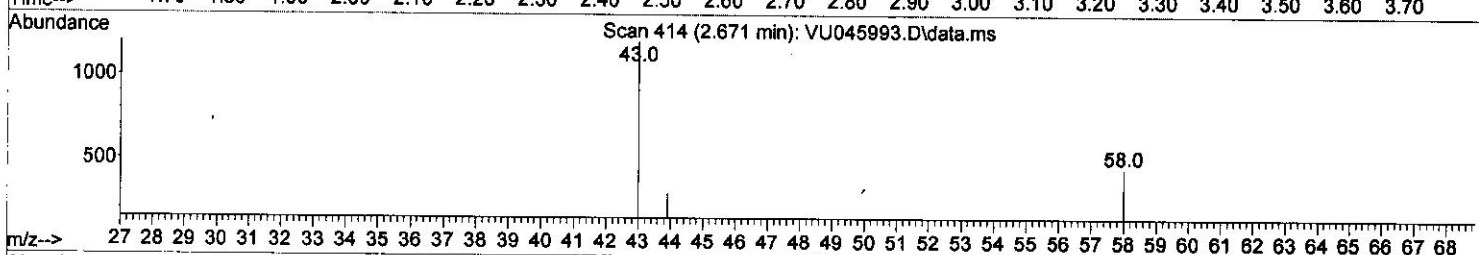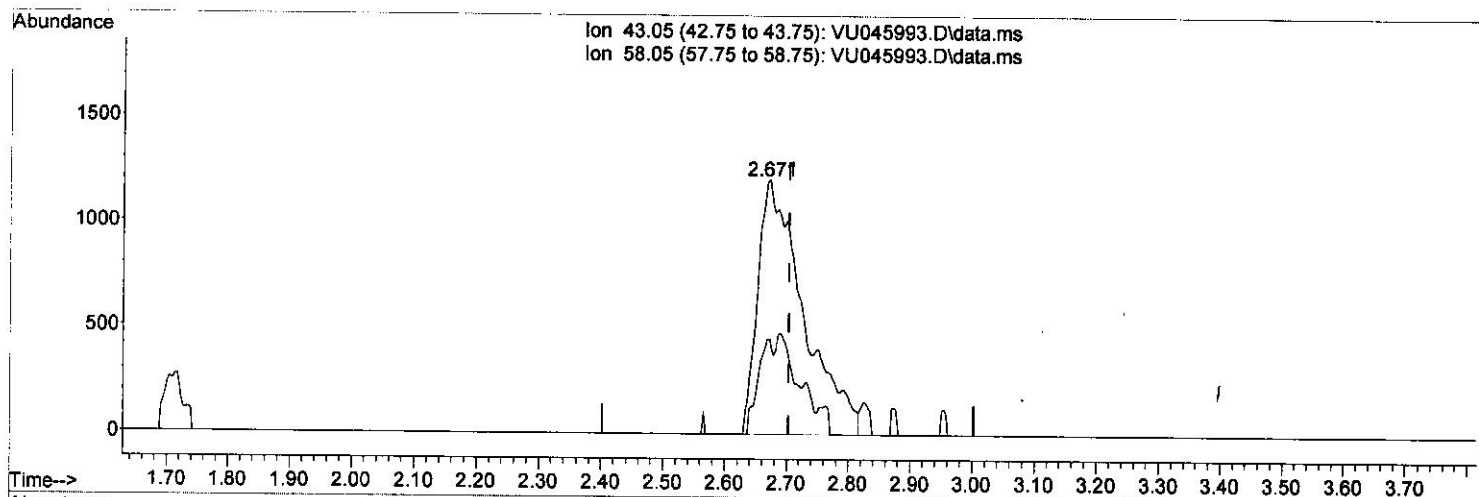

TIC: VU045993.D\data.ms

(13) Acetone (T)

2.671min (-0.032) 5.38 ug/L m

response 6173

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	12.21
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT/LSC Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
 Data File : VU045993.D
 Acq On : 24 Nov 2021 14:39
 Operator : SY/MD
 Sample : M4722-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 Client Sampled :
 C0G04

Quant Time: Nov 26 00:20:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 26 00:17:51 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/26/2021
 Supervised By : Semsettin Yesilyurt 11/29/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	91770	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	92121	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	44323	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	16488	2.268	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery =	45.400%		
7) Chloroethane-d5	1.919	69	24598	4.647	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery =	93.000%		
11) 1,1-Dichloroethene-d2	2.571	65	11569	3.794	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery =	75.800%		
20) 2-Butanone-d5	4.648	46	113877	58.444	ug/L	-0.02
Spiked Amount	50.000	Range 40 - 130	Recovery =	116.880%		
24) Chloroform-d	5.066	84	64190	5.299	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery =	106.000%		
26) 1,2-Dichloroethane-d4	5.706	65	38107	5.362	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery =	107.200%		
32) Benzene-d6	5.732	84	134585	5.305	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery =	106.200%		
36) 1,2-Dichloropropane-d6	6.693	67	45026	5.631	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery =	112.600%		
41) Toluene-d8	7.899	98	112230	4.890	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery =	97.800%		
43) trans-1,3-Dichloroprop...	8.182	79	12244	3.772	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery =	75.400%		
46) 2-Hexanone-d5	8.635	63	84708	57.984	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery =	115.960%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84	38041	5.632	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery =	112.600%		
66) 1,2-Dichlorobenzene-d4	12.195	152	46658	6.131	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery =	122.600%#		
Target Compounds						
13) Acetone	2.671	43	6173m	5.383	ug/L	Qvalue
14) Carbon disulfide	2.796	76	2496	0.139	ug/L	100
48) 2-Hexanone	8.690	43	13693	4.272	ug/L #	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

m
11/29/21