

Quantitation Report (QT/LSC Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
Data File : VU045996.D
Acq On : 24 Nov 2021 15:51
Operator : SY/MD
Sample : M4722-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampled :
C0G12

Quant Time: Nov 26 00:21:24 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 26 00:17:51 2021
Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/26/2021
Supervised By :Semsettin Yesilyurt 11/29/2021

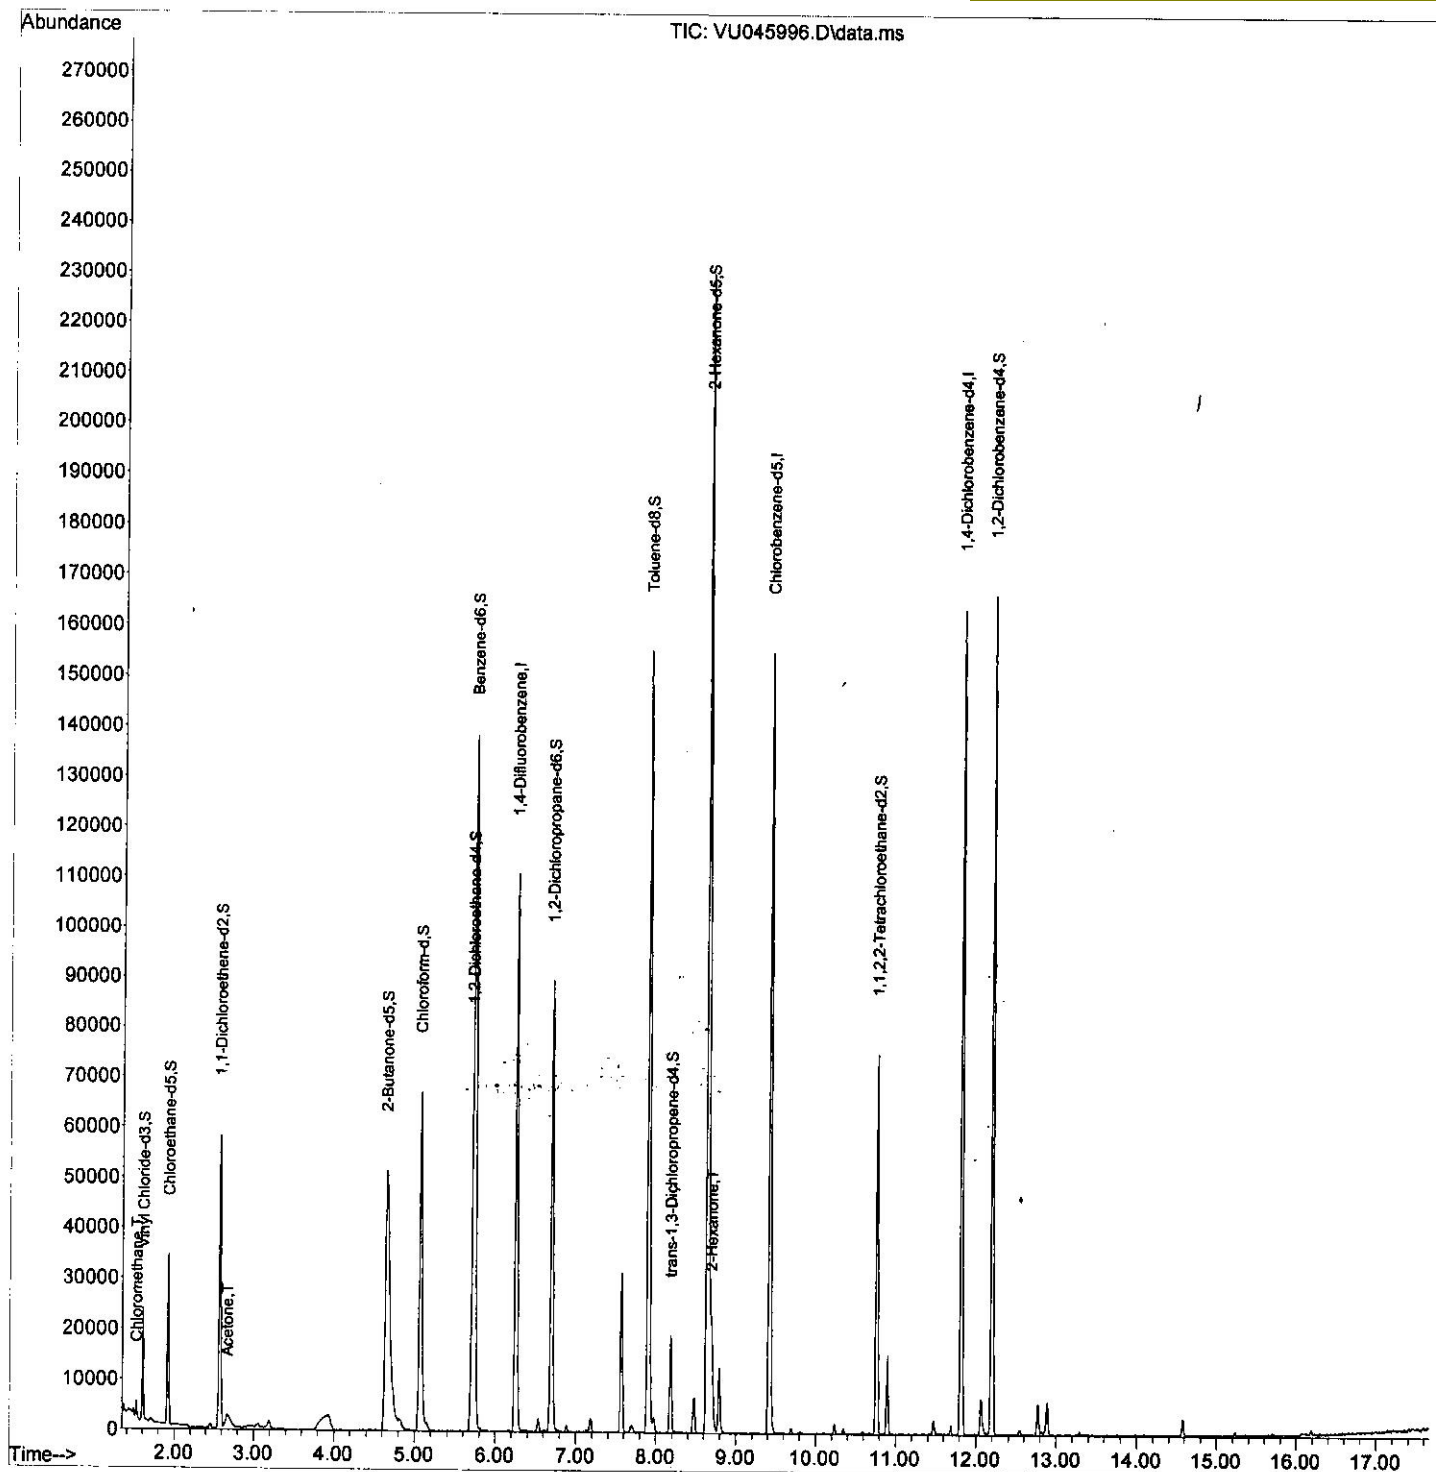

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
 Data File : VU045996.D
 Acq On : 24 Nov 2021 15:51
 Operator : SY/MD
 Sample : M4722-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampled :
 C0G12

Quant Time: Nov 26 00:21:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 26 00:17:51 2021
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 11/26/2021
 Supervised By :Semsettin Yesilyurt 11/29/2021

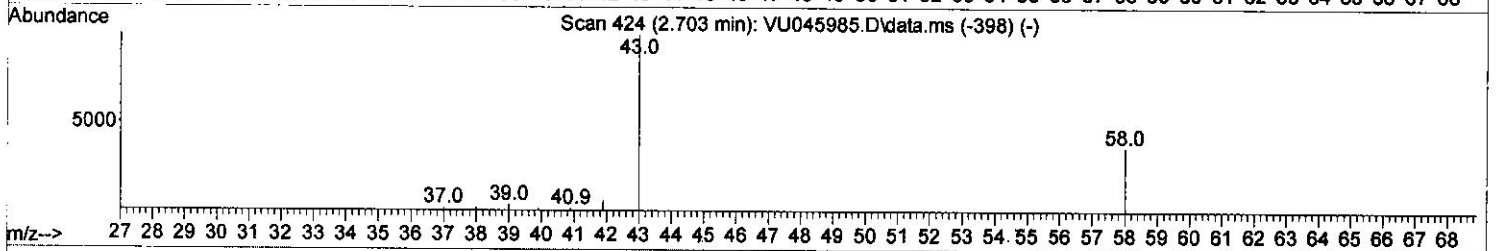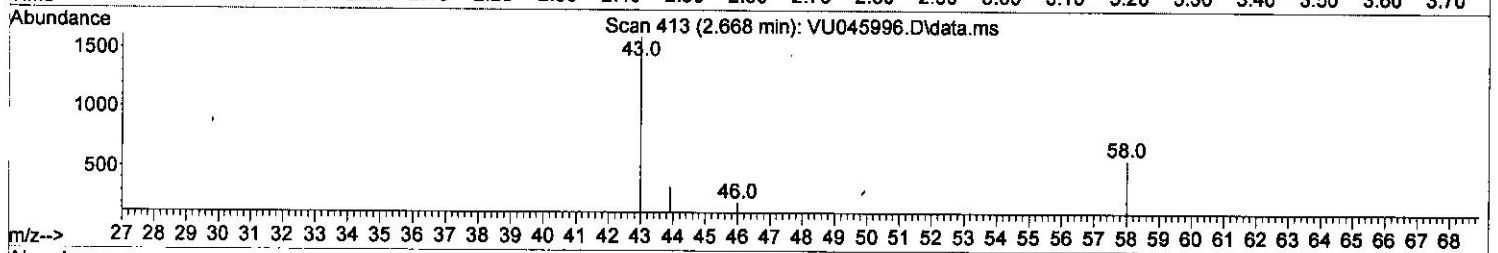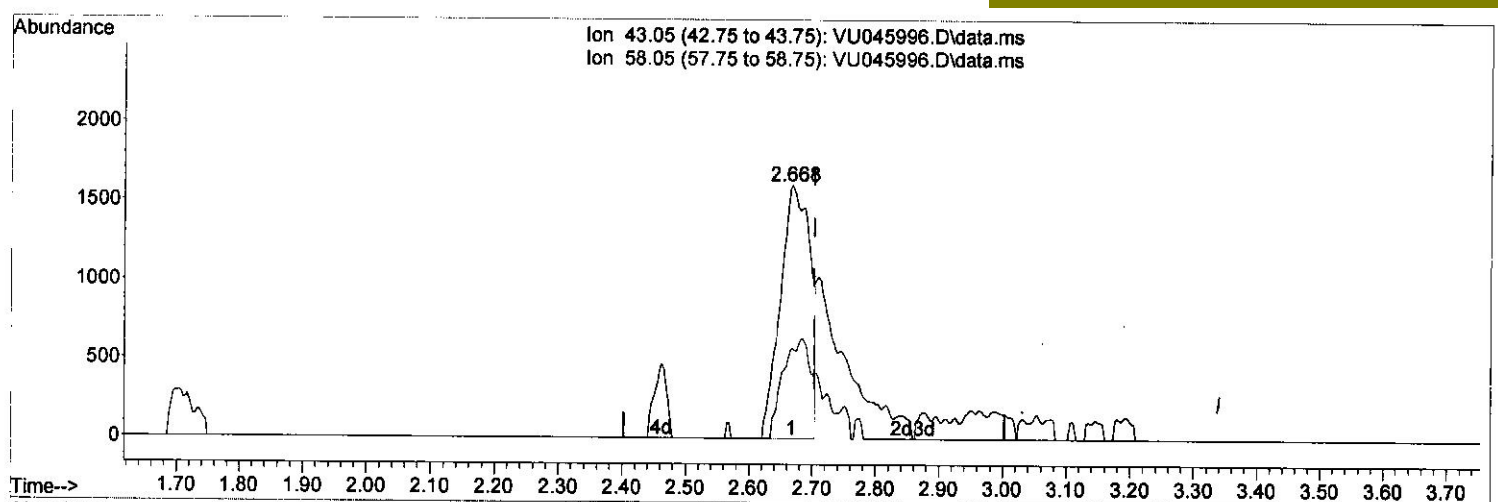

TIC: VU045996.D\data.ms

(13) Acetone (T)

2.668min (-0.035) 4.59 ug/L

response 5232

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	41.95
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
 Data File : VU045996.D
 Acq On : 24 Nov 2021 15:51
 Operator : SY/MD
 Sample : M4722-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 Client Sampled :
 C0G12

Quant Time: Nov 26 00:21:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 26 00:17:51 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/26/2021
 Supervised By : Semsettin Yesilyurt 11/29/2021

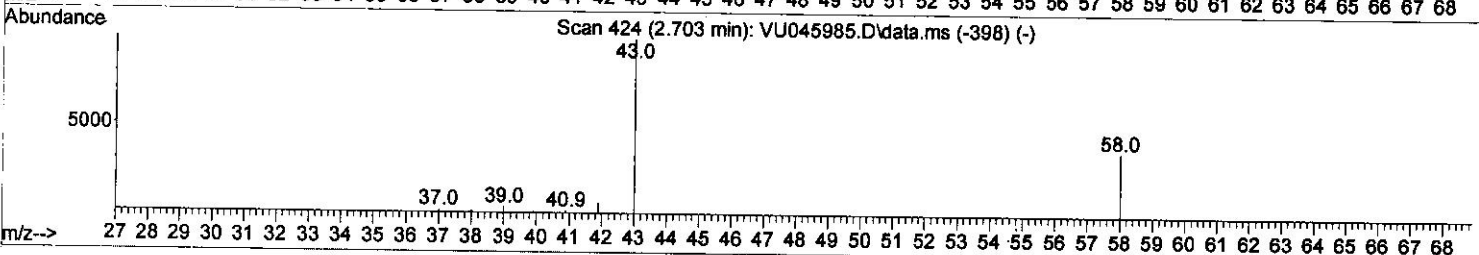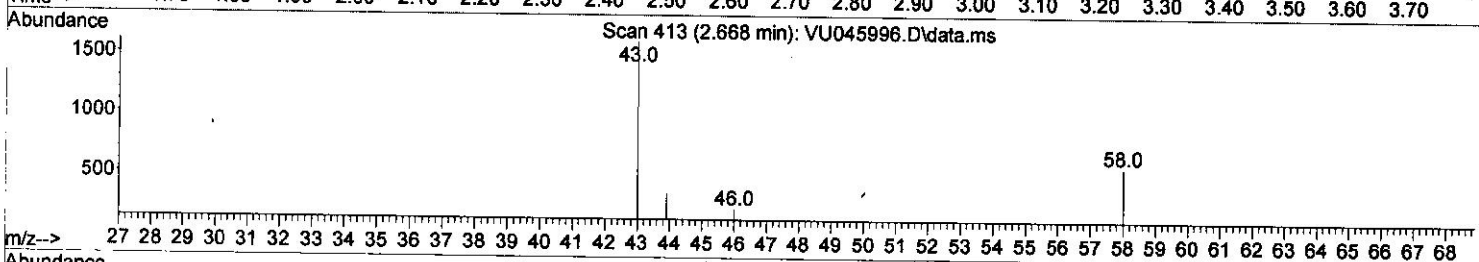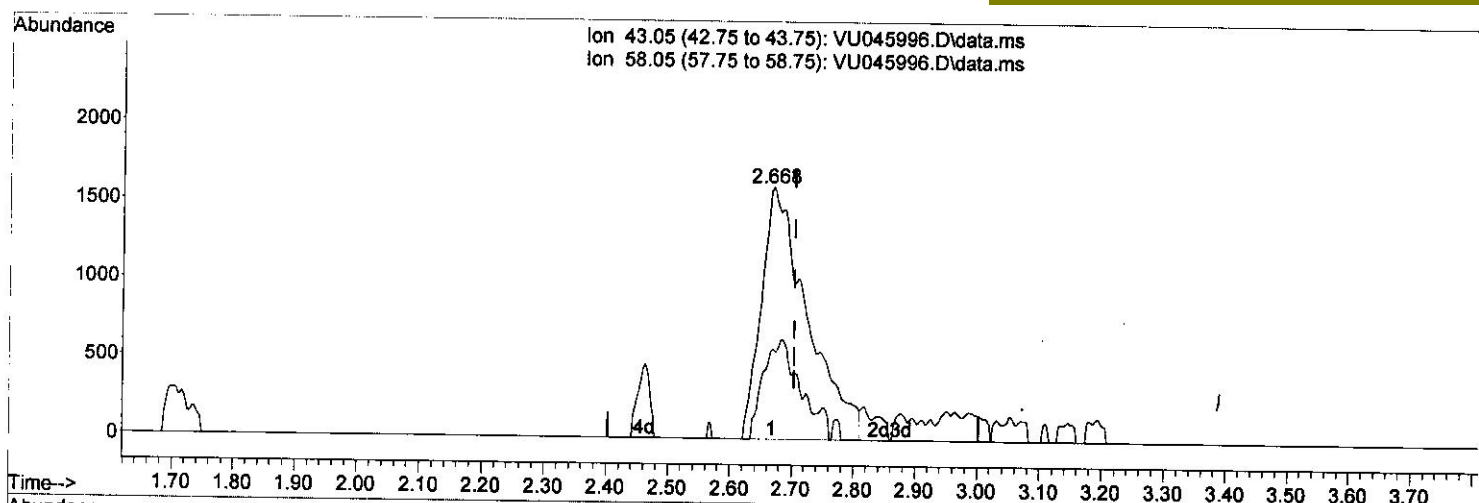

TIC: VU045996.D\data.ms

(13) Acetone (T)

2.668min (-0.035) 7.36 ug/L

response 8382

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	26.19
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT/LSC Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
 Data File : VU045996.D
 Acq On : 24 Nov 2021 15:51
 Operator : SY/MD
 Sample : M4722-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 Client Sampled :
 C0G12

Quant Time: Nov 26 00:21:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 26 00:17:51 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/26/2021
 Supervised By : Semsettin Yesilyurt 11/29/2021

Compound	R.T.	Q Ion	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	91116	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	89781	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	42668	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	15000	2.078	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	41.600%		
7) Chloroethane-d5	1.919	69	24440	4.651	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	93.000%		
11) 1,1-Dichloroethene-d2	2.572	65	11218	3.705	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	74.000%		
20) 2-Butanone-d5	4.649	46	125460	64.851	ug/L	-0.02
Spiked Amount 50.000	Range 40 - 130		Recovery =	129.700%		
24) Chloroform-d	5.067	84	63692	5.296	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	106.000%		
26) 1,2-Dichloroethane-d4	5.706	65	37177	5.268	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	105.400%		
32) Benzene-d6	5.732	84	131135	5.304	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	106.000%		
36) 1,2-Dichloropropane-d6	6.694	67	42479	5.451	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	109.000%		
41) Toluene-d8	7.899	98	109200	4.882	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	97.600%		
43) trans-1,3-Dichloroprop...	8.182	79	11902	3.763	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	75.200%		
46) 2-Hexanone-d5	8.636	63	85199	59.841	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	119.680%		
56) 1,1,2,2-Tetrachloroeth...	10.758	84	37080	5.633	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	112.600%		
66) 1,2-Dichlorobenzene-d4	12.195	152	43257	5.904	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	118.000%		
Target Compounds						
3) Chloromethane	1.520	50	2353	0.299	ug/L	92
13) Acetone	2.668	43	8382m	7.361	ug/L	
48) 2-Hexanone	8.693	43	12258	3.924	ug/L	97

Handwritten: mD 11/29/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed