

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
 Data File : VU045995.D
 Acq On : 24 Nov 2021 15:27
 Operator : SY/MD
 Sample : M4722-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0G05

Manual Integrations
 APPROVED

Reviewed By : John Carlone 11/26/2021
 Supervised By : Semsettin Yesilyurt 11/29/2021

Quant Time: Nov 26 00:21:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 26 00:17:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	91515	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	91449	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	43187	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	16070	2.216	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	44.400%
7) Chloroethane-d5	1.916	69	24333	4.610	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	92.200%
11) 1,1-Dichloroethene-d2	2.572	65	10770	3.542	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.800%
20) 2-Butanone-d5	4.646	46	125528	64.603	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	129.200%
24) Chloroform-d	5.067	84	61142	5.061	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.200%
26) 1,2-Dichloroethane-d4	5.707	65	37647	5.312	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.200%
32) Benzene-d6	5.732	84	128498	5.103	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.000%
36) 1,2-Dichloropropane-d6	6.694	67	42977	5.415	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.200%
41) Toluene-d8	7.899	98	106071	4.656	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.200%
43) trans-1,3-Dichloroprop...	8.182	79	11429	3.547	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	71.000%
46) 2-Hexanone-d5	8.636	63	87024	60.007	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	120.020%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	36877	5.500	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	110.000%
66) 1,2-Dichlorobenzene-d4	12.195	152	43848	5.913	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	118.200%
Target Compounds					Qvalue	
13) Acetone	2.668	43	5843m	5.109	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
Data File : VU045995.D
Acq On : 24 Nov 2021 15:27
Operator : SY/MD
Sample : M4722-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
C0G05

Quant Time: Nov 26 00:21:12 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 26 00:17:51 2021
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :John Carlone 11/26/2021
Supervised By :Semsettin Yesilyurt 11/29/2021

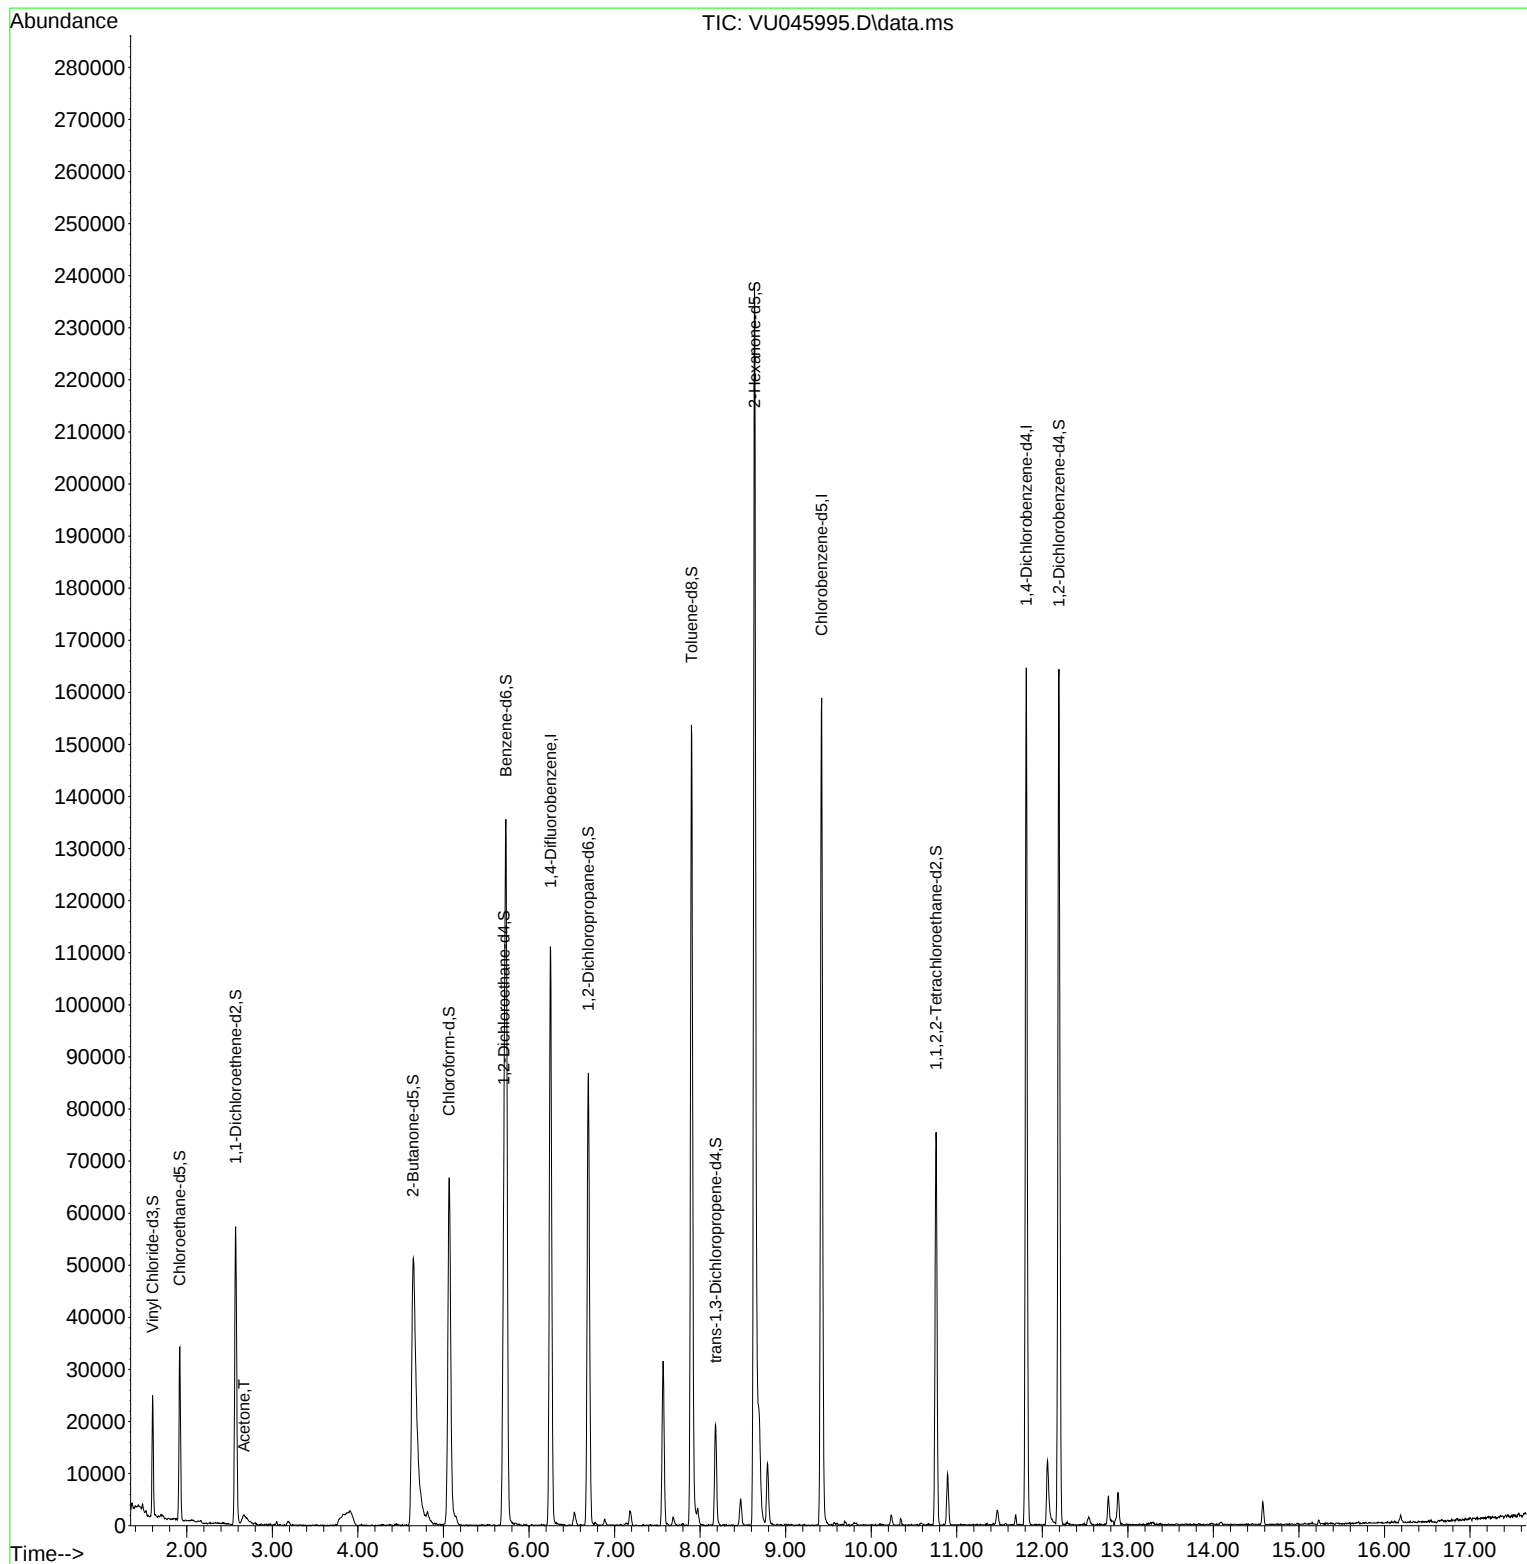

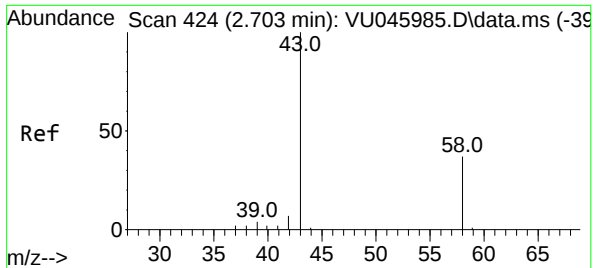

#13
 Acetone
 Concen: 5.109 ug/L m
 RT: 2.668 min Scan# 41
 Delta R.T. -0.035 min
 Lab File: VU045995.D
 Acq: 24 Nov 2021 15:27

Instrument :
 MSVOA_U
 ClientSampleId :
 C0G05

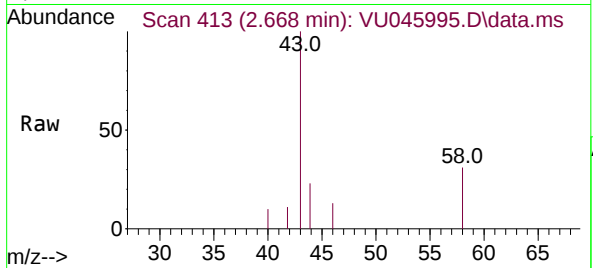

Tgt Ion: 43 Resp: 584
 Ion Ratio Lower Upper
 43 100
 58 16.5 0.0 71.6

Manual Integrations
 APPROVED

Reviewed By :John Carlone 11/26/2021
 Supervised By :Semsettin Yesilyurt 11/29/2021

