

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
 Data File : VU046002.D
 Acq On : 24 Nov 2021 18:14
 Operator : SY/MD
 Sample : M4779-11
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Nov 26 00:22:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 26 00:17:51 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	87799	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	87414	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	39550	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	30933	4.447	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.000%
7) Chloroethane-d5	1.919	69	25788	5.093	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.800%
11) 1,1-Dichloroethene-d2	2.571	65	12992	4.453	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	89.000%
20) 2-Butanone-d5	4.652	46	121049	64.935	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	129.860%
24) Chloroform-d	5.066	84	56218	4.851	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.000%
26) 1,2-Dichloroethane-d4	5.706	65	37277	5.482	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	109.600%
32) Benzene-d6	5.732	84	120684	5.013	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.200%
36) 1,2-Dichloropropane-d6	6.693	67	38902	5.128	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	102.600%
41) Toluene-d8	7.899	98	99660	4.576	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.600%
43) trans-1,3-Dichloroprop...	8.182	79	15839	5.143	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	102.800%
46) 2-Hexanone-d5	8.635	63	86809	62.622	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	125.240%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	37079	5.785	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	115.600%
66) 1,2-Dichlorobenzene-d4	12.195	152	39847	5.868	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	117.400%
Target Compounds						
					Qvalue	
48) 2-Hexanone	8.693	43	11720	3.853	ug/L	# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
Data File : VU046002.D
Acq On : 24 Nov 2021 18:14
Operator : SY/MD
Sample : M4779-11
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001


Quant Time: Nov 26 00:22:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 26 00:17:51 2021
Response via : Initial Calibration

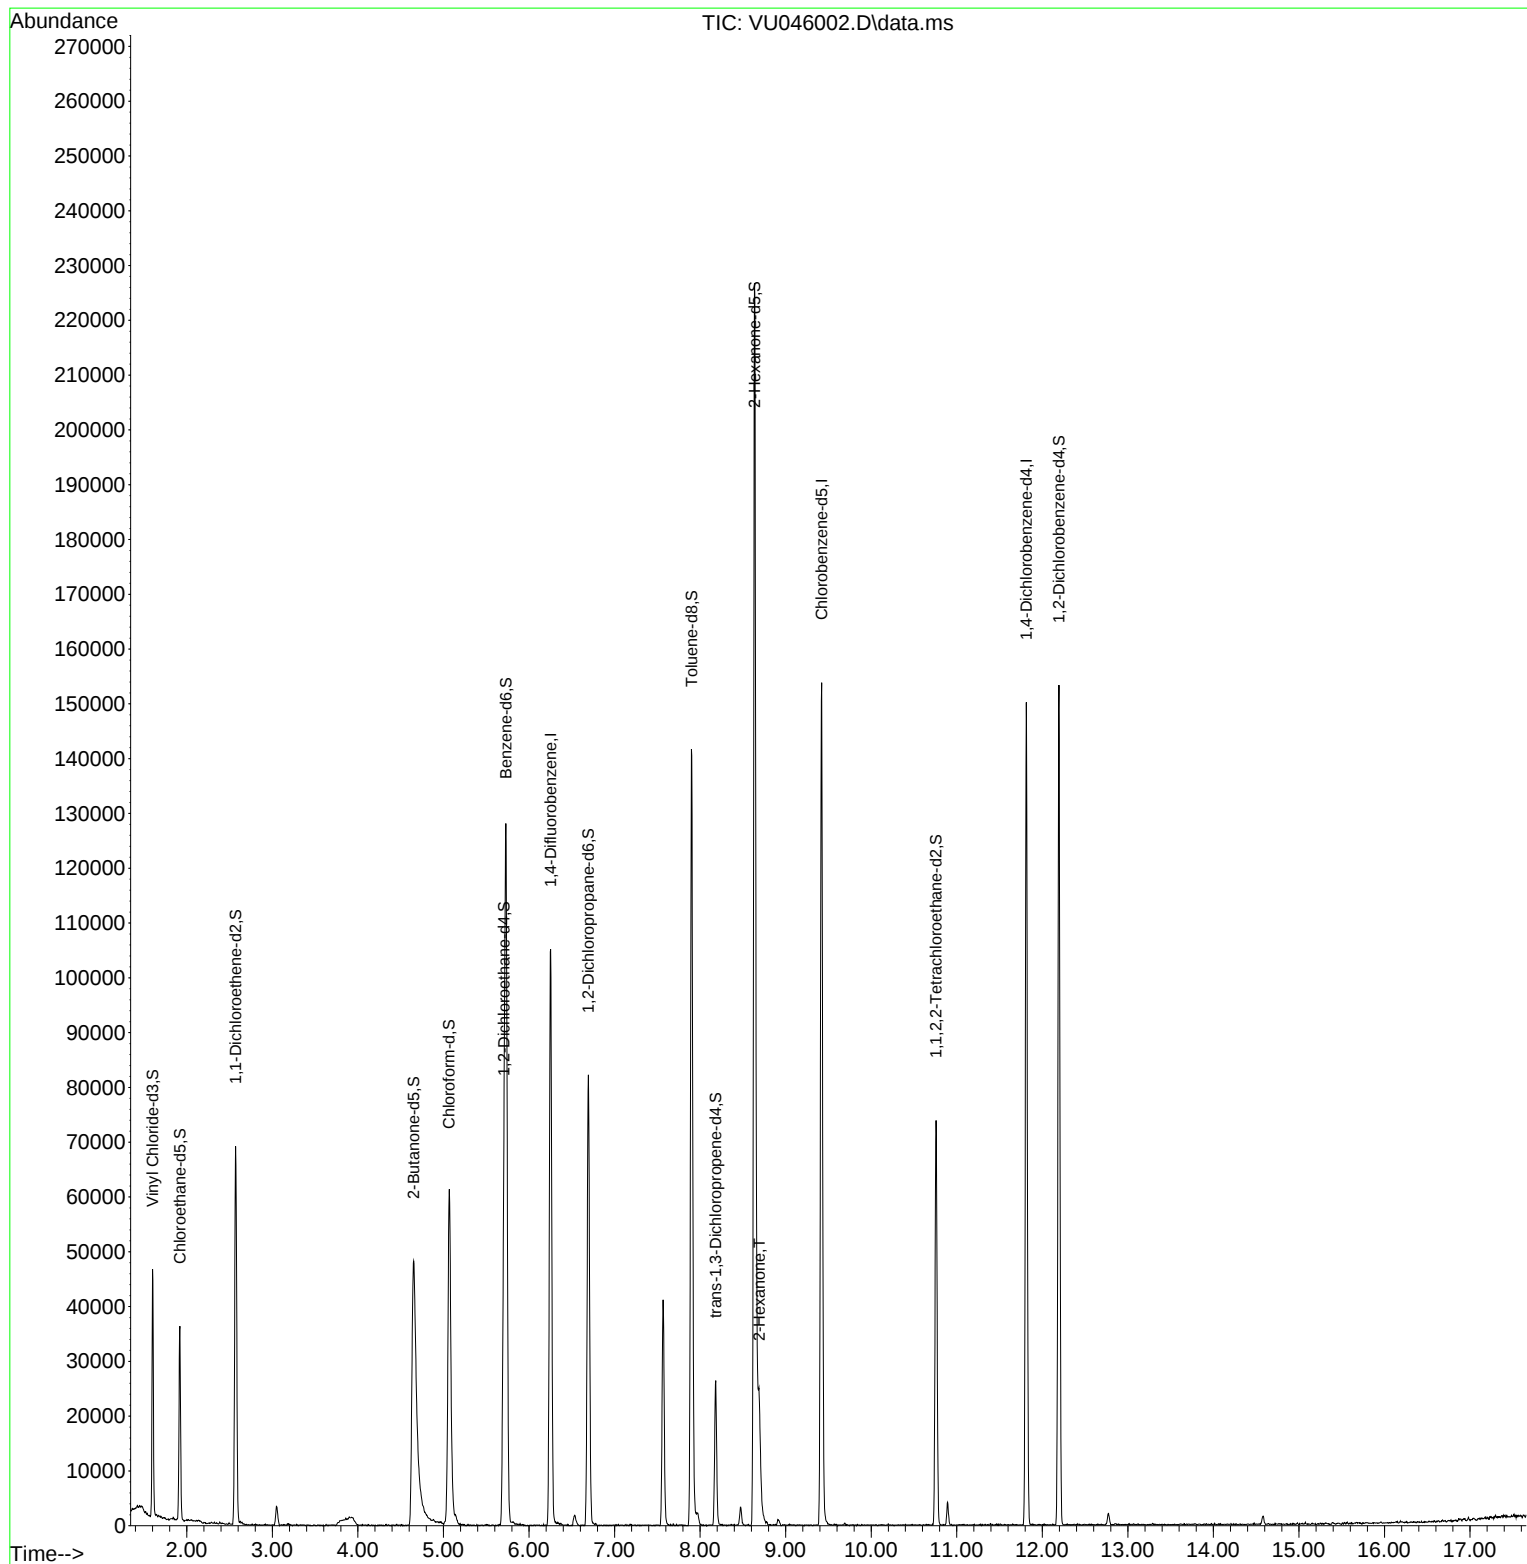

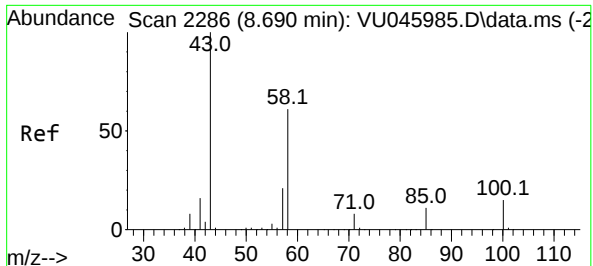

#48
 2-Hexanone
 Concen: 3.853 ug/L
 RT: 8.693 min Scan# 21
 Delta R.T. 0.003 min
 Lab File: VU046002.D
 Acq: 24 Nov 2021 18:14

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

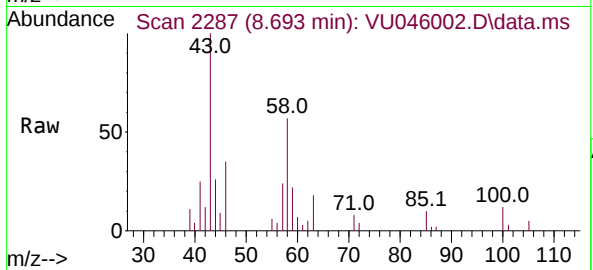

Tgt Ion: 43	Resp: 11720
Ion Ratio	Lower Upper
43 100	
58 57.5	46.7 70.1
57 25.4	16.3 24.5#
100 11.2	10.5 15.7

