

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
 Data File : VU045996.D
 Acq On : 24 Nov 2021 15:51
 Operator : SY/MD
 Sample : M4722-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0G12

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU045996.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	94	rVB	22380	24147	5.13%	0.772%
2	1.919	171	180	191	rVB	33670	42921	9.12%	1.372%
3	2.572	372	383	397	rBV	58165	94076	19.99%	3.007%
4	2.665	397	412	417	rBV2	2416	5158	1.10%	0.165%
5	3.835	753	776	778	rBV2	1920	5754	1.22%	0.184%
6	4.649	1010	1029	1067	rBV2	51664	208783	44.36%	6.674%
7	5.067	1143	1159	1178	rBV	67371	157496	33.47%	5.034%
8	5.729	1344	1365	1386	rBV2	138250	359893	76.47%	11.504%
9	6.253	1514	1528	1547	rBV	110764	207731	44.14%	6.640%
10	6.694	1650	1665	1684	rBV	89406	171130	36.36%	5.470%
11	7.182	1806	1817	1831	rVB5	2750	5643	1.20%	0.180%
12	7.568	1926	1937	1949	rBV2	31703	54830	11.65%	1.753%
13	7.899	2027	2040	2057	rBV	155268	279312	59.35%	8.928%
14	8.182	2117	2128	2142	rBV2	19286	32122	6.83%	1.027%
15	8.475	2208	2219	2232	rBV2	7194	12337	2.62%	0.394%
16	8.636	2256	2269	2306	rBV	230327	470603	100.00%	15.043%
17	8.787	2306	2316	2328	rVV2	12676	21015	4.47%	0.672%
18	9.420	2500	2513	2535	rBV	155120	265028	56.32%	8.472%
19	10.758	2918	2929	2944	rVB	75290	120166	25.53%	3.841%
20	10.893	2958	2971	2984	rBV	15712	24778	5.27%	0.792%
21	11.475	3144	3152	3163	rBV3	2911	4722	1.00%	0.151%
22	11.812	3246	3257	3275	rBV	163710	252275	53.61%	8.064%
23	12.063	3326	3335	3351	rBV2	7059	13761	2.92%	0.440%
24	12.195	3364	3376	3390	rVB	166187	267923	56.93%	8.564%
25	12.774	3545	3556	3565	rBV	6004	10021	2.13%	0.320%
26	12.886	3577	3591	3607	rVB4	6456	11602	2.47%	0.371%
27	14.578	4107	4117	4128	rVB	3370	5226	1.11%	0.167%




Sum of corrected areas: 3128453

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
Data File : VU045996.D
Acq On : 24 Nov 2021 15:51
Operator : SY/MD
Sample : M4722-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

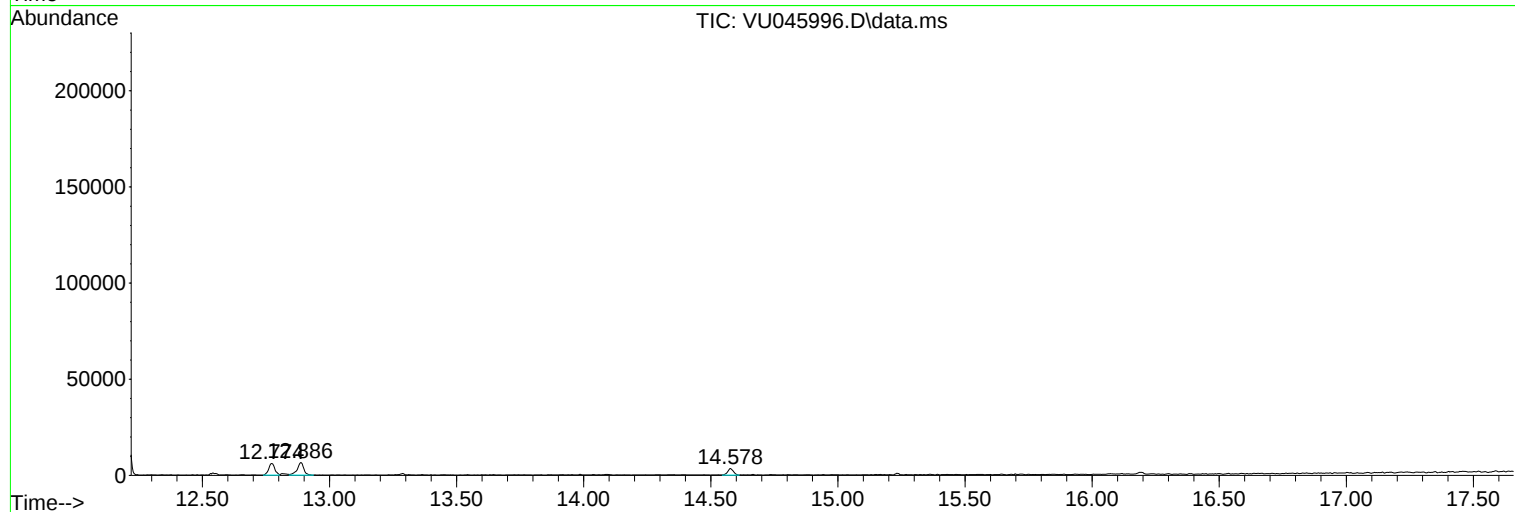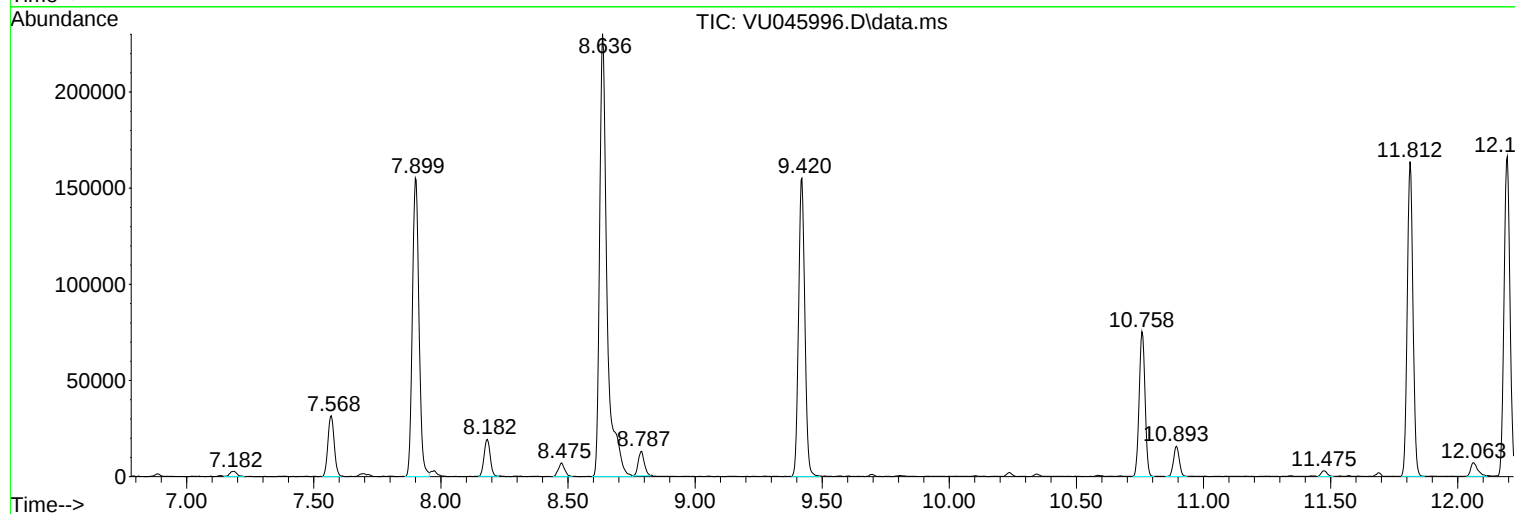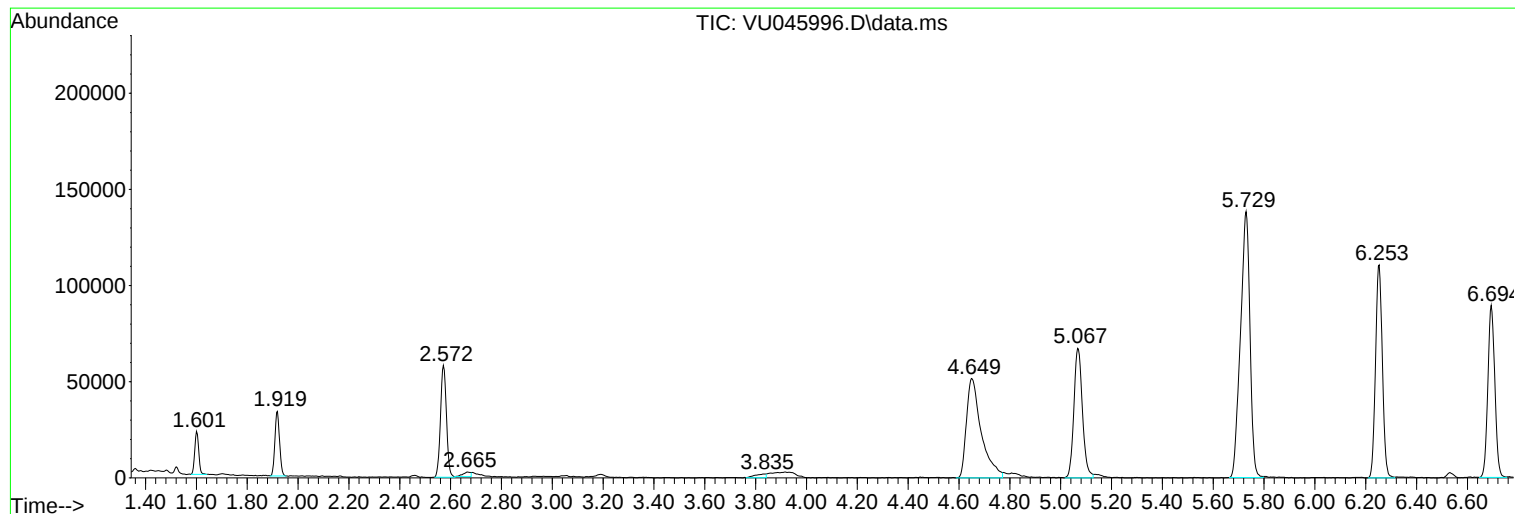

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
Data File : VU045996.D
Acq On : 24 Nov 2021 15:51
Operator : SY/MD
Sample : M4722-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
Data File : VU045996.D
Acq On : 24 Nov 2021 15:51
Operator : SY/MD
Sample : M4722-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0G12

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc