


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112421\
Data File : VU045984.D
Acq On : 24 Nov 2021 09:48
Operator : SY/MD
Sample : BFB031
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB031

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Nov 26 23:26:55 2021

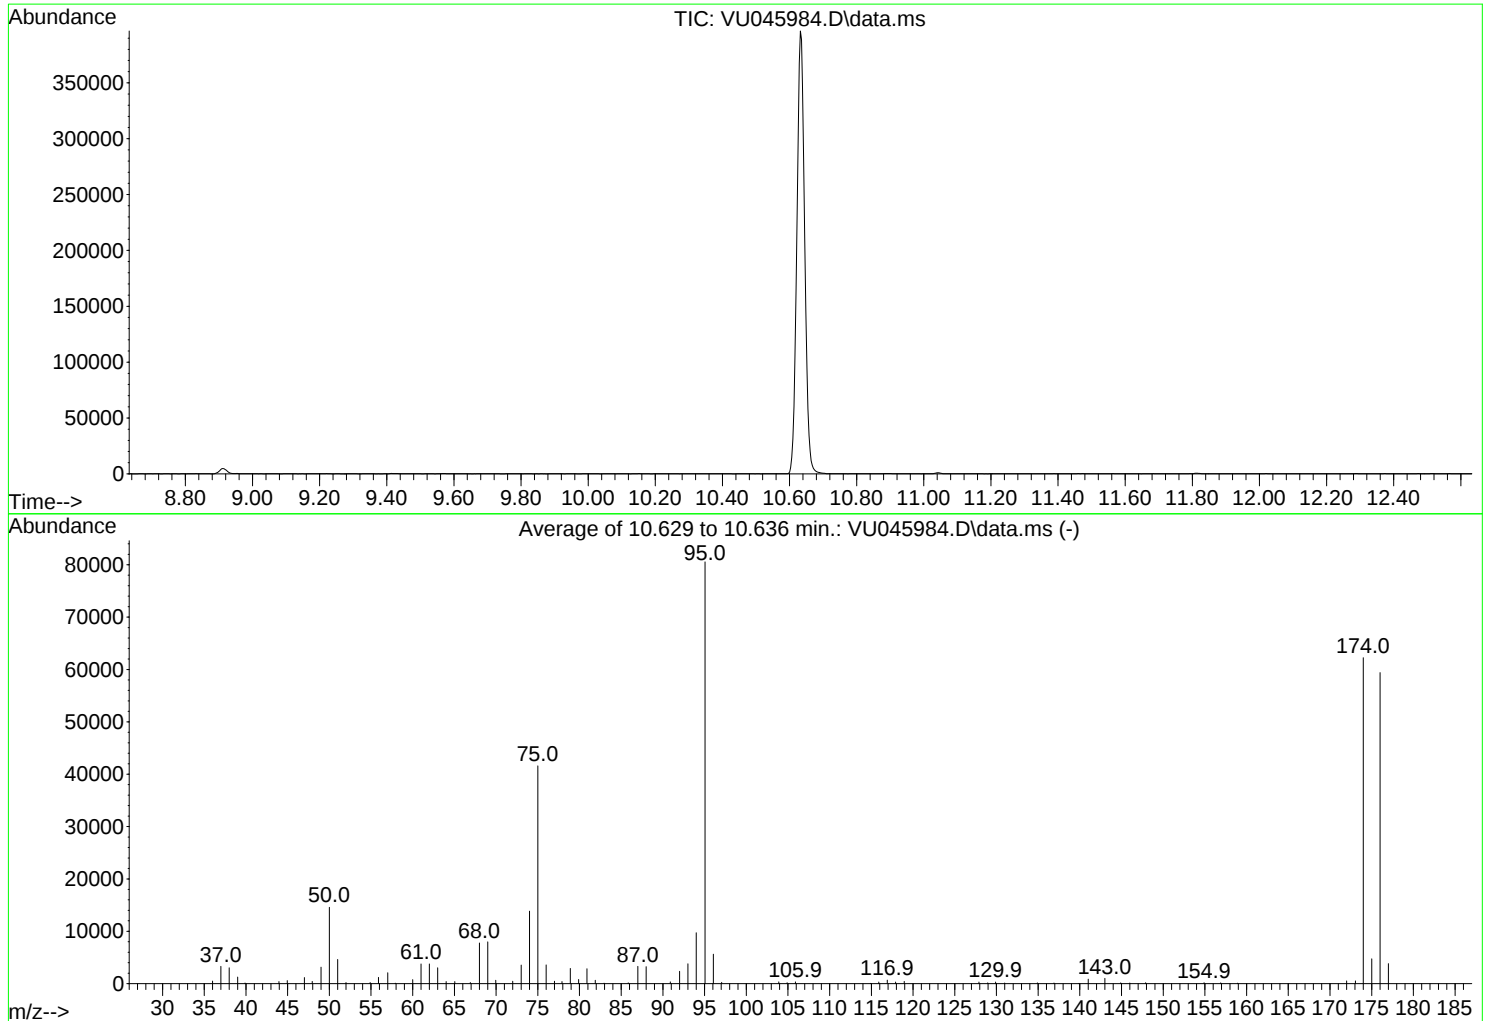

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	14584	PASS
75	95	30	80	51.6	41595	PASS
95	95	100	100	100.0	80557	PASS
96	95	5	9	7.0	5637	PASS
173	174	0.00	2	0.8	518	PASS
174	95	50	120	77.3	62251	PASS
175	174	5	9	7.6	4738	PASS
176	174	95	101	95.5	59419	PASS
177	176	5	9	6.4	3821	PASS

m/z	Abundance
44.00	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031

m/z	Abundance
36.00	499.0
37.00	3182.0
38.00	3119.0
39.00	1207.0
39.90	103.0
43.90	504.0
44.90	560.0
47.00	1074.0
48.00	437.0
49.00	3157.0
50.00	14233.0
51.00	4515.0
52.00	216.0
54.90	198.0
55.90	1184.0
57.00	1998.0
60.00	721.0
61.00	3680.0
62.00	3640.0
63.00	2884.0
64.00	427.0
65.10	408.0
66.90	211.0
68.00	7603.0
69.00	7632.0
69.90	612.0
72.00	462.0
73.00	3506.0
74.00	13540.0
75.00	40472.0
76.00	3514.0
77.00	410.0
77.90	350.0
78.90	2763.0
79.90	813.0
80.90	2860.0
81.90	613.0
83.00	133.0
85.80	109.0
87.00	3177.0
88.00	3068.0
90.90	351.0
92.00	2256.0
93.00	3755.0
94.00	9166.0
95.10	77264.0
96.00	5466.0
97.00	234.0
103.90	337.0
104.90	177.0
105.90	360.0
114.90	107.0
115.90	312.0
116.90	665.0
117.90	265.0
118.90	418.0
127.90	298.0
128.90	142.0
129.90	264.0
131.00	114.0
134.90	140.0
136.90	101.0
139.90	102.0
141.00	833.0
143.00	1000.0
144.90	129.0
146.00	121.0
147.90	212.0
154.90	164.0
156.90	122.0
172.00	512.0
173.10	533.0
174.00	58280.0
175.00	4504.0
176.00	55296.0
177.00	3622.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031

m/z	Abundance
36.00	484.0
37.00	3435.0
38.00	3095.0
39.00	1295.0
39.90	121.0
44.00	520.0
44.90	615.0
47.00	1196.0
48.00	460.0
49.00	3264.0
50.00	15067.0
51.00	4797.0
52.00	238.0
54.90	240.0
55.90	1225.0
57.00	2134.0
57.90	121.0
60.00	766.0
61.00	3872.0
62.00	3879.0
63.00	3130.0
64.00	410.0
65.00	407.0
66.90	229.0
68.00	7967.0
69.00	8249.0
70.00	690.0
72.00	475.0
73.00	3657.0
74.00	14292.0
75.00	42864.0
76.00	3713.0
77.00	462.0
77.90	432.0
78.90	3000.0
79.90	830.0
80.90	2933.0
81.90	669.0
82.90	122.0
85.90	153.0
87.00	3405.0
88.00	3343.0
90.90	366.0
92.00	2435.0
93.00	3945.0
94.00	10032.0
95.00	83128.0
96.10	5820.0
97.10	250.0
103.90	344.0
104.90	189.0
105.90	365.0
114.90	108.0
115.90	306.0
116.90	716.0
117.90	319.0
118.90	429.0
127.90	310.0
129.00	150.0
129.90	330.0
131.00	119.0
134.90	172.0
136.90	118.0
139.90	109.0
141.00	890.0
143.00	1041.0
144.90	140.0
146.00	126.0
147.90	199.0
154.90	180.0
156.90	150.0
158.90	134.0
172.00	519.0
173.10	520.0
174.00	64088.0
175.00	4929.0
176.00	61160.0
177.00	3962.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031

m/z	Abundance
36.00	458.0
37.00	3270.0
38.00	2856.0
39.00	1259.0
39.90	113.0
44.00	553.0
45.00	623.0
47.00	1174.0
47.90	434.0
49.00	3001.0
50.00	14451.0
51.00	4555.0
52.00	213.0
54.90	239.0
55.90	1147.0
57.00	2116.0
57.90	127.0
60.00	788.0
61.00	3696.0
62.00	3797.0
63.00	3053.0
64.00	381.0
65.00	377.0
66.90	231.0
68.00	7674.0
69.00	8073.0
70.00	673.0
72.00	423.0
73.00	3505.0
74.00	13672.0
75.00	41448.0
76.00	3522.0
77.00	510.0
77.90	419.0
78.90	2921.0
79.90	759.0
80.90	2736.0
81.90	654.0
85.90	176.0
87.00	3285.0
88.00	3341.0
90.90	349.0
92.00	2393.0
93.00	3700.0
94.00	9940.0
95.00	81280.0
96.10	5625.0
97.10	215.0
103.90	318.0
104.90	170.0
105.90	336.0
115.90	261.0
116.90	682.0
117.90	332.0
119.00	480.0
127.90	287.0
128.90	130.0
129.90	374.0
131.00	100.0
134.90	184.0
136.90	143.0
141.00	841.0
143.00	963.0
144.90	162.0
146.00	106.0
147.90	171.0
154.90	180.0
156.90	159.0
158.90	135.0
172.00	498.0
173.00	501.0
174.00	64384.0
175.00	4782.0
176.00	61800.0
177.00	3879.0

Instrument :
MSVOA_U
ClientSampleId :
BFB031