

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112423\
 Data File : VU056604.D
 Acq On : 24 Nov 2023 11:00
 Operator : MD/SY
 Sample : 05476-21
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056604.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.489	53	62	68	rBV2	8909	17572	1.83%	0.218%
2	1.595	86	95	109	rVB	138476	157658	16.43%	1.955%
3	1.907	184	192	208	rVB	94733	129144	13.46%	1.601%
4	2.560	383	395	415	rBV	212242	346902	36.16%	4.301%
5	3.039	533	544	561	rVB	16452	31846	3.32%	0.395%
6	3.181	573	588	606	rBV2	15107	36767	3.83%	0.456%
7	4.621	1022	1036	1085	rBV2	128043	363988	37.94%	4.513%
8	5.055	1155	1171	1192	rBV	190734	423581	44.16%	5.251%
9	5.721	1354	1378	1412	rBV2	366487	959285	100.00%	11.893%
10	6.242	1528	1540	1566	rBV	325059	644295	67.16%	7.988%
11	6.685	1659	1678	1704	rBV	224521	448121	46.71%	5.556%
12	7.560	1939	1950	1976	rBV	113979	208778	21.76%	2.588%
13	7.894	2037	2054	2078	rBV	427662	787579	82.10%	9.764%
14	8.177	2131	2142	2157	rBV	72220	125670	13.10%	1.558%
15	8.631	2271	2283	2317	rBV	456668	886888	92.45%	10.995%
16	9.412	2511	2526	2547	rBV	451012	815483	85.01%	10.110%
17	10.753	2930	2943	2956	rBV	162332	260191	27.12%	3.226%
18	10.888	2976	2985	2996	rVB2	8541	13461	1.40%	0.167%
19	11.807	3258	3271	3300	rBV	447587	740778	77.22%	9.184%
20	12.187	3376	3389	3410	rBV	396141	668033	69.64%	8.282%




Sum of corrected areas: 8066020

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112423\
Data File : VU056604.D
Acq On : 24 Nov 2023 11:00
Operator : MD/SY
Sample : 05476-21
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

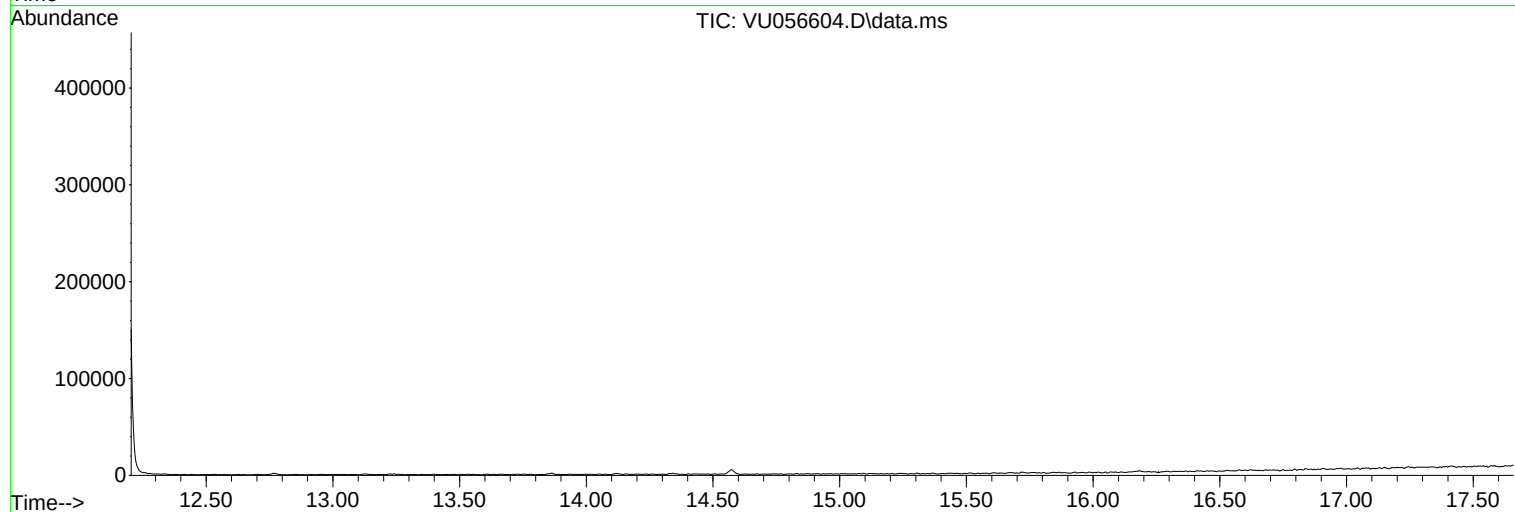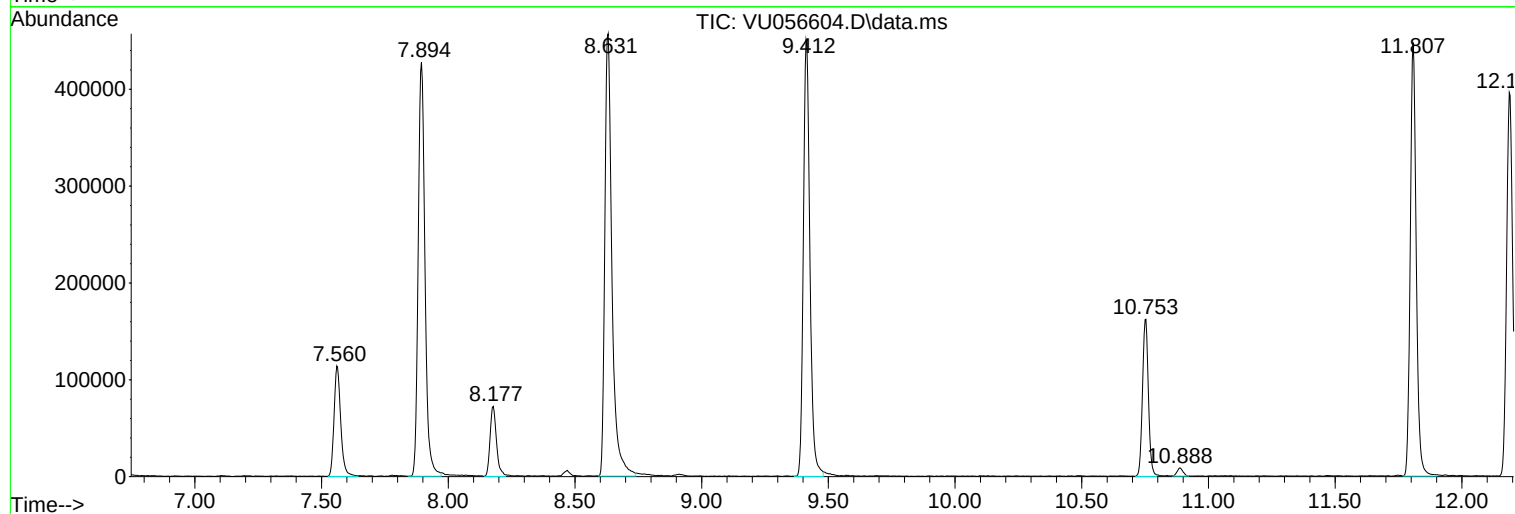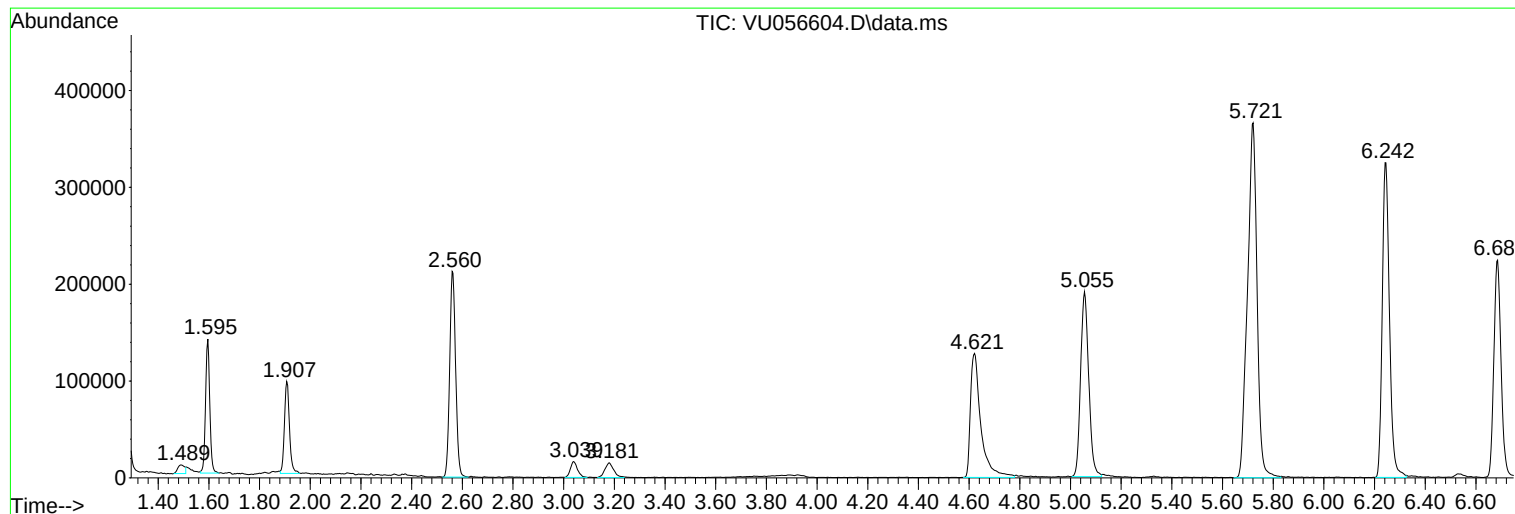

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112423\
Data File : VU056604.D
Acq On : 24 Nov 2023 11:00
Operator : MD/SY
Sample : 05476-21
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112423\
Data File : VU056604.D
Acq On : 24 Nov 2023 11:00
Operator : MD/SY
Sample : 05476-21
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc