


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112423\
Data File : VU056600.D
Acq On : 24 Nov 2023 08:46
Operator : MD/SY
Sample : BFB081
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB081

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat Nov 25 01:37:48 2023

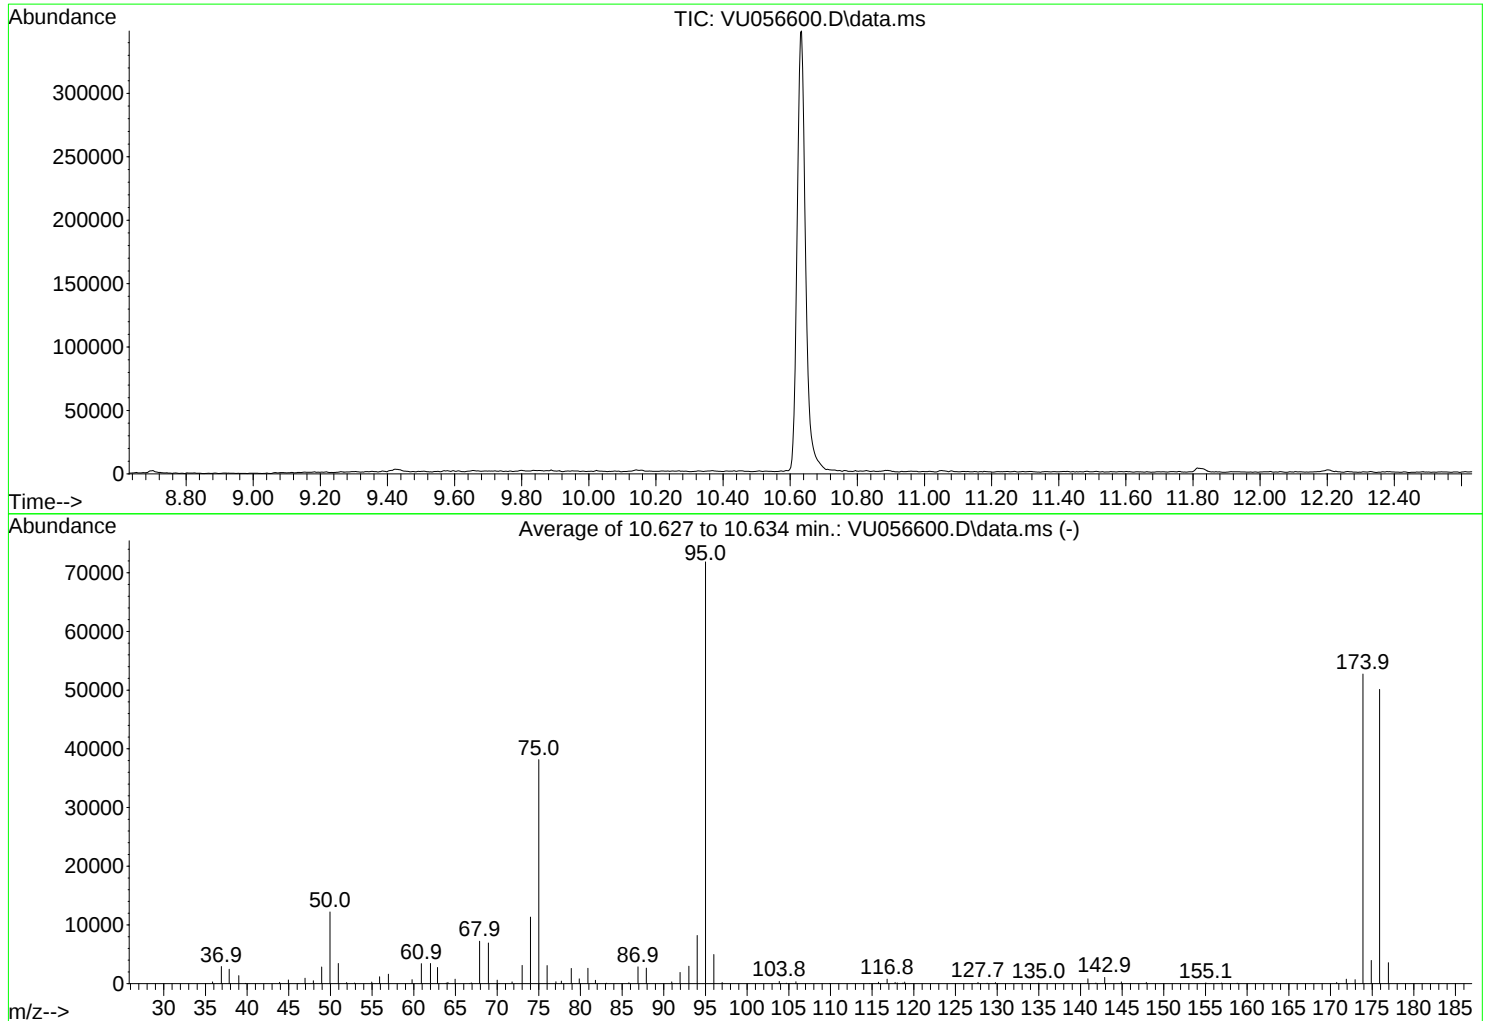

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	12224	PASS
75	95	30	80	53.1	38152	PASS
95	95	100	100	100.0	71851	PASS
96	95	5	9	6.9	4963	PASS
173	174	0.00	2	1.3	682	PASS
174	95	50	120	73.4	52755	PASS
175	174	5	9	7.5	3948	PASS
176	174	95	101	95.0	50120	PASS
177	176	5	9	7.1	3565	PASS

m/z	Abundance
35.90	1209.0
37.00	125.0
37.90	488.0
39.90	255.0
43.90	447.0
206.90	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081

m/z	Abundance
35.90	1458.0
36.90	2883.0
37.90	2896.0
39.00	1399.0
39.80	272.0
44.00	634.0
44.90	600.0
46.10	126.0
46.90	846.0
48.00	419.0
48.90	2581.0
50.00	11754.0
51.00	3479.0
51.90	148.0
55.00	304.0
55.90	1248.0
57.00	1491.0
59.80	671.0
60.90	3319.0
62.00	3525.0
62.90	2686.0
63.90	329.0
64.90	670.0
66.70	120.0
67.90	6953.0
69.00	6629.0
70.00	582.0
71.80	302.0
73.00	3030.0
74.00	10204.0
75.00	35752.0
76.00	2799.0
77.10	249.0
77.70	428.0
78.90	2690.0
79.90	722.0
80.90	2476.0
81.80	513.0
83.10	120.0
85.80	172.0
86.90	2833.0
87.90	2533.0
90.90	279.0
91.90	1780.0
93.00	2847.0
94.00	7686.0
95.00	67776.0
96.00	4890.0
97.00	244.0
103.90	291.0
104.70	123.0
105.80	276.0
115.70	237.0
116.80	726.0
117.70	287.0
118.70	324.0
127.70	196.0
129.80	199.0
140.90	736.0
142.00	111.0
143.00	946.0
145.00	299.0
147.90	153.0
155.10	106.0
156.90	100.0
158.80	121.0
170.80	218.0
171.90	603.0
173.00	464.0
173.90	48600.0
174.90	3669.0
175.90	45560.0
177.00	3404.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081

m/z	Abundance
35.90	1528.0
36.90	3097.0
37.90	3022.0
39.00	1395.0
39.80	321.0
43.90	665.0
44.90	656.0
47.00	943.0
47.90	526.0
49.00	2910.0
49.90	12676.0
51.00	3534.0
51.90	209.0
52.90	143.0
54.90	283.0
55.90	1259.0
56.90	1658.0
59.80	714.0
60.90	3496.0
62.00	3559.0
62.80	2890.0
64.10	326.0
64.90	774.0
66.90	175.0
67.90	7410.0
69.00	7205.0
70.00	648.0
71.80	313.0
73.00	3219.0
74.00	11627.0
75.00	39408.0
76.00	3168.0
77.00	342.0
77.70	495.0
78.90	2702.0
79.80	858.0
80.90	2745.0
81.80	593.0
83.10	117.0
85.80	168.0
86.90	2875.0
87.90	2611.0
90.90	287.0
92.00	1961.0
93.00	3038.0
94.00	8464.0
95.00	73960.0
96.00	5218.0
97.00	179.0
103.80	403.0
104.70	114.0
105.90	349.0
114.70	100.0
115.80	256.0
116.80	803.0
117.80	343.0
118.90	363.0
127.70	241.0
128.80	118.0
129.80	199.0
135.00	129.0
140.90	855.0
141.80	132.0
142.90	1073.0
144.90	304.0
147.90	175.0
155.00	139.0
157.00	106.0
158.80	119.0
170.70	265.0
171.90	787.0
172.90	677.0
173.90	54256.0
174.90	4051.0
175.90	51800.0
176.90	3649.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081

m/z	Abundance
35.90	1515.0
36.90	3143.0
37.90	2882.0
39.00	1339.0
39.80	309.0
43.90	675.0
45.00	611.0
47.00	958.0
47.90	544.0
48.90	3003.0
49.90	12242.0
50.90	3331.0
52.00	232.0
52.90	220.0
54.90	235.0
55.90	1048.0
56.90	1694.0
59.80	687.0
60.90	3417.0
62.00	3262.0
62.90	2712.0
64.10	355.0
65.00	829.0
66.90	204.0
67.90	7278.0
68.90	6982.0
70.00	602.0
71.80	292.0
73.00	3121.0
74.00	12235.0
75.00	39296.0
76.00	3277.0
77.00	374.0
77.70	386.0
78.90	2401.0
79.80	909.0
80.90	2647.0
81.80	607.0
85.80	127.0
86.90	2867.0
87.90	2755.0
91.00	299.0
92.00	1980.0
93.00	3035.0
94.00	8496.0
95.00	73816.0
96.00	4782.0
97.00	118.0
103.80	468.0
105.90	390.0
109.90	108.0
115.80	273.0
116.80	761.0
118.00	413.0
118.90	465.0
127.70	250.0
128.80	131.0
129.80	179.0
135.00	117.0
140.90	898.0
141.70	111.0
142.80	1174.0
144.80	339.0
146.00	138.0
147.70	180.0
148.00	187.0
155.00	169.0
157.00	113.0
170.70	192.0
171.90	879.0
173.00	906.0
173.90	55408.0
174.90	4125.0
175.90	53000.0
176.90	3642.0

Instrument :
MSVOA_U
ClientSampleId :
BFB081