

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
 Data File : VU063786.D
 Acq On : 24 Nov 2025 18:40
 Operator : MD/SY
 Sample : VIBLK062
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK062

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

Signal : TIC: VU063786.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.512	65	69	73	rBV2	1684	1731	0.13%	0.018%
2	1.586	84	92	102	rBV	178416	192750	14.47%	1.951%
3	1.895	179	188	200	rBV	138873	181110	13.60%	1.833%
4	2.493	370	374	377	rBV4	815	564	0.04%	0.006%
5	2.541	377	389	408	rBV	272981	458022	34.38%	4.635%
6	2.743	448	452	453	rBV	469	301	0.02%	0.003%
7	2.859	485	488	492	rBV	330	220	0.02%	0.002%
8	2.914	500	505	508	rBV2	327	327	0.02%	0.003%
9	3.020	528	538	549	rVB3	3563	6902	0.52%	0.070%
10	3.113	563	567	570	rBV2	296	297	0.02%	0.003%
11	3.165	572	583	589	rBV3	1495	2690	0.20%	0.027%
12	3.261	609	613	619	rVB2	374	440	0.03%	0.004%
13	3.338	624	637	650	rBV5	2881	5500	0.41%	0.056%
14	3.386	650	652	658	rVB	247	214	0.02%	0.002%
15	3.602	714	719	723	rVB2	295	296	0.02%	0.003%
16	3.628	723	727	729	rBV	276	226	0.02%	0.002%
17	3.676	736	742	746	rBV2	288	312	0.02%	0.003%
18	3.766	767	770	775	rVB2	395	403	0.03%	0.004%
19	3.837	784	792	798	rBV4	823	1586	0.12%	0.016%
20	3.994	839	841	845	rVB2	380	210	0.02%	0.002%
21	4.030	849	852	856	rBV2	266	253	0.02%	0.003%
22	4.165	891	894	896	rBV	282	213	0.02%	0.002%
23	4.595	1019	1028	1062	rBV	86963	253048	19.00%	2.561%
24	5.029	1147	1163	1206	rBV	226253	533617	40.06%	5.400%
25	5.271	1232	1238	1239	rBV3	1072	938	0.07%	0.009%
26	5.351	1254	1263	1267	rBV6	1491	2368	0.18%	0.024%
27	5.406	1275	1280	1283	rVB2	395	378	0.03%	0.004%
28	5.492	1302	1307	1308	rBV2	661	660	0.05%	0.007%
29	5.695	1349	1370	1414	rBV2	444489	1332050	100.00%	13.479%
30	6.219	1517	1533	1579	rBV	350852	739380	55.51%	7.482%
31	6.512	1613	1624	1638	rBV6	7682	17446	1.31%	0.177%
32	6.660	1656	1670	1697	rBV	279360	587121	44.08%	5.941%
33	6.853	1728	1730	1736	rVB2	521	388	0.03%	0.004%
34	6.898	1741	1744	1747	rVV3	410	245	0.02%	0.002%
35	6.978	1764	1769	1775	rBV4	448	619	0.05%	0.006%
36	7.017	1779	1781	1788	rVB2	295	211	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
 Data File : VU063786.D
 Acq On : 24 Nov 2025 18:40
 Operator : MD/SY
 Sample : VIBLK062
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK062

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

37	7.068	1795	1797	1800	rBV	697	469	0.04%	0.005%
38	7.328	1876	1878	1882	rVV2	262	223	0.02%	0.002%
39	7.357	1883	1887	1890	rVB2	228	213	0.02%	0.002%
40	7.444	1910	1914	1920	rVB2	259	260	0.02%	0.003%

41	7.541	1932	1944	1970	rBV	126753	243059	18.25%	2.460%
42	7.721	1994	2000	2005	rVB4	547	731	0.05%	0.007%
43	7.779	2010	2018	2028	rBV6	1810	2690	0.20%	0.027%
44	7.872	2034	2047	2078	rBV	567559	1073628	80.60%	10.864%
45	8.155	2124	2135	2156	rBV2	79303	147146	11.05%	1.489%

46	8.380	2198	2205	2216	rVB5	2067	2995	0.22%	0.030%
47	8.531	2245	2252	2265	rVB6	2793	4568	0.34%	0.046%
48	8.615	2265	2278	2323	rBV3	207260	580922	43.61%	5.879%
49	8.946	2376	2381	2384	rBV4	307	342	0.03%	0.003%
50	9.045	2407	2412	2419	rVB2	538	655	0.05%	0.007%

51	9.094	2419	2427	2431	rBV2	528	601	0.05%	0.006%
52	9.139	2438	2441	2443	rBV2	344	218	0.02%	0.002%
53	9.180	2451	2454	2460	rVB3	301	271	0.02%	0.003%
54	9.393	2507	2520	2562	rVV	516422	947274	71.11%	9.586%
55	9.550	2562	2569	2584	rVB2	4114	7099	0.53%	0.072%

56	9.679	2597	2609	2624	rBV2	3347	5794	0.43%	0.059%
57	9.817	2647	2652	2655	rBV	268	245	0.02%	0.002%
58	9.914	2675	2682	2686	rBV	178	240	0.02%	0.002%
59	9.959	2692	2696	2698	rBV	276	234	0.02%	0.002%
60	10.084	2725	2735	2740	rBV4	3273	5731	0.43%	0.058%

61	10.261	2785	2790	2792	rBV3	417	312	0.02%	0.003%
62	10.277	2792	2795	2798	rVB3	463	280	0.02%	0.003%
63	10.399	2830	2833	2836	rBV	347	256	0.02%	0.003%
64	10.463	2843	2853	2861	rBV3	3534	5550	0.42%	0.056%
65	10.521	2866	2871	2874	rBV2	383	343	0.03%	0.003%

66	10.537	2874	2876	2881	rVB2	283	217	0.02%	0.002%
67	10.595	2890	2894	2899	rBV2	295	230	0.02%	0.002%
68	10.730	2924	2936	2955	rBV	398269	659022	49.47%	6.669%
69	10.868	2976	2979	2986	rVB4	701	922	0.07%	0.009%
70	10.904	2986	2990	2996	rVB	317	255	0.02%	0.003%

71	11.068	3030	3041	3060	rVV3	2980	5096	0.38%	0.052%
72	11.264	3097	3102	3104	rBV2	269	274	0.02%	0.003%
73	11.454	3149	3161	3174	rVB3	2821	4554	0.34%	0.046%
74	11.663	3223	3226	3231	rBV	353	372	0.03%	0.004%
75	11.727	3239	3246	3252	rBV3	3379	4763	0.36%	0.048%

76	11.788	3252	3265	3288	rVV	525686	896345	67.29%	9.070%
----	--------	------	------	------	-----	--------	--------	--------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
 Data File : VU063786.D
 Acq On : 24 Nov 2025 18:40
 Operator : MD/SY
 Sample : VIBLK062
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK062

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
 Title : VOC Analysis

77	11.949	3312	3315	3319	rVB3	933	674	0.05%	0.007%
78	12.032	3337	3341	3346	rBV2	514	580	0.04%	0.006%
79	12.103	3358	3363	3367	rBV2	718	798	0.06%	0.008%
80	12.167	3370	3383	3413	rVV	553296	936318	70.29%	9.475%
81	12.357	3440	3442	3447	rVB2	408	273	0.02%	0.003%
82	12.737	3552	3560	3563	rBV2	454	564	0.04%	0.006%
83	12.756	3563	3566	3570	rVB2	469	375	0.03%	0.004%
84	12.981	3632	3636	3639	rBV2	340	329	0.02%	0.003%
85	13.167	3691	3694	3696	rBV3	405	210	0.02%	0.002%
86	13.206	3699	3706	3714	rVB5	1993	2972	0.22%	0.030%
87	13.267	3718	3725	3729	rBV3	376	537	0.04%	0.005%
88	13.290	3729	3732	3735	rVV2	468	369	0.03%	0.004%
89	13.309	3735	3738	3741	rVB2	401	245	0.02%	0.002%
90	13.344	3746	3749	3754	rVB2	400	286	0.02%	0.003%
91	13.476	3785	3790	3792	rBV	357	345	0.03%	0.003%
92	13.669	3845	3850	3853	rVB2	567	578	0.04%	0.006%
93	13.691	3853	3857	3860	rBV2	535	498	0.04%	0.005%
94	13.827	3892	3899	3909	rBV8	2051	3293	0.25%	0.033%
95	14.013	3955	3957	3964	rVB2	430	288	0.02%	0.003%
96	14.081	3971	3978	3984	rBV3	1795	2526	0.19%	0.026%
97	14.103	3984	3985	3991	rVB2	638	413	0.03%	0.004%
98	14.309	4043	4049	4050	rBV2	1917	1530	0.11%	0.015%
99	14.412	4078	4081	4084	rBV2	614	374	0.03%	0.004%
100	14.444	4089	4091	4094	rBV2	438	239	0.02%	0.002%




Sum of corrected areas: 9882049

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
Data File : VU063786.D
Acq On : 24 Nov 2025 18:40
Operator : MD/SY
Sample : VIBLK062
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK062

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

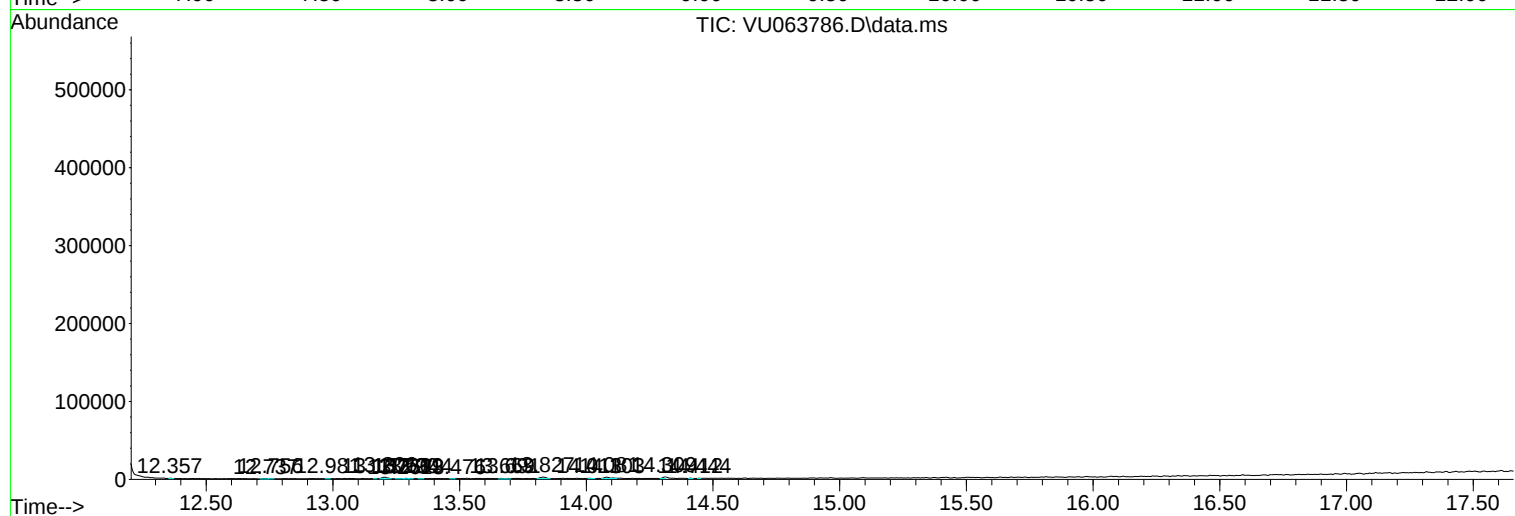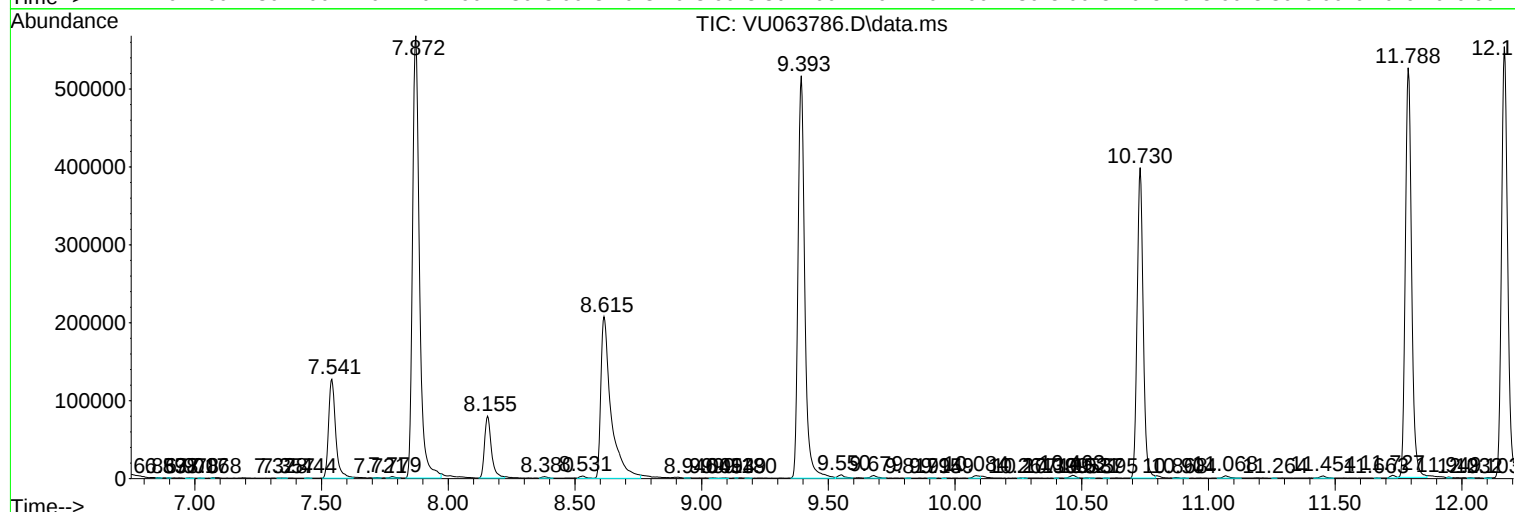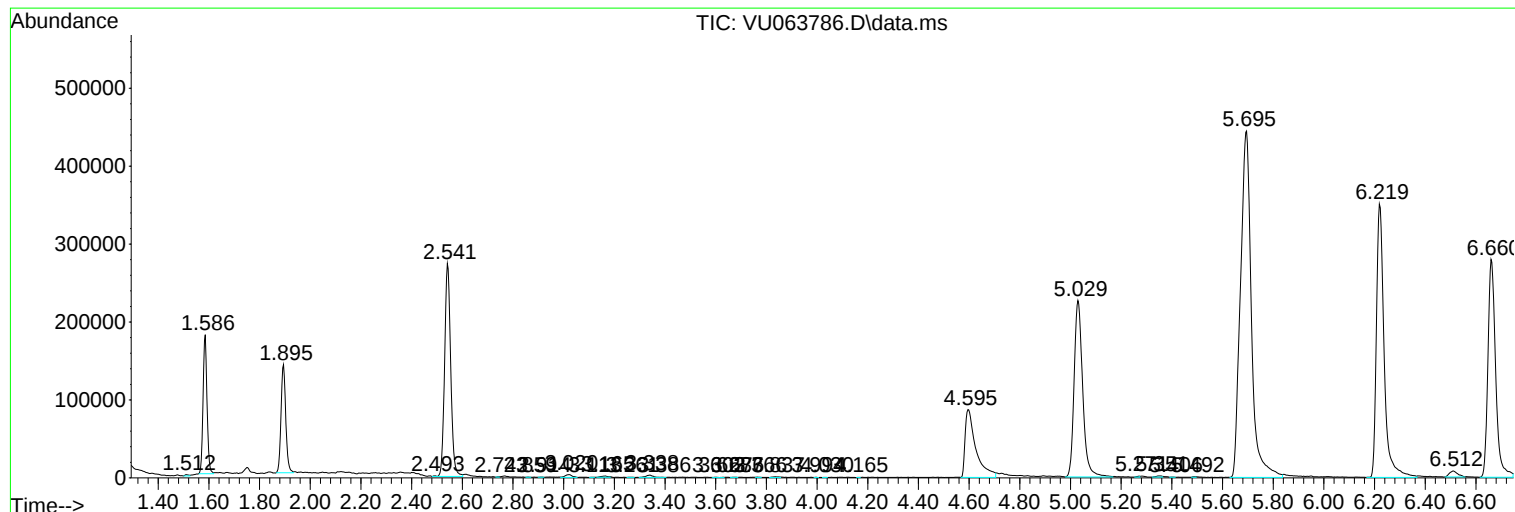

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
Data File : VU063786.D
Acq On : 24 Nov 2025 18:40
Operator : MD/SY
Sample : VIBLK062
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK062

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
Data File : VU063786.D
Acq On : 24 Nov 2025 18:40
Operator : MD/SY
Sample : VIBLK062
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK062

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc