


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112425\
Data File : VU063773.D
Acq On : 24 Nov 2025 12:38
Operator : MD/SY
Sample : BFB093
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB093

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM111725WMA.M
Title : VOC Analysis
Last Update : Tue Nov 25 00:22:49 2025

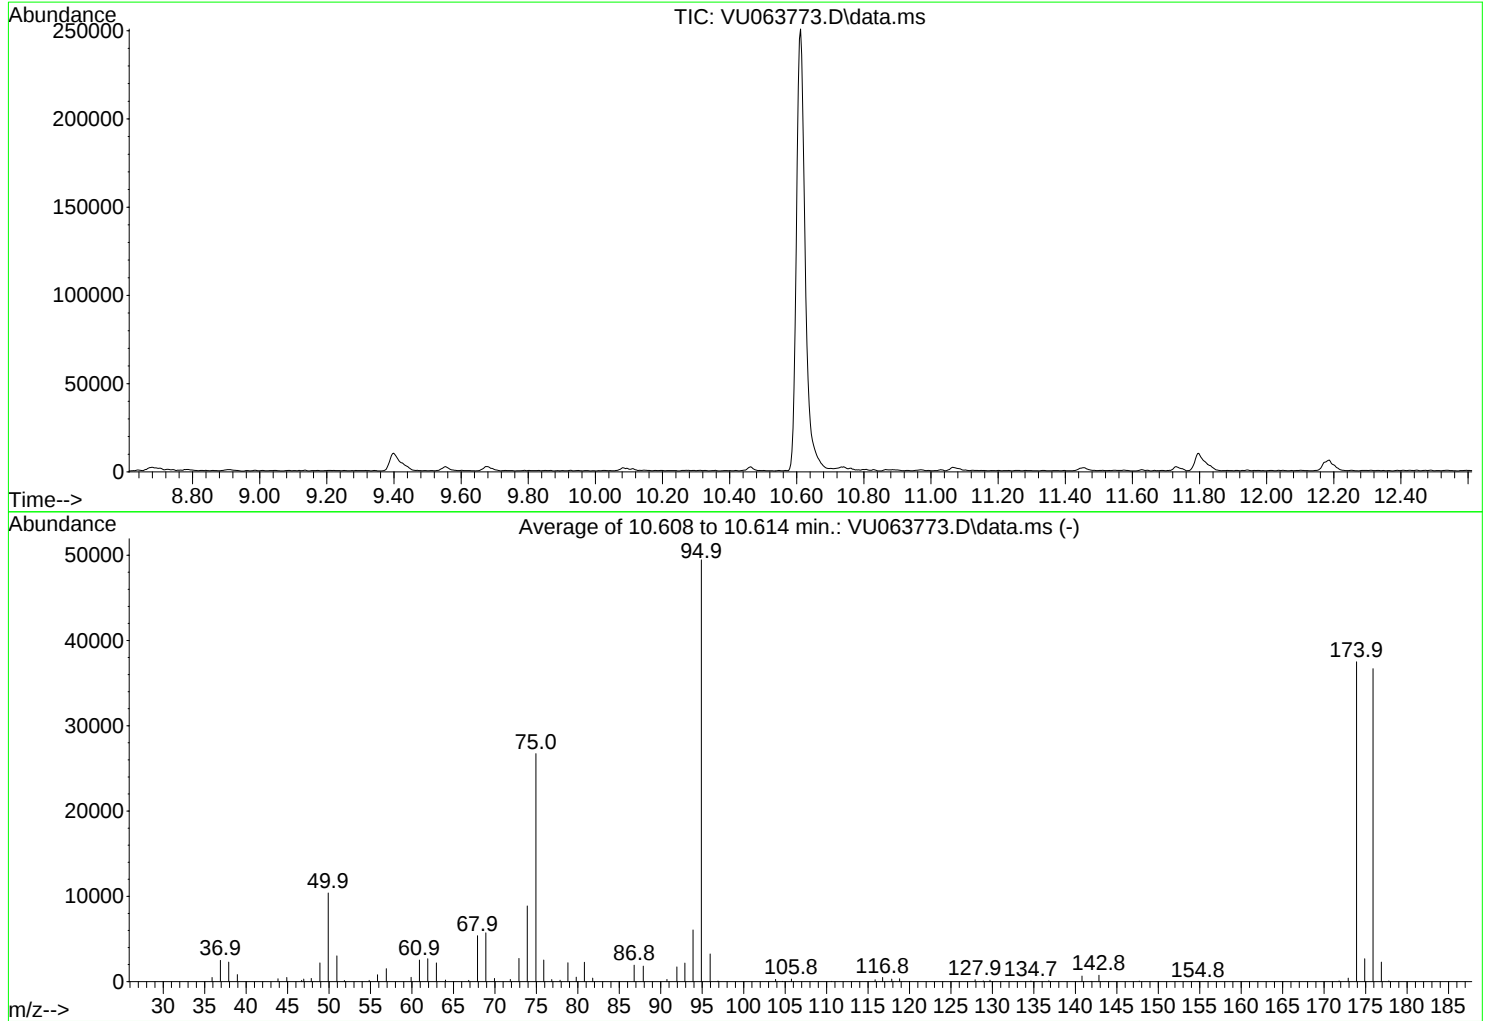

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2887

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.0	10395	PASS
75	95	30	80	54.1	26731	PASS
95	95	100	100	100.0	49453	PASS
96	95	5	9	6.6	3255	PASS
173	174	0.00	2	1.1	409	PASS
174	95	50	120	75.8	37496	PASS
175	174	5	9	7.2	2681	PASS
176	174	95	101	97.8	36688	PASS
177	176	5	9	6.3	2294	PASS

m/z	Abundance
39.90	222.0
43.80	490.0

Instrument :
MSVOA_U
ClientSampleId :
BFB093

m/z	Abundance
35.90	522.0
36.90	2600.0
37.90	2338.0
39.00	849.0
39.80	222.0
43.90	927.0
44.90	506.0
46.70	432.0
47.80	378.0
48.90	2264.0
49.90	10535.0
50.90	2995.0
51.90	145.0
54.90	167.0
55.80	837.0
56.90	1704.0
59.90	508.0
60.90	2607.0
61.90	2809.0
62.90	2250.0
64.00	231.0
66.90	159.0
67.90	5466.0
68.90	5701.0
70.00	310.0
71.80	280.0
72.90	2791.0
73.90	8729.0
74.90	26784.0
75.90	2527.0
77.00	249.0
77.80	178.0
78.80	2346.0
79.80	476.0
80.80	2220.0
81.80	474.0
86.80	1945.0
87.90	1653.0
90.70	274.0
91.90	1828.0
92.90	2222.0
93.90	6123.0
94.90	49464.0
95.90	3425.0
96.90	120.0
103.80	268.0
105.80	304.0
115.90	224.0
116.80	492.0
117.80	345.0
118.80	341.0
127.90	213.0
128.90	155.0
129.70	147.0
136.80	116.0
140.80	705.0
142.80	716.0
172.90	424.0
173.90	37344.0
174.90	2638.0
175.90	36576.0
176.90	2415.0
177.80	163.0

Instrument :
MSVOA_U
ClientSampleId :
BFB093

m/z	Abundance
35.90	496.0
36.90	2575.0
37.90	2319.0
38.90	830.0
39.80	213.0
43.90	849.0
44.90	493.0
46.90	463.0
47.80	381.0
48.90	2273.0
49.90	10609.0
50.90	3113.0
51.90	148.0
54.80	161.0
55.90	808.0
56.90	1527.0
59.90	515.0
60.90	2599.0
61.90	2779.0
62.90	2303.0
64.10	189.0
66.90	164.0
67.90	5519.0
68.90	5868.0
69.90	369.0
71.80	249.0
72.90	2807.0
73.90	9020.0
74.90	27424.0
75.90	2620.0
76.80	243.0
77.80	183.0
78.80	2275.0
79.80	517.0
80.80	2341.0
81.80	421.0
86.80	2035.0
87.90	1840.0
90.80	281.0
91.90	1763.0
92.90	2260.0
93.90	6264.0
94.90	50672.0
95.90	3346.0
96.90	115.0
103.90	266.0
104.70	105.0
105.80	307.0
110.60	103.0
115.90	223.0
116.70	504.0
117.90	320.0
118.80	344.0
127.90	230.0
128.90	136.0
129.70	180.0
134.70	107.0
136.80	130.0
140.80	672.0
142.90	794.0
147.70	100.0
171.80	128.0
172.90	415.0
173.90	38728.0
174.90	2763.0
175.90	37656.0
176.90	2330.0
177.80	125.0

Instrument :
MSVOA_U
ClientSampleId :
BFB093

m/z	Abundance
35.90	430.0
36.90	2338.0
37.90	2213.0
38.90	789.0
39.80	224.0
43.90	731.0
44.90	485.0
47.00	456.0
47.90	366.0
48.90	2069.0
49.90	10040.0
51.00	2932.0
51.80	131.0
54.80	155.0
55.90	750.0
56.90	1309.0
59.90	510.0
60.90	2394.0
61.90	2469.0
63.00	2011.0
64.10	161.0
66.70	156.0
67.90	5150.0
68.90	5582.0
69.90	443.0
71.90	284.0
72.90	2588.0
73.90	8868.0
75.00	25984.0
75.90	2439.0
76.80	266.0
77.90	176.0
78.80	2012.0
79.80	593.0
80.80	2225.0
81.80	347.0
86.80	1816.0
87.90	1974.0
90.80	242.0
92.00	1593.0
92.90	2028.0
93.90	5800.0
94.90	48224.0
96.00	2994.0
103.90	267.0
105.70	282.0
115.80	248.0
116.70	456.0
117.90	245.0
118.80	319.0
127.90	228.0
129.70	180.0
134.60	115.0
136.80	102.0
140.80	608.0
141.90	106.0
142.80	751.0
147.70	104.0
154.80	112.0
171.80	158.0
172.90	387.0
173.90	36416.0
174.90	2643.0
175.90	35832.0
176.90	2138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB093