

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U112519\
 Data File : VU035826.D
 Acq On : 25 Nov 2019 15:47
 Operator : JC/SP
 Sample : VU1125WBL01
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK13

Quant Time: Nov 26 01:12:24 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Nov 26 01:03:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	250535	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	284932	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	121569	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	144656	4.42	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	88.40%
7) Chloroethane-d5	1.93	69	140588	4.96	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	99.20%
11) 1,1-Dichloroethene-d2	2.59	63	188507	3.10	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.00%
20) 2-Butanone-d5	4.70	46	464112	61.28	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	122.56%
24) Chloroform-d	5.11	84	280927	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.40%
26) 1,2-Dichloroethane-d4	5.75	65	159011	5.11	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.20%
32) Benzene-d6	5.77	84	532948	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.00%
36) 1,2-Dichloropropane-d6	6.73	67	186127	5.08	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.60%
41) Toluene-d8	7.93	98	424995	4.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.80%
43) trans-1,3-Dichloropropene-	8.21	79	66972	4.69	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.80%
46) 2-Hexanone-d5	8.68	63	357885	62.47	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	124.94%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	160475	5.20	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	104.00%
64) 1,2-Dichlorobenzene-d4	12.22	152	148127	5.61	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	112.20%


Target Compounds				Ovalue
13) Acetone	2.69	43	13668	2.055 ug/L 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU112519\
Data File : VU035826.D
Acq On : 25 Nov 2019 15:47
Operator : JC/SP
Sample : VU1125WBL01
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK13

Quant Time: Nov 26 01:12:24 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 26 01:03:35 2019
Response via : Initial Calibration

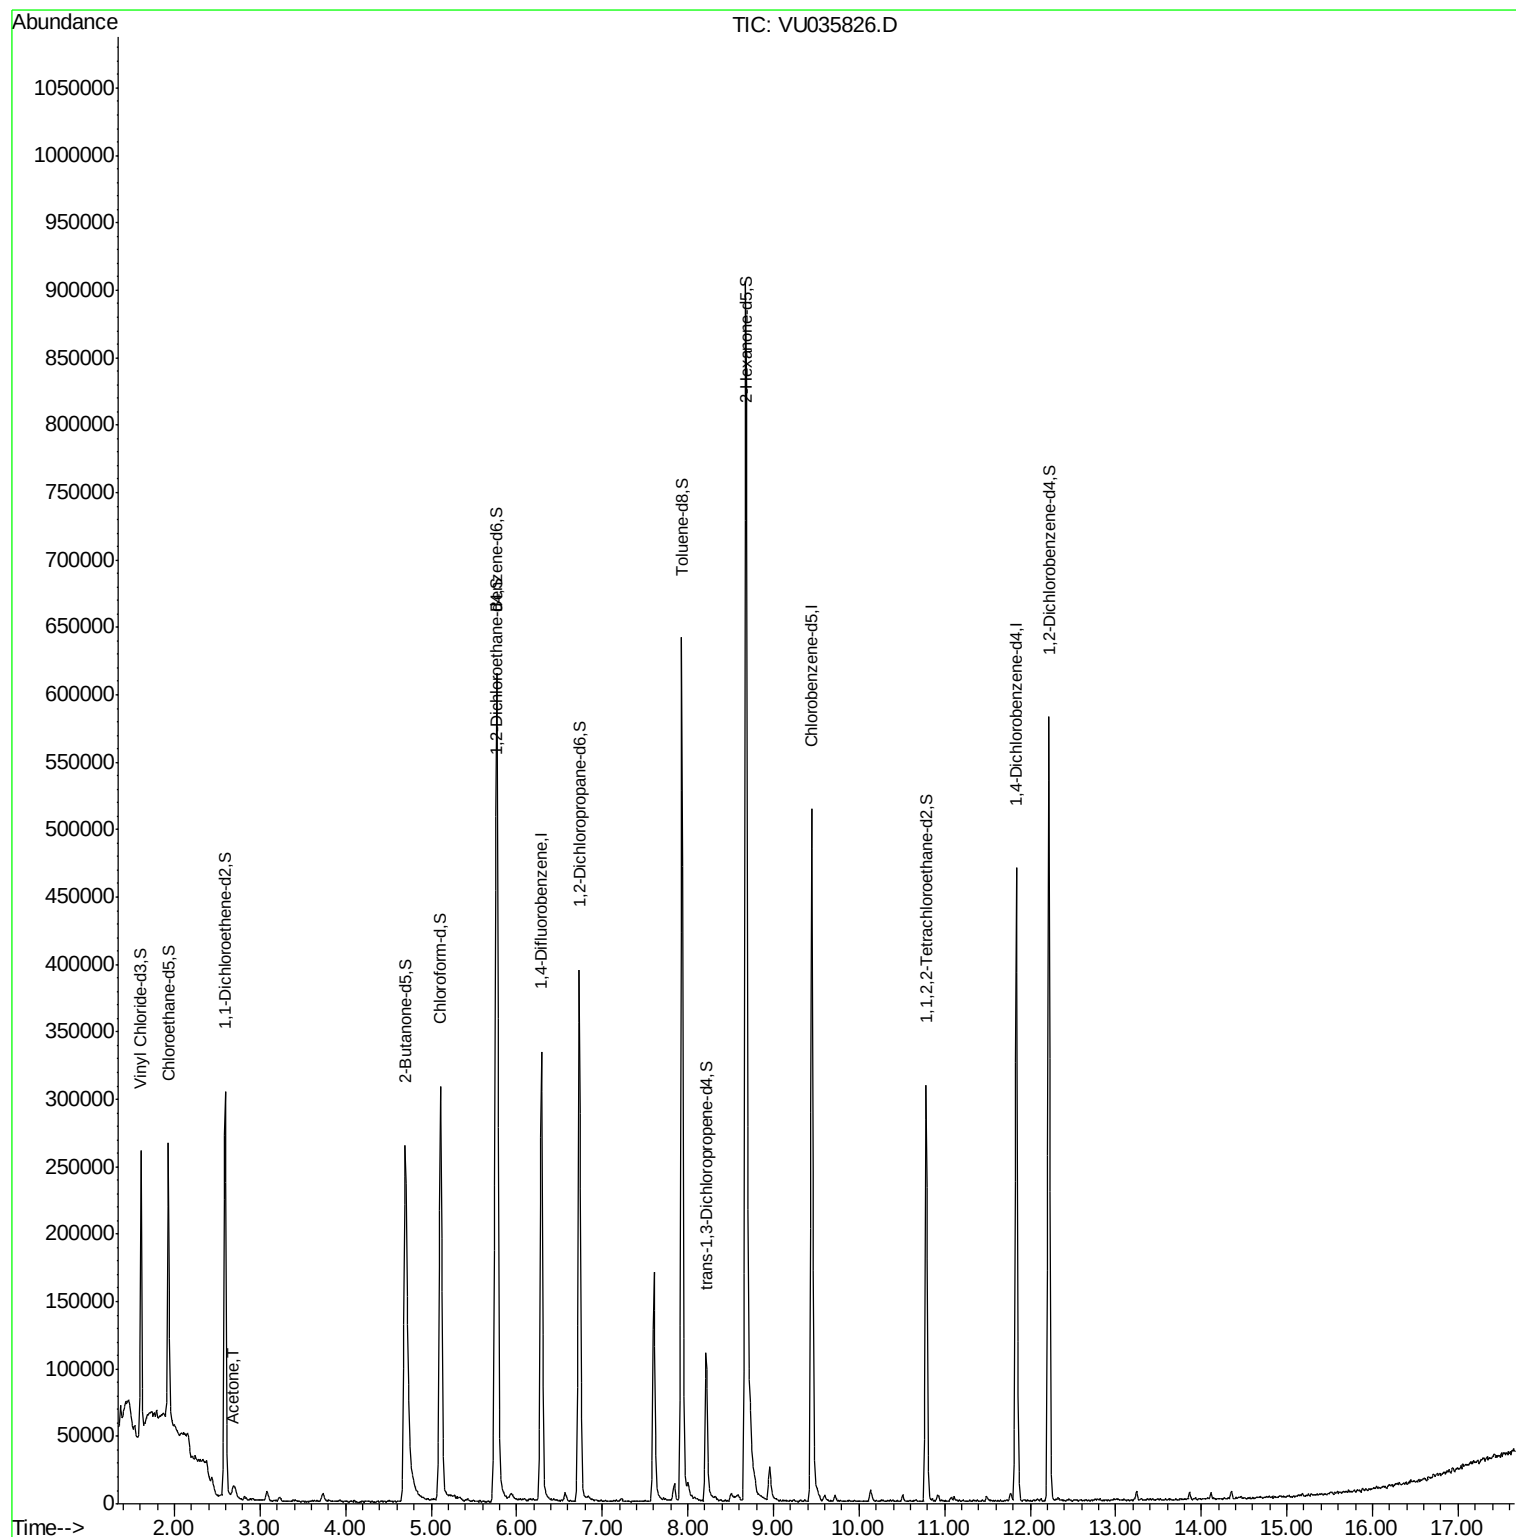

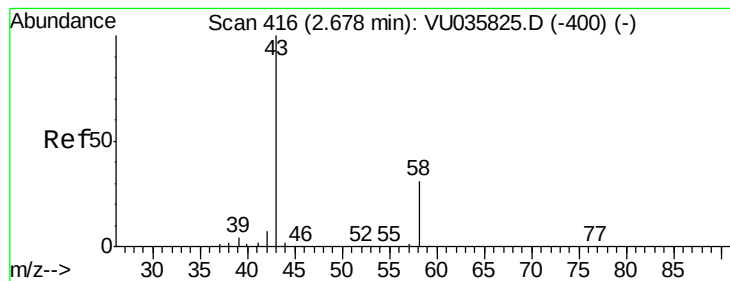

#13

Acetone

Concen: 2.055 ug/L

RT: 2.69 min Scan# 419

Delta R.T. 0.01 min

Lab File: VU035826.D

Acq: 25 Nov 2019 15:47

Instrument :

MSVOA_U

ClientSampleId :

VBLK13

Tot Ion: 43 Resp: 13668

Ion Ratio Lower Upper

43 100

58 34.6 0.0 61.2

