

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U112519\
 Data File : VU035828.D
 Acq On : 25 Nov 2019 16:55
 Operator : JC/SP
 Sample : K5992-15
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GARF6

Quant Time: Nov 26 01:29:05 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Nov 26 01:03:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	240809	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	275869	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	116401	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	131586	4.18	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.60%
7) Chloroethane-d5	1.93	69	128064	4.70	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.00%
11) 1,1-Dichloroethene-d2	2.59	63	169096	2.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	57.80%#
20) 2-Butanone-d5	4.70	46	414084	56.88	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.76%
24) Chloroform-d	5.11	84	258209	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.00%
26) 1,2-Dichloroethane-d4	5.75	65	142462	4.76	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.20%
32) Benzene-d6	5.77	84	487184	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.60%
36) 1,2-Dichloropropane-d6	6.73	67	171420	4.83	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.60%
41) Toluene-d8	7.93	98	385376	3.97	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	79.40%
43) trans-1,3-Dichloropropene-	8.21	79	60774	4.40	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	88.00%
46) 2-Hexanone-d5	8.68	63	322589	58.16	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	116.32%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	144143	4.83	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.60%
64) 1,2-Dichlorobenzene-d4	12.22	152	132327	5.23	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	104.60%

Target Compounds


					Ovalue
3) Chloromethane	1.54	50	5488	0.137 ug/L	87
13) Acetone	2.68	43	21478	3.359 ug/L	99
14) Carbon disulfide	2.82	76	7701	0.093 ug/L	96
16) Methylene chloride	3.08	84	3342	0.110 ug/L	99
25) Chloroform	5.13	83	26807	0.497 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU112519\
Data File : VU035828.D
Acq On : 25 Nov 2019 16:55
Operator : JC/SP
Sample : K5992-15
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GARF6

Quant Time: Nov 26 01:29:05 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 26 01:03:35 2019
Response via : Initial Calibration

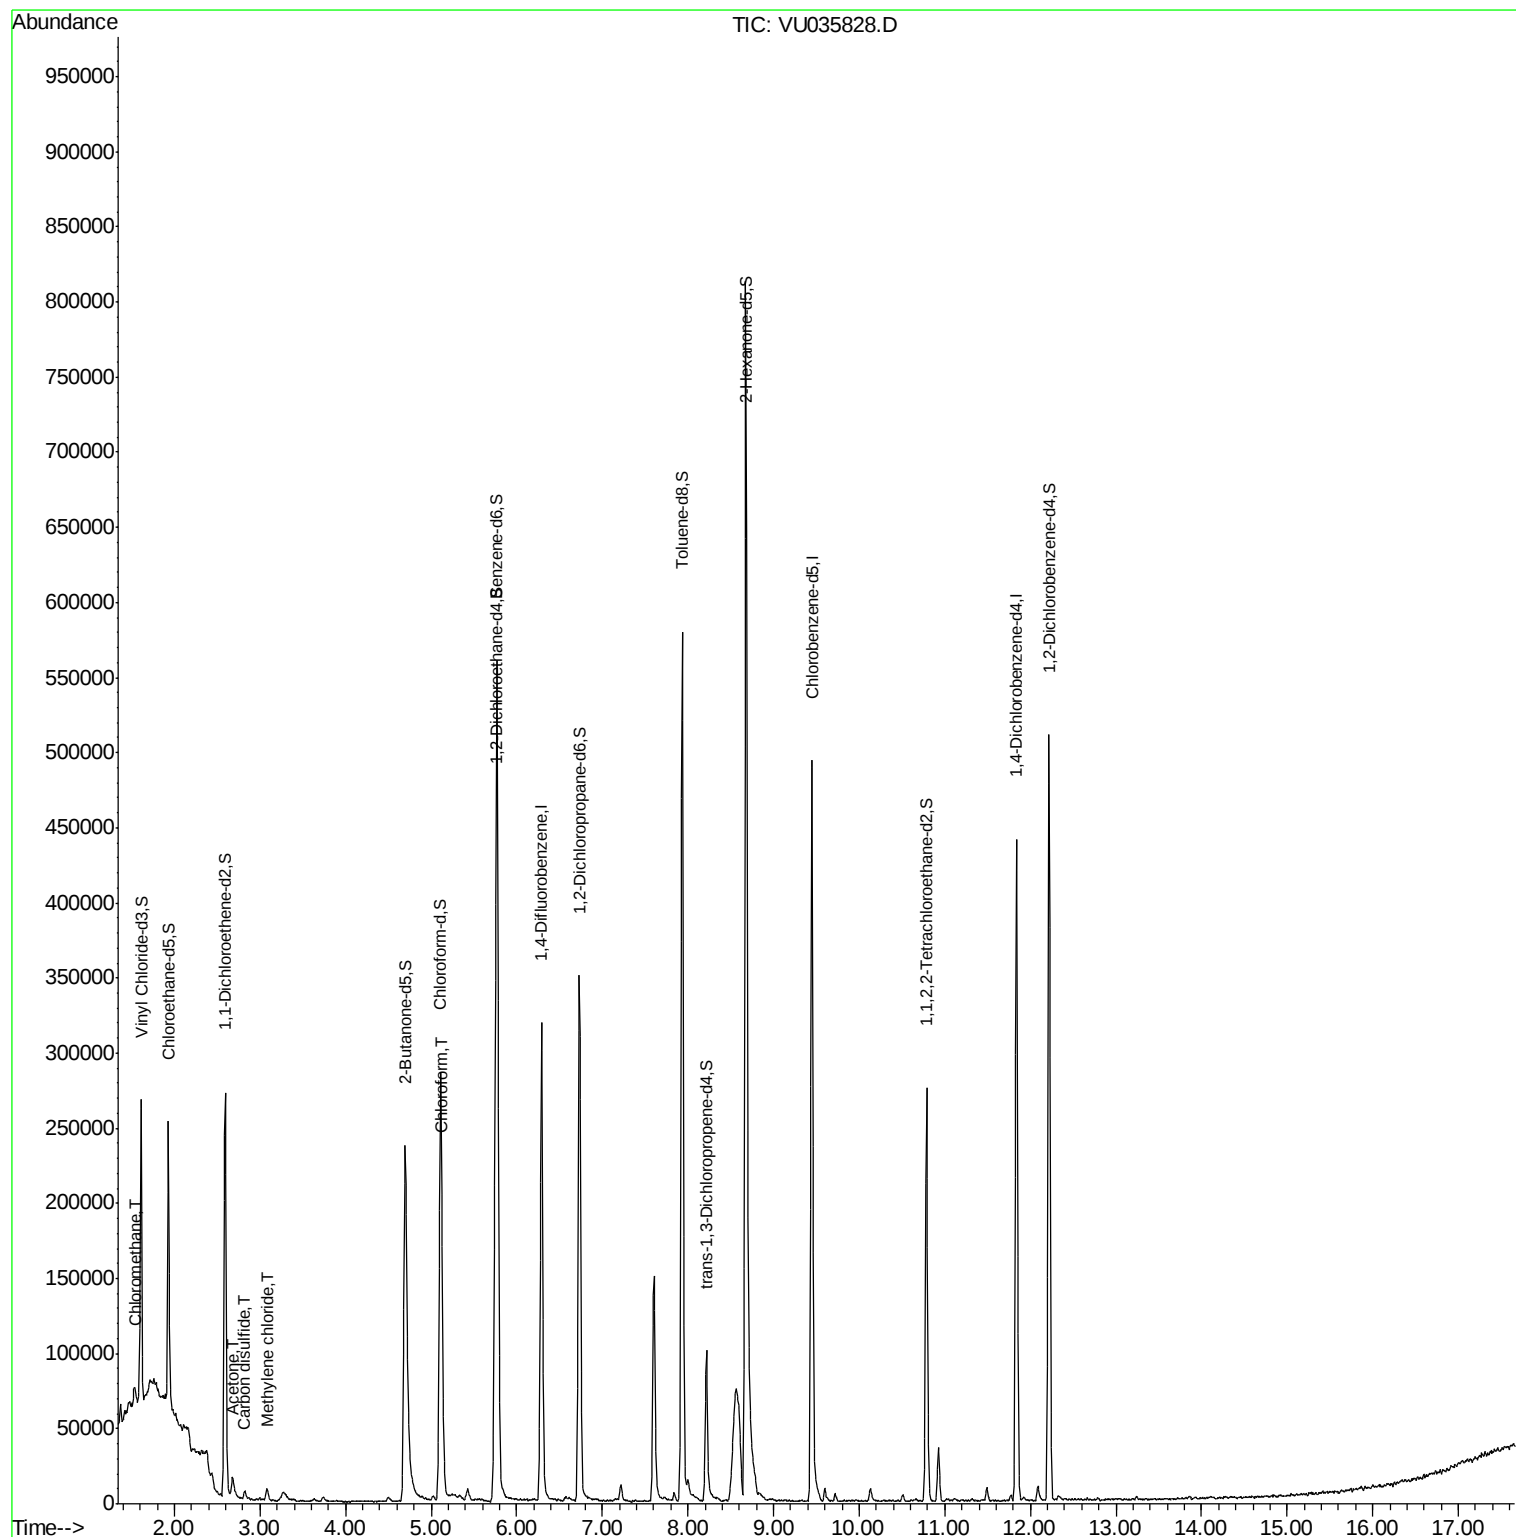

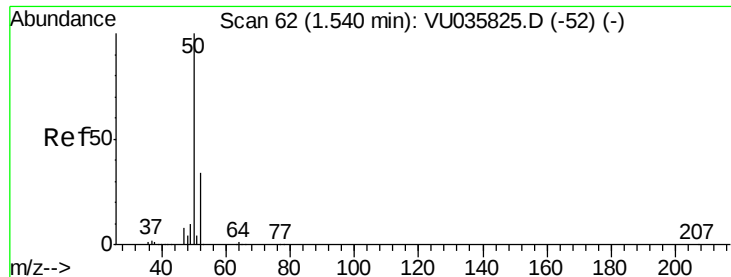

#3

Chloromethane

Concen: 0.137 ug/L

RT: 1.54 min Scan# 61

Delta R.T. -0.00 min

Lab File: VU035828.D

Acq: 25 Nov 2019 16:55

Instrument :

MSVOA_U

ClientSampleId :





GARF6

Tot Ion: 50 Resp: 5488

Ion Ratio Lower Upper

50 100

52 39.8 22.7 42.3

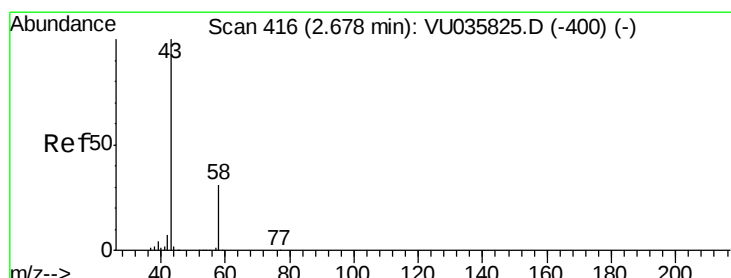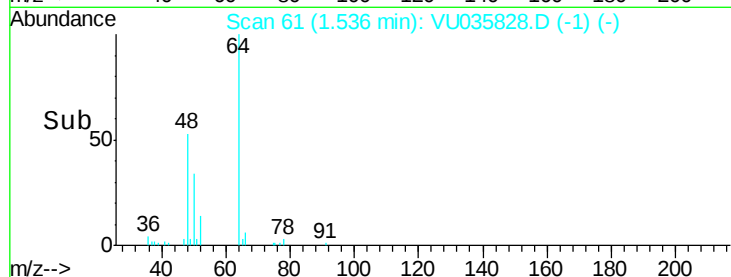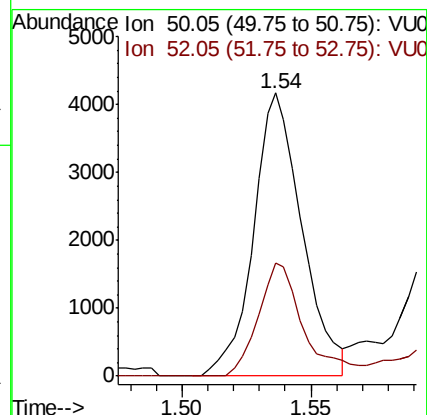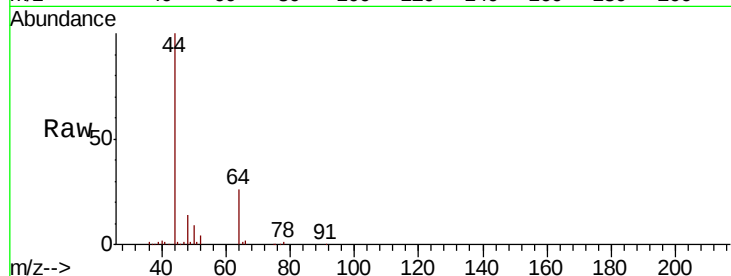

#13

Acetone

Concen: 3.359 ug/L

RT: 2.68 min Scan# 417

Delta R.T. 0.00 min

Lab File: VU035828.D




Acq: 25 Nov 2019 16:55


Tgt Ion: 43 Resp: 21478

Ion Ratio Lower Upper

43 100

58 30.3 0.0 61.2

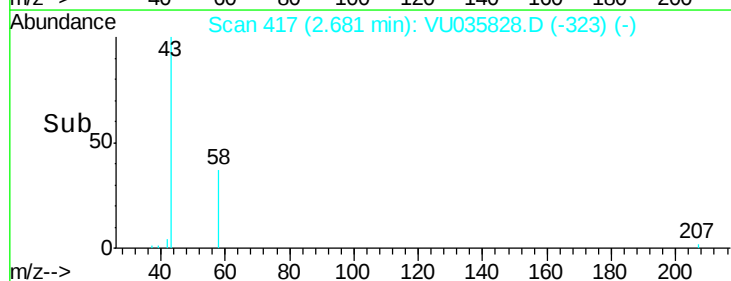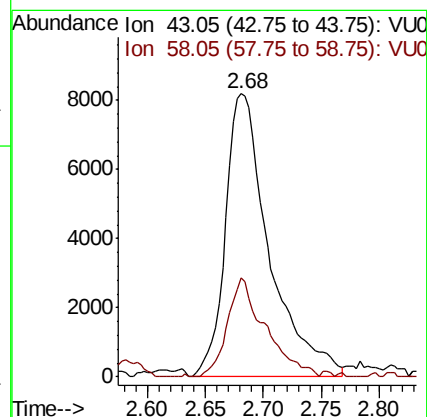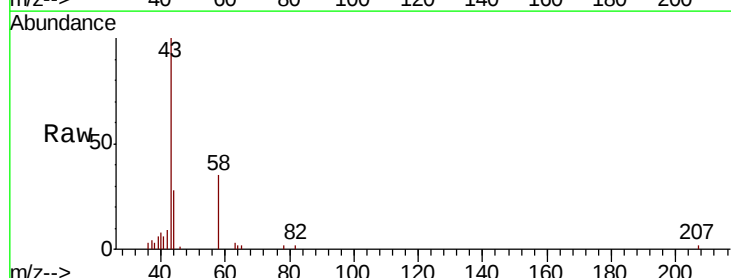

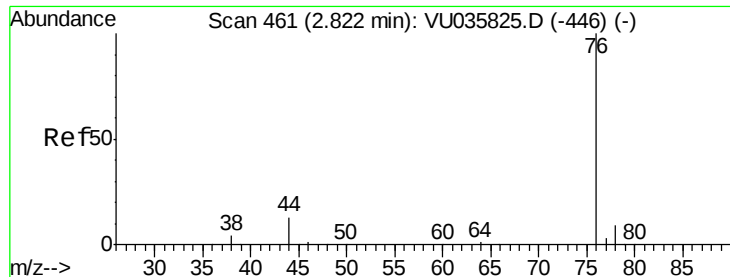

#14

Carbon disulfide

Concen: 0.093 ug/L

RT: 2.82 min Scan# 461

Delta R.T. 0.00 min

Lab File: VU035828.D

Acq: 25 Nov 2019 16:55

Instrument :

MSVOA_U

ClientSampleId :


GARF6

Tot Ion: 76 Resp: 7701

Ion Ratio Lower Upper




76 100

78 10.7 7.3 10.9

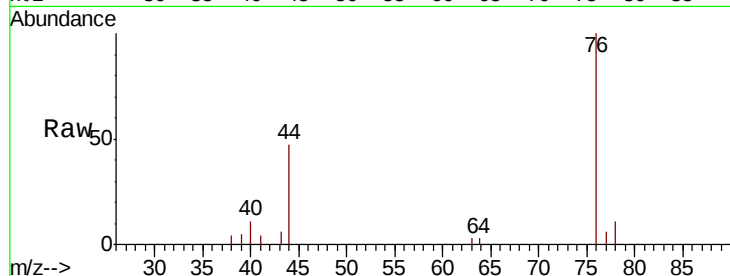

Abundance Ion 76.05 (75.75 to 76.75): VU035828.D (-446) (-)

Ion 78.00 (77.70 to 78.70): VU035828.D (-446) (-)

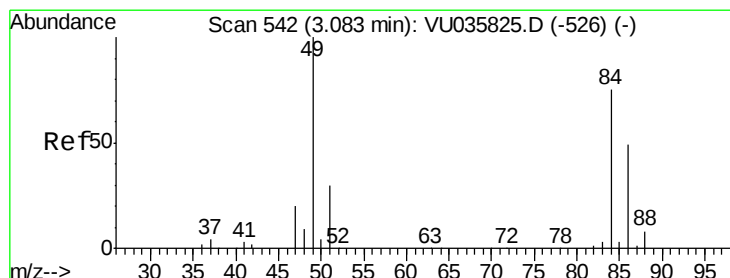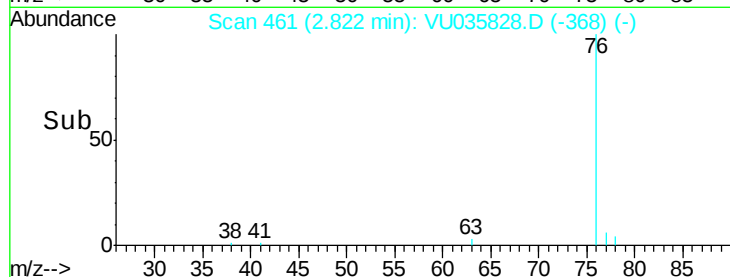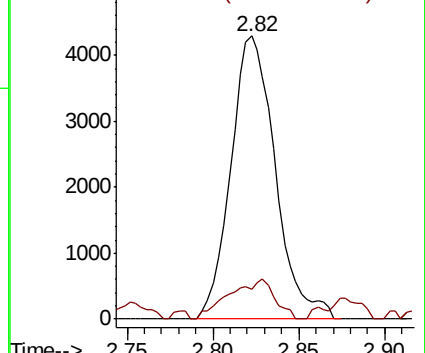

#16

Methylene chloride

Concen: 0.110 ug/L

RT: 3.08 min Scan# 540

Delta R.T. -0.01 min

Lab File: VU035828.D

Acq: 25 Nov 2019 16:55


Tgt Ion: 84 Resp: 3342

Ion Ratio Lower Upper

84 100

86 60.3 44.4 82.5



49 134.0 94.0 174.6

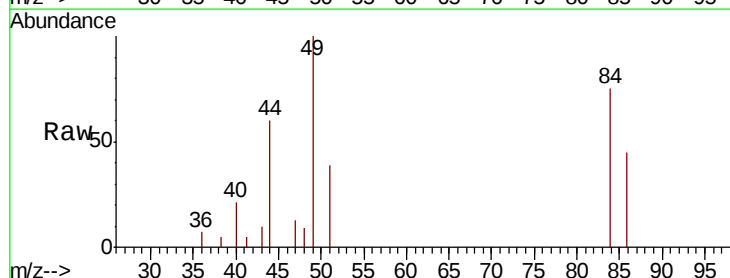


Abundance Ion 84.05 (83.75 to 84.75): VU035828.D (-449) (-)

Ion 86.00 (85.70 to 86.70): VU035828.D (-449) (-)

Ion 49.10 (48.80 to 49.80): VU035828.D (-449) (-)

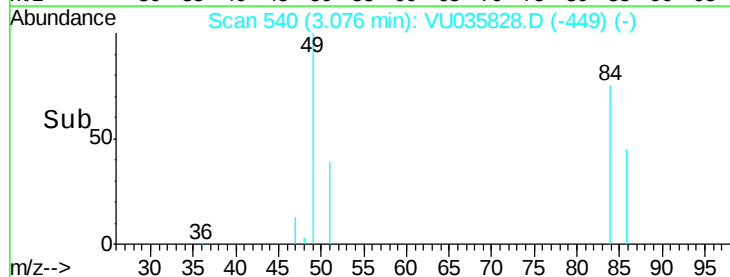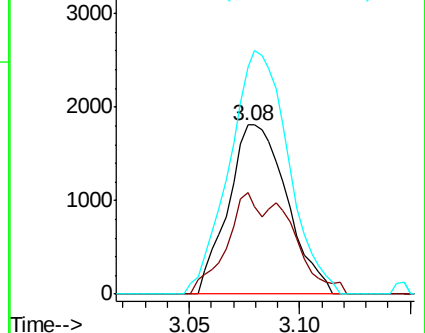

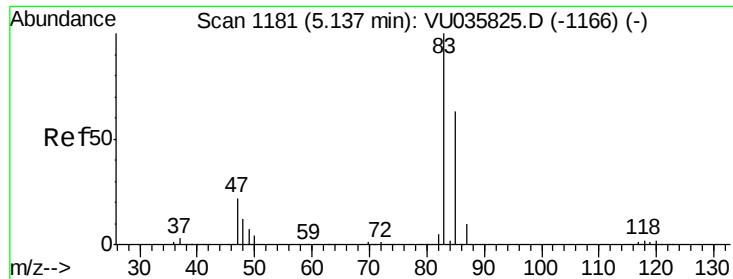

#25
 Chloroform
 Concen: 0.497 ug/L
 RT: 5.13 min Scan# 1180
 Delta R.T. -0.00 min
 Lab File: VU035828.D
 Acq: 25 Nov 2019 16:55

Instrument :
 MSVOA_U
 ClientSampleId :
 GARF6

Tot Ion: 83 Resp: 26807
 Ion Ratio Lower Upper
 83 100
 85 63.7 44.6 82.8

