

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U112519\
 Data File : VU035829.D
 Acq On : 25 Nov 2019 17:18
 Operator : JC/SP
 Sample : K5992-16
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GARF7

Quant Time: Nov 26 01:33:53 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Tue Nov 26 01:03:35 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	234574	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	268298	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	96789	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	127915	4.17	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.40%
7) Chloroethane-d5	1.93	69	124475	4.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.80%
11) 1,1-Dichloroethene-d2	2.59	63	167591	2.94	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.80%#
20) 2-Butanone-d5	4.69	46	442354	62.38	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	124.76%
24) Chloroform-d	5.11	84	253827	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.80%
26) 1,2-Dichloroethane-d4	5.75	65	152157	5.22	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.40%
32) Benzene-d6	5.77	84	480156	4.69	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	93.80%
36) 1,2-Dichloropropane-d6	6.74	67	171497	4.97	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.40%
41) Toluene-d8	7.93	98	384892	4.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.40%
43) trans-1,3-Dichloropropene-	8.21	79	61222	4.56	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	91.20%
46) 2-Hexanone-d5	8.68	63	349954	64.87	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	129.74%
57) 1,1,2,2-Tetrachloroethane-	10.79	84	153020	5.27	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	105.40%
64) 1,2-Dichlorobenzene-d4	12.22	152	111523	5.30	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.00%


Target Compounds					Ovalue
13) Acetone	2.67	43	18054	2.899 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU112519\
Data File : VU035829.D
Acq On : 25 Nov 2019 17:18
Operator : JC/SP
Sample : K5992-16
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GARF7

Quant Time: Nov 26 01:33:53 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 26 01:03:35 2019
Response via : Initial Calibration

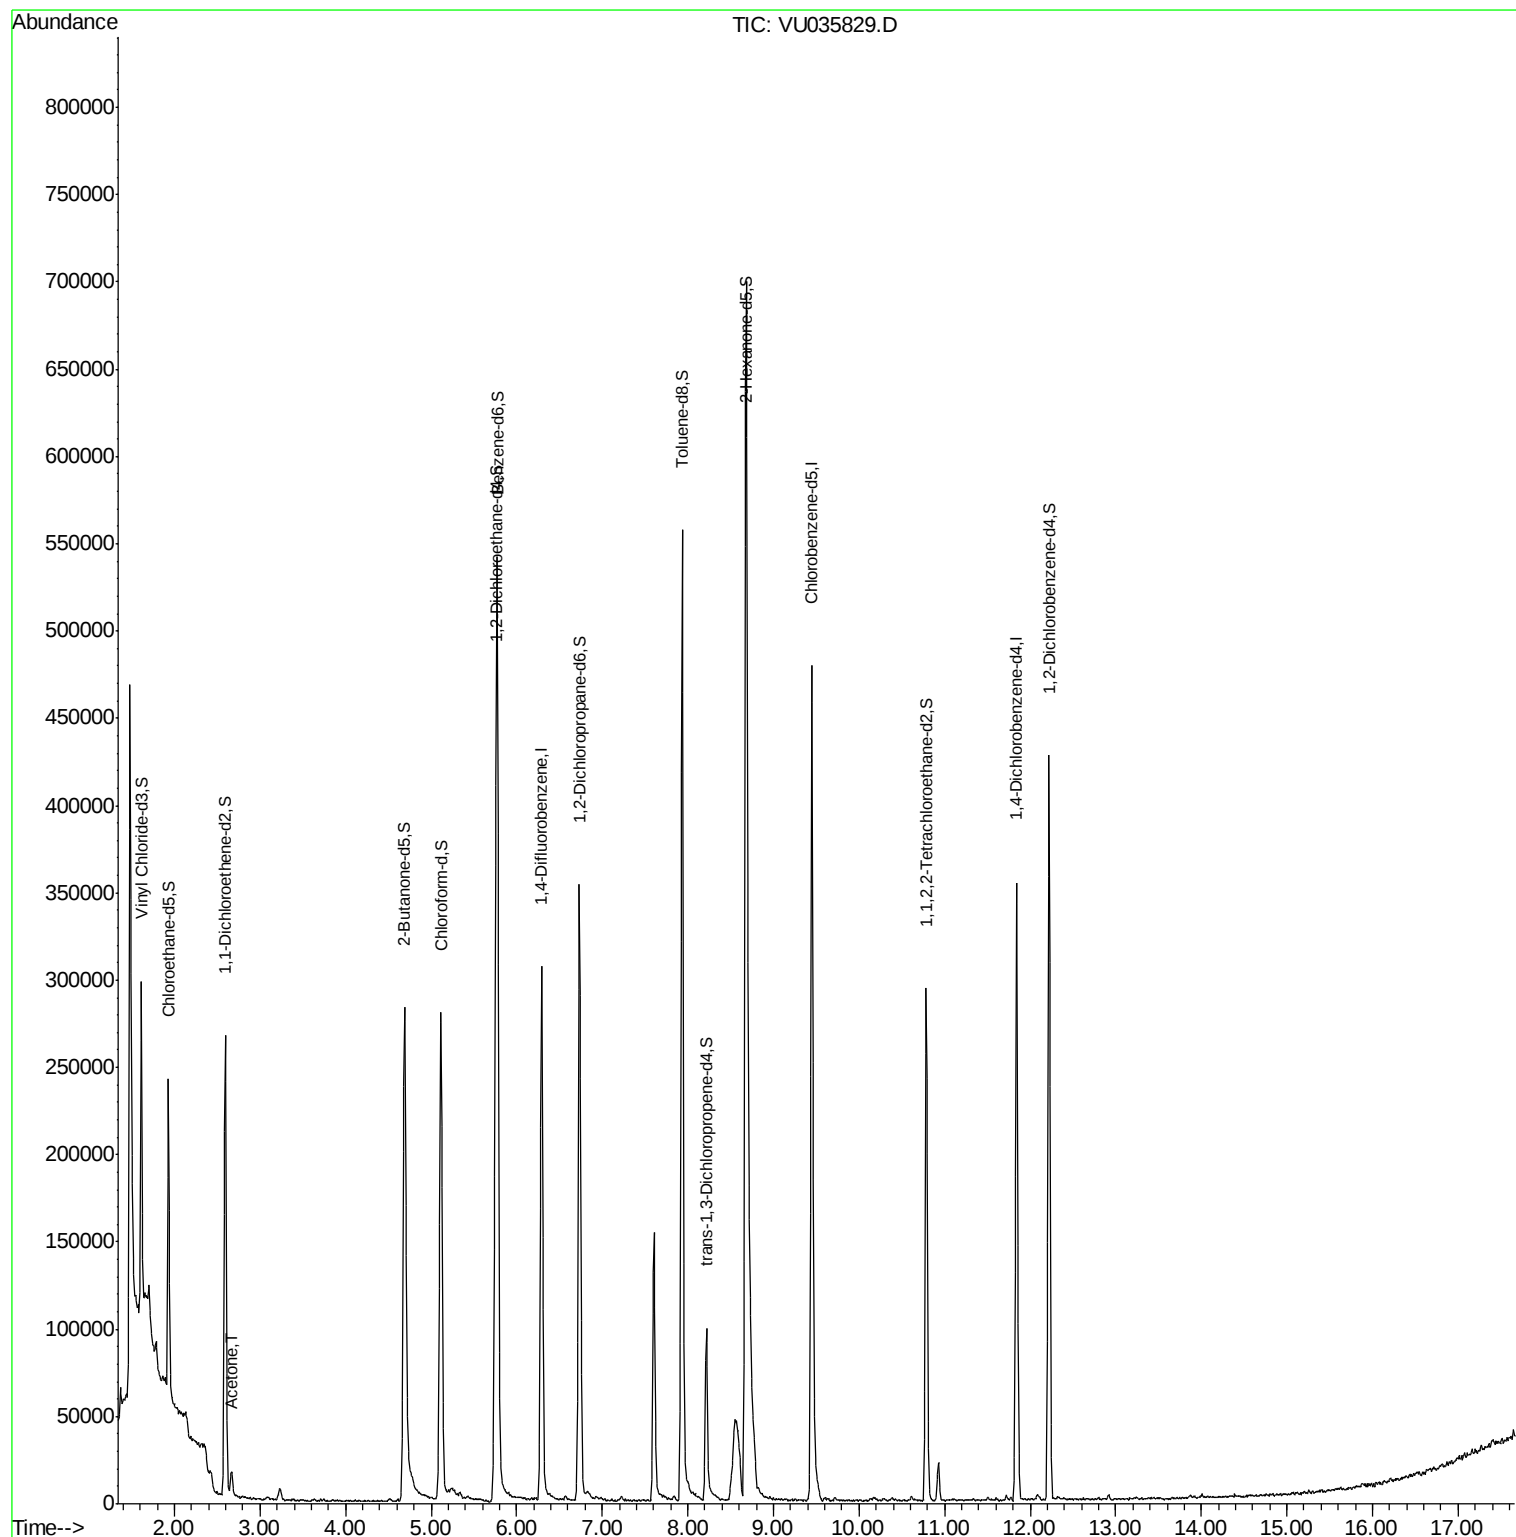

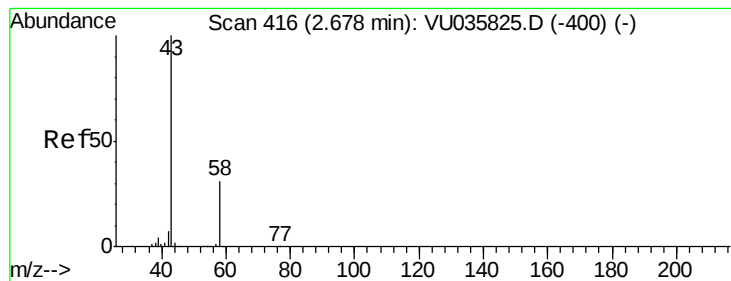

#13

Acetone

Concen: 2.899 ug/L

RT: 2.67 min Scan# 413

Delta R.T. -0.01 min

Lab File: VU035829.D

Acq: 25 Nov 2019 17:18

Instrument :

MSVOA_U

ClientSampleId :

GARF7

Tot Ion: 43 Resp: 18054

Ion Ratio Lower Upper

43 100

58 31.8 0.0 61.2

