


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU112519\
Data File : VU035824.D
Acq On : 25 Nov 2019 13:21
Operator : JC/SP
Sample : BFB05
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB05

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Nov 27 03:16:13 2019

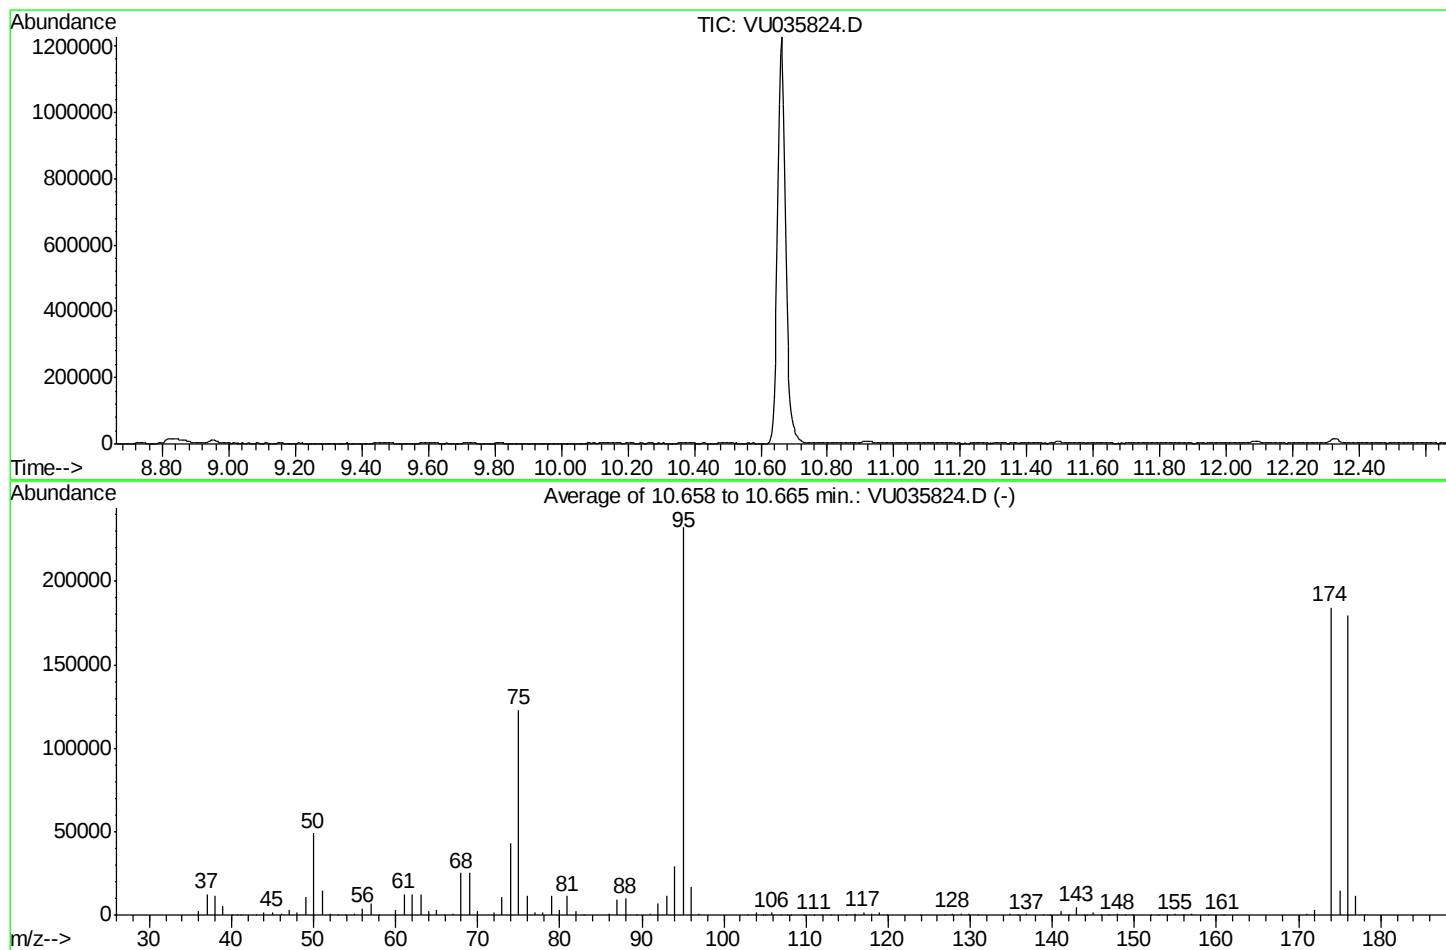

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	48901	PASS
75	95	30	80	53.0	123152	PASS
95	95	100	100	100.0	232362	PASS
96	95	5	9	7.2	16629	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.4	184533	PASS
175	174	5	9	7.8	14430	PASS
176	174	95	101	97.5	179840	PASS
177	176	5	9	6.4	11513	PASS

m/z	Abundance
36.00	2353.0
37.00	12385.0
38.10	11835.0
39.00	5028.0
40.00	747.0
40.70	315.0
41.20	211.0
43.00	220.0
44.00	2743.0
45.00	1752.0
46.00	435.0
47.00	3074.0
48.00	1576.0
49.00	10654.0
50.00	48904.0
51.10	14769.0
52.10	861.0
53.00	405.0
54.00	324.0
55.10	573.0
56.00	3895.0
57.00	6905.0
58.00	330.0
60.00	2860.0
61.00	12460.0
62.00	13318.0
63.00	12435.0
64.10	2448.0
65.10	3112.0
66.00	322.0
67.10	612.0
68.00	25000.0
69.00	25072.0
70.00	1806.0
72.10	1296.0
73.00	10673.0
74.10	43072.0
75.00	122600.0
76.00	11176.0
77.10	1679.0
77.90	1141.0
78.90	11772.0
80.00	3283.0
81.00	11198.0
82.00	2762.0
85.90	636.0
87.00	9339.0
88.00	9885.0
91.00	1086.0
92.00	7455.0
93.00	11065.0
94.00	28712.0
95.10	230592.0
96.00	16440.0
97.00	545.0
103.90	1330.0
105.00	321.0
105.90	1427.0
106.90	251.0
107.70	107.0
109.80	178.0
111.00	241.0
111.90	199.0
113.00	199.0
114.90	212.0
115.90	875.0
117.00	1741.0
118.00	921.0
118.90	1843.0
123.90	189.0
127.90	731.0
128.90	492.0
129.80	779.0
130.90	295.0
134.90	480.0
135.70	106.0
136.90	484.0
138.80	118.0
139.70	102.0
141.00	2479.0
142.00	333.0
142.90	5103.0
144.10	366.0
145.00	1763.0
145.90	330.0
146.80	137.0
147.90	469.0
148.80	191.0
149.80	295.0
151.90	110.0
152.90	172.0
153.90	167.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

155.00	575.0
156.10	163.0
156.90	589.0
159.00	244.0
160.90	335.0
170.90	981.0
172.00	2924.0
173.90	178944.0
175.00	14350.0
176.00	172544.0
176.90	11524.0
178.00	278.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
36.00	2511.0
37.00	12735.0
38.10	12065.0
39.00	5309.0
40.00	706.0
40.60	273.0
41.10	166.0
42.80	195.0
43.10	190.0
44.00	2543.0
45.00	1840.0
46.10	443.0
47.10	3433.0
48.00	1749.0
49.00	10935.0
50.00	50480.0
51.10	15127.0
52.10	927.0
52.90	389.0
54.00	360.0
55.10	638.0
56.00	4120.0
57.00	7092.0
58.00	427.0
60.00	2823.0
61.00	12655.0
62.00	12771.0
63.10	12892.0
64.00	2553.0
65.10	3269.0
65.90	403.0
67.00	669.0
68.00	26088.0
69.00	25784.0
70.00	2068.0
72.10	1301.0
73.00	10993.0
74.10	43672.0
75.00	127032.0
76.00	11520.0
77.10	1788.0
78.00	1370.0
78.90	11577.0
80.00	3343.0
80.90	11582.0
82.00	2834.0
82.90	135.0
85.90	602.0
87.00	9703.0
88.00	9897.0
89.30	100.0
91.00	1012.0
92.00	7216.0
93.10	11758.0
94.00	30360.0
95.10	239424.0
96.00	17248.0
97.00	452.0
102.80	118.0
103.90	1322.0
105.10	354.0
105.90	1529.0
106.90	242.0
107.60	172.0
109.80	159.0
111.00	326.0
111.90	170.0
113.00	198.0
114.80	220.0
116.00	879.0
117.00	1974.0
118.00	909.0
119.00	1979.0
119.80	111.0
123.80	228.0
126.90	146.0
127.80	862.0
128.90	503.0
129.80	869.0
131.00	323.0
134.90	478.0
135.70	128.0
136.90	625.0
138.90	123.0
141.00	2359.0
143.00	4923.0
144.20	352.0
145.00	1777.0
146.00	294.0
146.90	206.0
148.00	527.0
148.80	157.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

149.90	290.0
152.90	239.0
154.00	111.0
155.00	705.0
155.80	128.0
156.90	574.0
159.00	212.0
160.80	383.0
171.00	934.0
172.00	3352.0
174.00	190656.0
175.00	14823.0
176.00	185344.0
176.90	11752.0
178.00	384.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

m/z	Abundance
36.00	2339.0
37.00	12067.0
38.00	11180.0
39.00	5047.0
40.00	666.0
41.10	123.0
43.10	212.0
44.00	2380.0
45.00	1850.0
46.10	507.0
47.00	3262.0
48.00	1697.0
49.00	10136.0
50.00	47320.0
51.00	14536.0
52.10	888.0
52.90	413.0
53.90	364.0
55.00	741.0
56.00	3884.0
57.10	6603.0
58.00	446.0
60.00	2571.0
61.00	12493.0
62.00	11304.0
63.10	11745.0
64.00	2560.0
65.00	3147.0
65.90	395.0
67.00	719.0
68.00	24720.0
69.00	24104.0
70.00	2108.0
72.00	1378.0
73.00	10435.0
74.00	41792.0
75.00	119824.0
76.00	10996.0
77.00	1726.0
78.00	1383.0
79.00	10279.0
80.00	3109.0
80.90	10780.0
82.00	2532.0
83.00	241.0
86.00	562.0
87.00	9504.0
88.00	9568.0
89.30	118.0
90.90	910.0
92.00	6498.0
93.10	11047.0
94.00	29000.0
95.10	227072.0
96.00	16200.0
97.00	357.0
102.80	115.0
103.90	1211.0
104.80	341.0
105.90	1315.0
106.90	219.0
107.60	184.0
108.10	111.0
109.80	130.0
111.00	294.0
111.90	120.0
113.10	145.0
114.90	209.0
116.00	847.0
117.00	2031.0
117.90	886.0
119.00	1895.0
119.80	130.0
123.80	183.0
126.90	196.0
127.90	903.0
128.90	449.0
129.80	786.0
131.00	348.0
134.90	497.0
136.90	651.0
138.90	114.0
141.00	2024.0
143.00	4435.0
143.90	297.0
145.00	1786.0
146.00	233.0
146.90	235.0
147.90	539.0
148.90	100.0
149.90	196.0
152.80	260.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

155.00	688.0
155.80	135.0
156.90	473.0
159.00	217.0
160.80	329.0
171.00	883.0
172.00	3289.0
174.00	184000.0
175.00	14118.0
176.00	181632.0
177.00	11263.0
178.00	375.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05

Scan 2883 (10.610 min): VU035824.D
BFB05

m/z	Abundance
40.00	496.0
40.90	140.0
42.00	146.0
44.00	1116.0

Instrument :
MSVOA_U
ClientSampleId :
BFB05