

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112522\
 Data File : VU052134.D
 Acq On : 25 Nov 2022 11:12
 Operator : JC/MD
 Sample : VU1125WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK032

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

Signal : TIC: VU052134.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	35	42	51	rBV2	10301	20647	1.18%	0.163%
2	1.601	73	81	103	rVB	258823	302715	17.31%	2.384%
3	1.906	167	176	200	rVB	176159	265674	15.19%	2.093%
4	2.565	368	381	398	rBV	382855	630468	36.04%	4.966%
5	2.793	445	452	459	rVB3	948	1353	0.08%	0.011%
6	2.967	504	506	509	rVB2	395	209	0.01%	0.002%
7	2.986	509	512	514	rBV2	296	233	0.01%	0.002%
8	3.044	521	530	539	rBV4	3176	5981	0.34%	0.047%
9	3.134	554	558	561	rBV2	353	266	0.02%	0.002%
10	3.176	563	571	573	rBV3	1376	1828	0.10%	0.014%
11	3.318	612	615	619	rBV3	315	246	0.01%	0.002%
12	3.395	634	639	642	rBV2	245	227	0.01%	0.002%
13	3.433	647	651	654	rVB2	488	307	0.02%	0.002%
14	3.456	654	658	661	rBV3	240	213	0.01%	0.002%
15	3.774	753	757	758	rBV2	501	326	0.02%	0.003%
16	3.883	786	791	797	rVV2	267	351	0.02%	0.003%
17	4.147	869	873	877	rBV2	218	230	0.01%	0.002%
18	4.276	910	913	917	rBV2	328	245	0.01%	0.002%
19	4.533	989	993	1000	rVB	380	399	0.02%	0.003%
20	4.565	1000	1003	1008	rVB2	326	270	0.02%	0.002%
21	4.617	1008	1019	1057	rBV	148732	366831	20.97%	2.889%
22	4.842	1086	1089	1092	rBV2	321	210	0.01%	0.002%
23	5.060	1139	1157	1193	rBV	313242	687483	39.30%	5.415%
24	5.285	1222	1227	1232	rBV5	1080	1270	0.07%	0.010%
25	5.372	1252	1254	1263	rVB3	636	628	0.04%	0.005%
26	5.555	1308	1311	1317	rVB2	352	294	0.02%	0.002%
27	5.588	1317	1321	1322	rBV	323	211	0.01%	0.002%
28	5.636	1330	1336	1340	rBV	376	357	0.02%	0.003%
29	5.723	1340	1363	1387	rBV2	652059	1749199	100.00%	13.778%
30	6.047	1460	1464	1471	rVV3	381	460	0.03%	0.004%
31	6.128	1481	1489	1494	rVB4	639	925	0.05%	0.007%
32	6.247	1512	1526	1561	rBV	530407	1016805	58.13%	8.009%
33	6.481	1596	1599	1602	rBV3	317	220	0.01%	0.002%
34	6.520	1606	1611	1613	rBV5	1639	1348	0.08%	0.011%
35	6.616	1638	1641	1645	rVB2	287	212	0.01%	0.002%
36	6.687	1649	1663	1692	rBV	402171	792577	45.31%	6.243%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112522\
 Data File : VU052134.D
 Acq On : 25 Nov 2022 11:12
 Operator : JC/MD
 Sample : VU1125WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK032

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

37	6.787	1692	1694	1696	rVV3	1074	653	0.04%	0.005%
38	6.806	1698	1700	1708	rVB6	1151	1036	0.06%	0.008%
39	6.993	1753	1758	1759	rBV2	286	215	0.01%	0.002%
40	7.417	1884	1890	1893	rBV	320	253	0.01%	0.002%
41	7.504	1911	1917	1923	rBV2	282	305	0.02%	0.002%
42	7.562	1923	1935	1962	rBV	196408	345878	19.77%	2.724%
43	7.655	1962	1964	1968	rVV3	478	297	0.02%	0.002%
44	7.681	1969	1972	1975	rVV3	454	304	0.02%	0.002%
45	7.706	1975	1980	1984	rVB4	499	415	0.02%	0.003%
46	7.739	1987	1990	1995	rVB2	370	293	0.02%	0.002%
47	7.793	2001	2007	2015	rVB4	966	1371	0.08%	0.011%
48	7.835	2015	2020	2022	rBV2	363	308	0.02%	0.002%
49	7.896	2025	2039	2077	rBV	747980	1296435	74.12%	10.211%
50	8.176	2115	2126	2152	rVV	137335	233703	13.36%	1.841%
51	8.308	2165	2167	2172	rBV4	299	258	0.01%	0.002%
52	8.359	2180	2183	2185	rBV2	336	210	0.01%	0.002%
53	8.465	2211	2216	2220	rBV2	543	637	0.04%	0.005%
54	8.552	2240	2243	2249	rBV4	577	438	0.03%	0.003%
55	8.632	2255	2268	2295	rBV	430886	802393	45.87%	6.320%
56	8.874	2340	2343	2346	rBV2	422	241	0.01%	0.002%
57	8.922	2352	2358	2361	rBV3	1141	1103	0.06%	0.009%
58	9.044	2394	2396	2400	rBV2	279	212	0.01%	0.002%
59	9.414	2498	2511	2541	rBV	767724	1268969	72.55%	9.995%
60	9.642	2580	2582	2588	rBV2	227	219	0.01%	0.002%
61	9.713	2602	2604	2607	rVB	382	214	0.01%	0.002%
62	9.848	2643	2646	2652	rBV2	348	323	0.02%	0.003%
63	10.031	2700	2703	2707	rVB2	304	216	0.01%	0.002%
64	10.099	2719	2724	2726	rBV2	463	444	0.03%	0.003%
65	10.147	2736	2739	2744	rVB3	415	382	0.02%	0.003%
66	10.301	2783	2787	2789	rBV2	269	227	0.01%	0.002%
67	10.346	2797	2801	2804	rVB3	308	233	0.01%	0.002%
68	10.443	2827	2831	2834	rBV2	242	228	0.01%	0.002%
69	10.465	2834	2838	2843	rVV3	494	592	0.03%	0.005%
70	10.491	2844	2846	2851	rVB2	578	322	0.02%	0.003%
71	10.597	2875	2879	2882	rBV	217	216	0.01%	0.002%
72	10.639	2885	2892	2900	rBV3	2233	3645	0.21%	0.029%
73	10.703	2908	2912	2915	rBV2	349	221	0.01%	0.002%
74	10.755	2915	2928	2951	rBV	574593	932921	53.33%	7.348%
75	10.922	2978	2980	2983	rVB2	475	263	0.02%	0.002%
76	11.095	3031	3034	3041	rVB2	661	622	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112522\
 Data File : VU052134.D
 Acq On : 25 Nov 2022 11:12
 Operator : JC/MD
 Sample : VU1125WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK032

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

77	11.468	3143	3150	3158	rVB4	670	1103	0.06%	0.009%
78	11.748	3229	3237	3244	rBV4	1222	1814	0.10%	0.014%
79	11.809	3244	3256	3282	rBV	567214	917510	52.45%	7.227%
80	12.002	3313	3316	3320	rVB3	386	303	0.02%	0.002%
81	12.034	3324	3326	3328	rBV2	297	209	0.01%	0.002%
82	12.099	3343	3346	3348	rBV2	358	250	0.01%	0.002%
83	12.134	3354	3357	3361	rBV2	439	333	0.02%	0.003%
84	12.192	3361	3375	3398	rBV	601733	995336	56.90%	7.840%
85	12.549	3484	3486	3493	rBV2	395	409	0.02%	0.003%
86	12.684	3525	3528	3533	rBV2	348	299	0.02%	0.002%
87	12.742	3543	3546	3549	rBV2	468	218	0.01%	0.002%
88	12.996	3623	3625	3628	rBV2	502	361	0.02%	0.003%
89	13.053	3640	3643	3646	rVB	354	239	0.01%	0.002%
90	13.073	3646	3649	3652	rBV	294	229	0.01%	0.002%
91	13.227	3688	3697	3706	rBV6	1857	3308	0.19%	0.026%
92	13.324	3724	3727	3732	rBV2	355	311	0.02%	0.002%
93	13.381	3742	3745	3750	rBV3	569	499	0.03%	0.004%
94	13.844	3882	3889	3906	rBV5	3639	6559	0.37%	0.052%
95	13.976	3927	3930	3937	rBV3	501	560	0.03%	0.004%
96	14.092	3959	3966	3975	rBV	5081	8331	0.48%	0.066%
97	14.182	3992	3994	3998	rBV3	417	319	0.02%	0.003%
98	14.330	4033	4040	4054	rVB5	4331	7476	0.43%	0.059%
99	14.574	4112	4116	4125	rVB5	728	1021	0.06%	0.008%
100	15.147	4291	4294	4297	rVB	805	469	0.03%	0.004%




Sum of corrected areas: 12695899

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112522\
Data File : VU052134.D
Acq On : 25 Nov 2022 11:12
Operator : JC/MD
Sample : VU1125WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK032

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

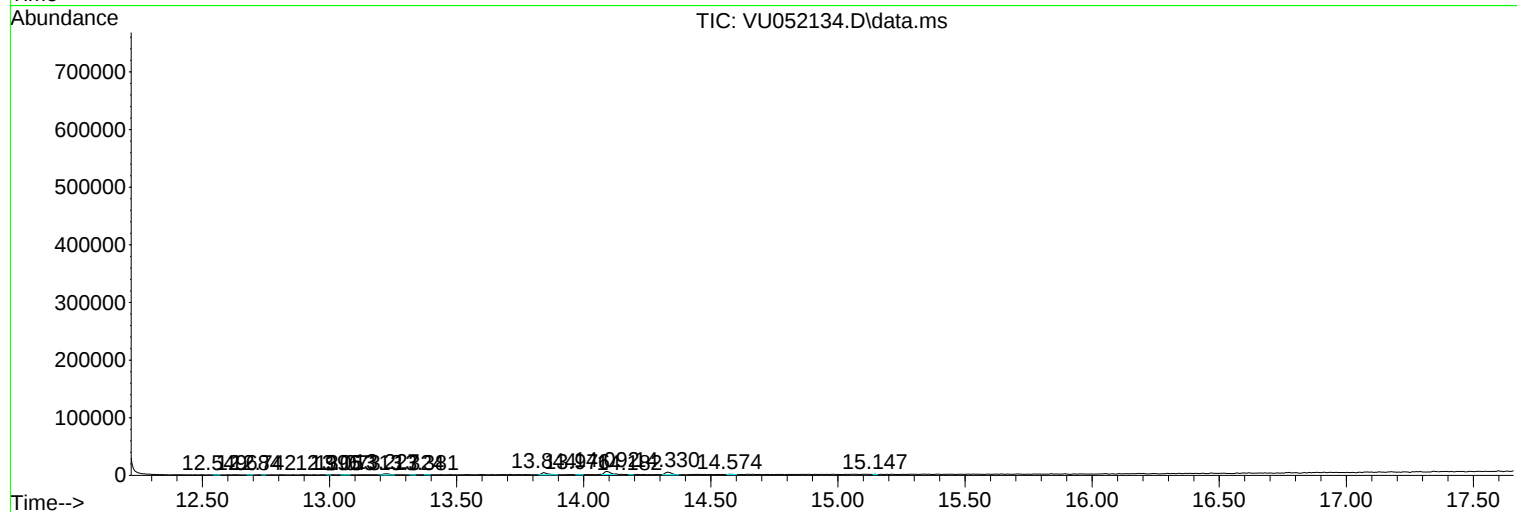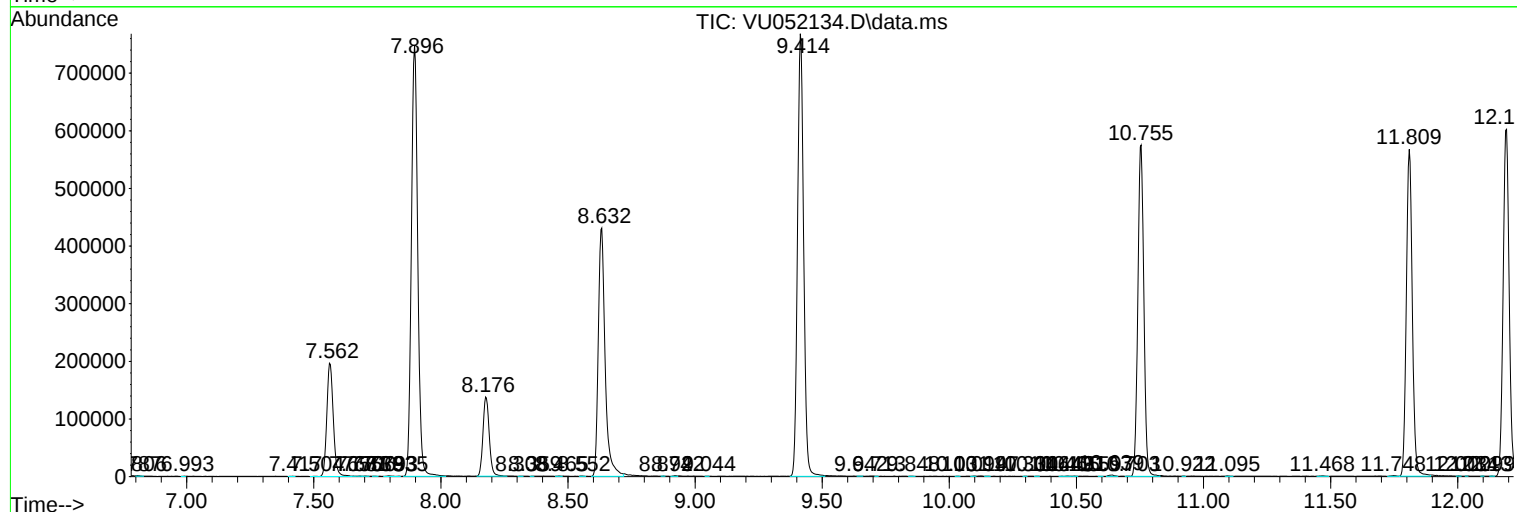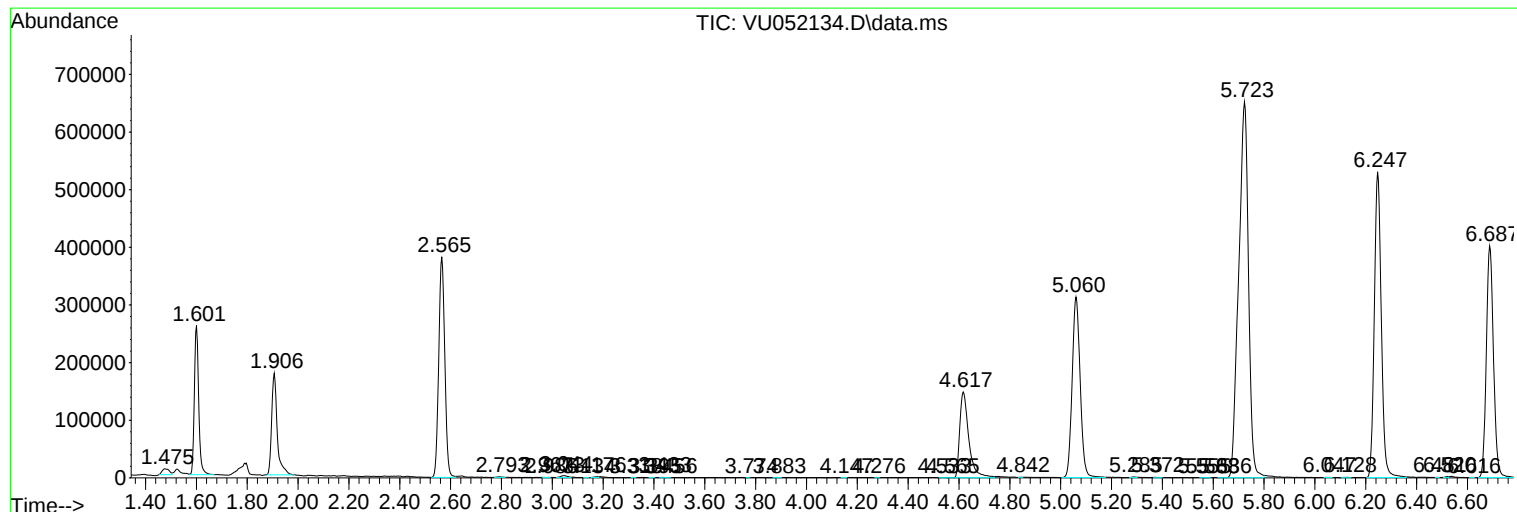

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112522\
Data File : VU052134.D
Acq On : 25 Nov 2022 11:12
Operator : JC/MD
Sample : VU1125WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK032

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112522\
Data File : VU052134.D
Acq On : 25 Nov 2022 11:12
Operator : JC/MD
Sample : VU1125WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK032

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc