

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112522\
 Data File : VU052137.D
 Acq On : 25 Nov 2022 12:31
 Operator : JC/MD
 Sample : N5711-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

Signal : TIC: VU052137.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.472	36	41	52	rBV2	7287	13305	0.79%	0.108%
2	1.600	73	81	101	rVB	231105	266560	15.79%	2.171%
3	1.906	167	176	200	rVB	161437	246512	14.60%	2.007%
4	2.565	368	381	398	rBV	346273	560171	33.19%	4.562%
5	2.784	445	449	451	rBV	535	412	0.02%	0.003%
6	2.909	486	488	493	rVB2	390	239	0.01%	0.002%
7	2.935	493	496	498	rBV	495	324	0.02%	0.003%
8	2.954	498	502	510	rBV2	1211	1357	0.08%	0.011%
9	3.009	517	519	522	rBV3	442	326	0.02%	0.003%
10	3.047	522	531	547	rVV3	4676	9663	0.57%	0.079%
11	3.186	559	574	586	rBV2	6314	14420	0.85%	0.117%
12	3.340	619	622	625	rBV2	365	265	0.02%	0.002%
13	3.391	636	638	643	rVB3	435	243	0.01%	0.002%
14	3.430	647	650	655	rBV2	238	201	0.01%	0.002%
15	3.610	701	706	709	rBV2	224	198	0.01%	0.002%
16	3.710	734	737	743	rVB2	214	223	0.01%	0.002%
17	3.906	792	798	801	rBV3	507	505	0.03%	0.004%
18	3.977	817	820	823	rBV	399	279	0.02%	0.002%
19	4.108	858	861	867	rVB2	320	316	0.02%	0.003%
20	4.137	867	870	876	rBV2	219	237	0.01%	0.002%
21	4.346	931	935	939	rBV2	224	277	0.02%	0.002%
22	4.414	951	956	961	rBV2	356	326	0.02%	0.003%
23	4.616	1007	1019	1045	rBV	146857	356289	21.11%	2.901%
24	4.935	1115	1118	1122	rBV2	318	271	0.02%	0.002%
25	5.060	1139	1157	1181	rBV	303459	666348	39.48%	5.426%
26	5.288	1220	1228	1230	rBV4	829	1097	0.06%	0.009%
27	5.491	1288	1291	1294	rVV3	302	198	0.01%	0.002%
28	5.536	1303	1305	1310	rVB	319	215	0.01%	0.002%
29	5.722	1342	1363	1392	rBV2	621831	1688005	100.00%	13.746%
30	5.867	1407	1408	1419	rVB4	846	961	0.06%	0.008%
31	6.038	1459	1461	1469	rVB3	676	698	0.04%	0.006%
32	6.118	1480	1486	1489	rBV2	535	715	0.04%	0.006%
33	6.150	1493	1496	1501	rVB2	234	234	0.01%	0.002%
34	6.247	1512	1526	1550	rBV	507266	976001	57.82%	7.948%
35	6.526	1608	1613	1615	rBV2	997	991	0.06%	0.008%
36	6.558	1621	1623	1628	rVB3	376	225	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112522\
 Data File : VU052137.D
 Acq On : 25 Nov 2022 12:31
 Operator : JC/MD
 Sample : N5711-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

37	6.687	1648	1663	1692	rBV	396249	775178	45.92%	6.312%
38	6.787	1692	1694	1696	rBV	424	198	0.01%	0.002%
39	6.851	1710	1714	1716	rBV3	389	312	0.02%	0.003%
40	7.021	1762	1767	1769	rBV2	340	314	0.02%	0.003%
41	7.057	1773	1778	1780	rBV3	518	391	0.02%	0.003%
42	7.150	1805	1807	1812	rVV2	321	290	0.02%	0.002%
43	7.185	1815	1818	1822	rVV2	502	518	0.03%	0.004%
44	7.272	1842	1845	1852	rVB2	293	232	0.01%	0.002%
45	7.494	1907	1914	1917	rBV2	369	297	0.02%	0.002%
46	7.562	1923	1935	1958	rBV	190456	337640	20.00%	2.749%
47	7.896	2021	2039	2064	rBV	720754	1240991	73.52%	10.106%
48	8.176	2114	2126	2143	rBV	135302	230671	13.67%	1.878%
49	8.288	2159	2161	2165	rVB3	594	376	0.02%	0.003%
50	8.340	2172	2177	2178	rBV	269	248	0.01%	0.002%
51	8.430	2201	2205	2208	rVB3	388	361	0.02%	0.003%
52	8.459	2208	2214	2216	rBV3	687	636	0.04%	0.005%
53	8.632	2255	2268	2299	rBV	430375	803162	47.58%	6.540%
54	8.809	2321	2323	2326	rVB3	689	332	0.02%	0.003%
55	8.880	2342	2345	2348	rBV	495	318	0.02%	0.003%
56	8.896	2348	2350	2354	rVB2	377	237	0.01%	0.002%
57	8.925	2357	2359	2364	rVV3	377	313	0.02%	0.003%
58	9.041	2392	2395	2399	rBV2	286	243	0.01%	0.002%
59	9.079	2403	2407	2412	rBV2	376	300	0.02%	0.002%
60	9.172	2430	2436	2439	rBV2	418	376	0.02%	0.003%
61	9.201	2441	2445	2447	rBV2	496	373	0.02%	0.003%
62	9.336	2484	2487	2494	rVB3	444	485	0.03%	0.004%
63	9.414	2498	2511	2535	rBV	739512	1228680	72.79%	10.005%
64	9.619	2572	2575	2577	rBV2	530	301	0.02%	0.002%
65	9.668	2587	2590	2592	rVV2	385	218	0.01%	0.002%
66	9.693	2596	2598	2601	rVV2	391	282	0.02%	0.002%
67	9.722	2604	2607	2610	rVB3	320	230	0.01%	0.002%
68	9.832	2636	2641	2643	rBV2	329	261	0.02%	0.002%
69	9.918	2665	2668	2672	rBV	393	311	0.02%	0.003%
70	9.983	2683	2688	2689	rBV3	265	202	0.01%	0.002%
71	10.037	2700	2705	2708	rBV2	209	231	0.01%	0.002%
72	10.057	2708	2711	2715	rVV	292	238	0.01%	0.002%
73	10.095	2720	2723	2726	rBV2	386	350	0.02%	0.003%
74	10.340	2794	2799	2801	rBV2	298	244	0.01%	0.002%
75	10.385	2809	2813	2817	rBV2	312	307	0.02%	0.002%
76	10.516	2852	2854	2859	rVB2	287	239	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112522\
 Data File : VU052137.D
 Acq On : 25 Nov 2022 12:31
 Operator : JC/MD
 Sample : N5711-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

77	10.754	2914	2928	2952	rBV	571959	922398	54.64%	7.511%
78	10.860	2958	2961	2968	rBV4	365	399	0.02%	0.003%
79	10.915	2976	2978	2982	rVB2	436	254	0.02%	0.002%
80	10.954	2986	2990	2993	rBV2	493	349	0.02%	0.003%
81	10.992	2999	3002	3004	rVB2	400	243	0.01%	0.002%
82	11.211	3067	3070	3072	rBV	334	232	0.01%	0.002%
83	11.240	3076	3079	3084	rBV3	256	271	0.02%	0.002%
84	11.372	3116	3120	3125	rBV2	471	437	0.03%	0.004%
85	11.475	3148	3152	3154	rBV3	391	308	0.02%	0.003%
86	11.722	3226	3229	3232	rBV	426	270	0.02%	0.002%
87	11.751	3235	3238	3242	rVB2	399	285	0.02%	0.002%
88	11.809	3243	3256	3276	rBV	564586	922423	54.65%	7.511%
89	11.957	3298	3302	3306	rVB3	1058	795	0.05%	0.006%
90	12.028	3322	3324	3329	rVB3	440	271	0.02%	0.002%
91	12.053	3329	3332	3335	rVB2	375	253	0.01%	0.002%
92	12.192	3358	3375	3399	rBV	601040	993128	58.83%	8.087%
93	12.413	3441	3444	3446	rBV2	318	239	0.01%	0.002%
94	12.577	3492	3495	3499	rVB2	278	231	0.01%	0.002%
95	12.880	3586	3589	3591	rBV2	330	267	0.02%	0.002%
96	12.970	3614	3617	3619	rBV	311	215	0.01%	0.002%
97	13.574	3800	3805	3810	rBV3	484	722	0.04%	0.006%
98	13.745	3856	3858	3860	rBV3	403	207	0.01%	0.002%
99	15.073	4269	4271	4273	rBV2	535	325	0.02%	0.003%
100	15.532	4412	4414	4417	rBV	590	329	0.02%	0.003%




Sum of corrected areas: 12280344

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112522\
Data File : VU052137.D
Acq On : 25 Nov 2022 12:31
Operator : JC/MD
Sample : N5711-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

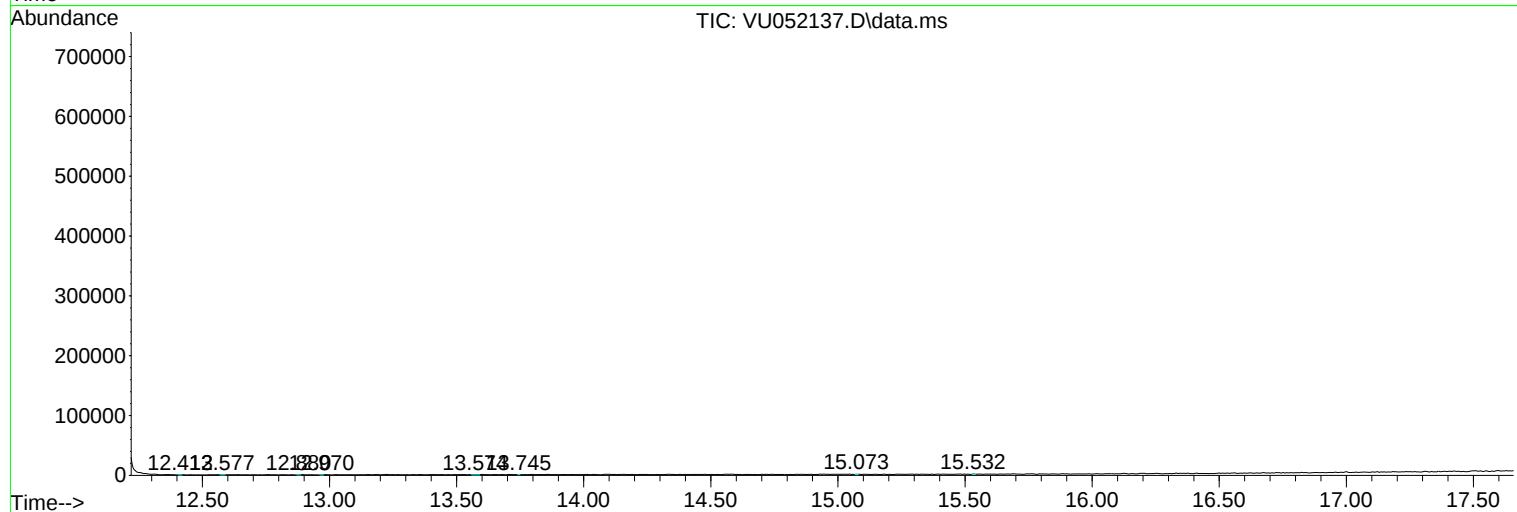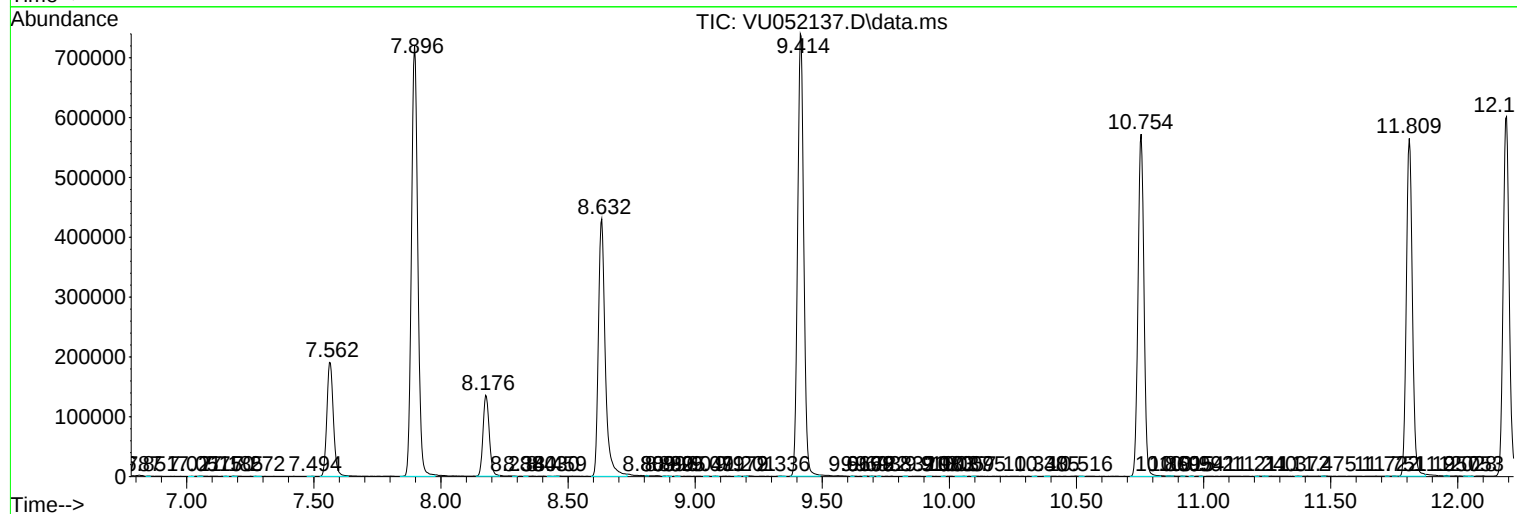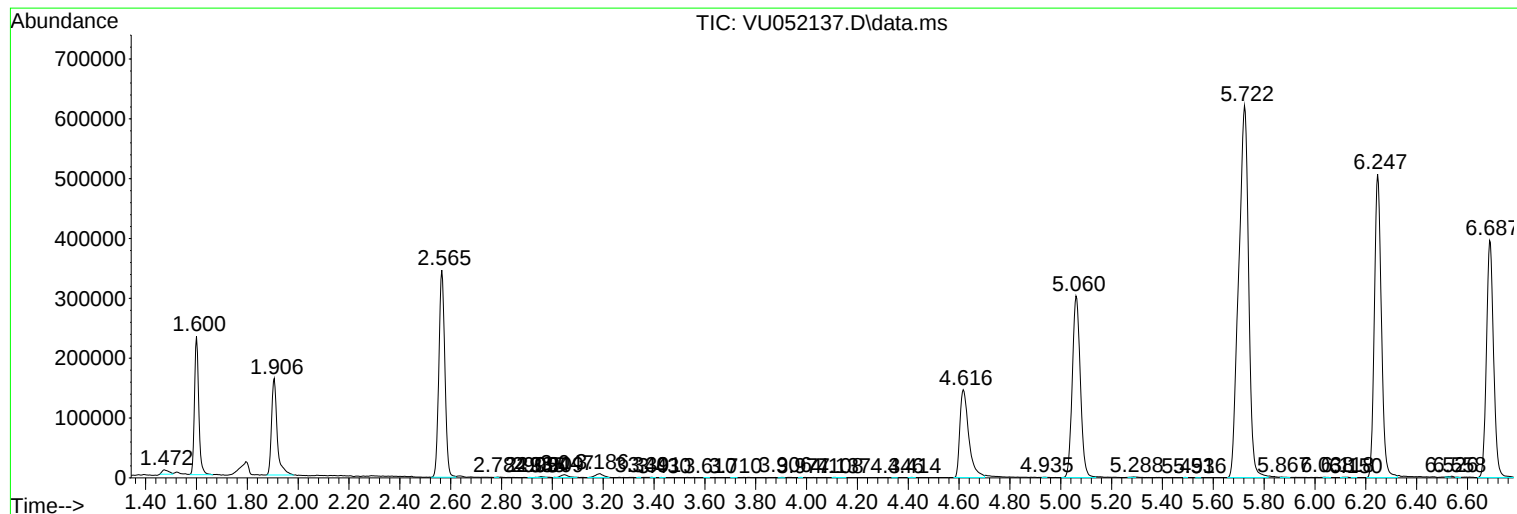

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112522\
Data File : VU052137.D
Acq On : 25 Nov 2022 12:31
Operator : JC/MD
Sample : N5711-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112522\
Data File : VU052137.D
Acq On : 25 Nov 2022 12:31
Operator : JC/MD
Sample : N5711-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc