
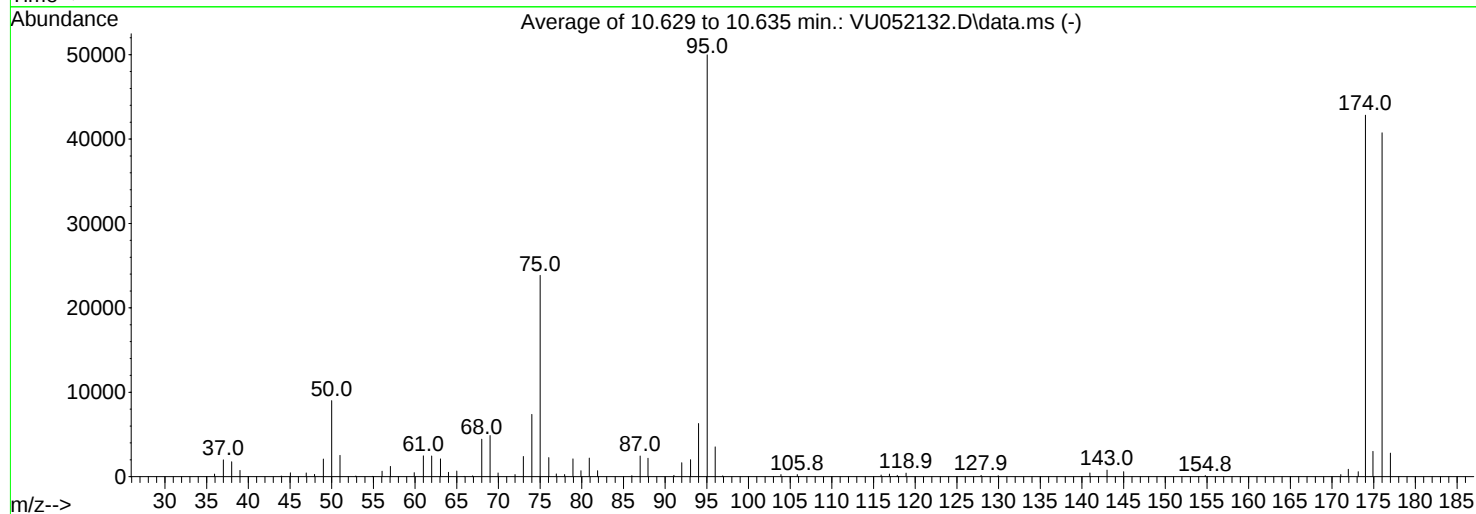


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112522\
Data File : VU052132.D
Acq On : 25 Nov 2022 09:54
Operator : JC/MD
Sample : BFB148
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB148

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Title : VOC Analysis
Last Update : Fri Nov 25 21:01:09 2022

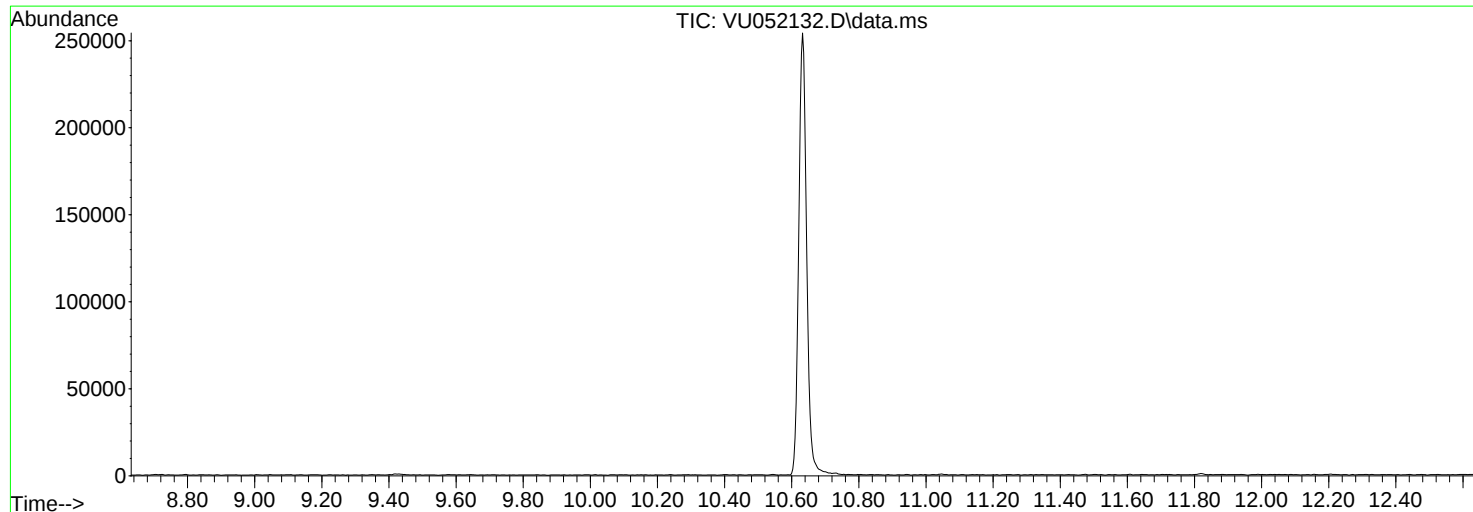

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	9014	PASS
75	95	30	80	47.7	23848	PASS
95	95	100	100	100.0	49981	PASS
96	95	5	9	7.1	3529	PASS
173	174	0.00	2	1.4	594	PASS
174	95	50	120	85.7	42837	PASS
175	174	5	9	7.0	2994	PASS
176	174	95	101	95.1	40739	PASS
177	176	5	9	6.8	2784	PASS

m/z	Abundance
39.90	209.0
43.90	440.0

Instrument :
MSVOA_U
ClientSampleId :
BFB148

m/z	Abundance
36.00	316.0
37.00	1950.0
38.00	1754.0
39.00	755.0
39.90	206.0
44.00	523.0
45.10	444.0
47.00	387.0
48.00	266.0
49.00	2151.0
50.00	9164.0
51.00	2596.0
54.90	138.0
56.00	565.0
57.00	1145.0
59.90	475.0
61.00	2518.0
62.00	2526.0
63.00	2210.0
64.00	503.0
65.00	603.0
66.90	137.0
68.00	4288.0
69.00	4727.0
69.90	409.0
72.00	249.0
73.00	2478.0
74.00	7643.0
75.00	23712.0
76.00	2000.0
76.90	327.0
77.90	244.0
78.90	2182.0
79.90	631.0
80.90	2045.0
81.90	645.0
87.00	2531.0
88.00	2384.0
91.00	142.0
92.00	1727.0
93.00	1986.0
94.00	6304.0
95.10	49616.0
96.00	3630.0
96.90	158.0
103.90	257.0
105.90	234.0
115.90	163.0
116.90	330.0
117.80	135.0
118.90	355.0
127.90	141.0
130.00	116.0
141.00	424.0
143.00	823.0
145.00	594.0
154.80	150.0
171.00	234.0
172.00	787.0
173.20	633.0
174.00	40648.0
174.90	2947.0
176.00	39104.0
177.00	2721.0

Instrument :
MSVOA_U
ClientSampleId :
BFB148

m/z	Abundance
36.00	302.0
37.00	2102.0
38.00	1826.0
39.00	743.0
39.80	193.0
44.00	523.0
45.00	457.0
46.90	443.0
48.00	267.0
49.00	2210.0
50.00	9346.0
51.00	2618.0
52.90	104.0
56.00	677.0
57.10	1274.0
59.90	484.0
61.00	2556.0
62.00	2475.0
63.00	2137.0
64.00	527.0
65.00	695.0
65.90	100.0
66.90	132.0
68.00	4558.0
69.00	4984.0
70.00	455.0
72.00	257.0
73.00	2436.0
74.00	7511.0
75.00	24376.0
76.10	2348.0
77.00	326.0
78.00	247.0
79.00	2119.0
79.90	716.0
80.90	2282.0
81.90	742.0
86.00	133.0
87.00	2572.0
88.00	2247.0
91.10	162.0
92.00	1726.0
93.10	2088.0
94.00	6550.0
95.10	51456.0
96.00	3667.0
96.90	144.0
103.90	261.0
105.80	274.0
115.90	205.0
116.90	311.0
117.80	164.0
118.90	425.0
127.90	168.0
130.00	106.0
140.90	446.0
143.00	786.0
145.00	601.0
154.80	140.0
171.10	259.0
171.90	898.0
173.20	632.0
174.00	44352.0
174.90	3143.0
176.00	42040.0
177.00	2905.0

Instrument :
MSVOA_U
ClientSampleId :
BFB148

m/z	Abundance
35.90	311.0
37.00	1931.0
38.00	1739.0
39.00	744.0
39.90	210.0
44.00	507.0
45.00	456.0
46.90	503.0
47.90	254.0
49.00	1889.0
50.00	8532.0
51.00	2369.0
52.90	134.0
56.10	717.0
57.10	1247.0
59.90	466.0
61.00	2346.0
62.00	2317.0
63.10	1961.0
64.00	530.0
65.00	696.0
68.00	4473.0
69.00	4890.0
70.00	474.0
72.00	258.0
73.00	2249.0
74.00	6990.0
75.00	23456.0
76.10	2407.0
77.00	321.0
78.00	232.0
79.00	2009.0
79.90	741.0
80.90	2265.0
81.90	737.0
86.00	201.0
87.00	2234.0
87.90	1943.0
91.10	166.0
92.00	1522.0
93.00	1956.0
94.00	6048.0
95.00	48872.0
96.00	3289.0
103.90	203.0
105.80	256.0
115.90	212.0
116.90	285.0
117.90	166.0
118.90	459.0
127.90	157.0
129.80	103.0
141.00	427.0
143.00	745.0
145.00	544.0
154.80	122.0
171.00	228.0
171.90	916.0
173.10	518.0
174.00	43512.0
174.90	2893.0
176.00	41072.0
177.00	2725.0

Instrument :
MSVOA_U
ClientSampleId :
BFB148