

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112525\
 Data File : VU063795.D
 Acq On : 25 Nov 2025 12:08
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK013

Quant Time: Nov 26 03:32:58 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM112525.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Nov 26 03:25:40 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.234	114	35445	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.403	117	48054	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.791	152	18584	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.583	65	12634	0.511	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	102.000%
4) 1,2-Dichloroethane-d4	5.685	65	9020	0.493	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	98.000%
7) 1,2-Dichloropropane-d6	6.664	67	8507	0.623	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	124.000%
8) Toluene-d8	7.872	98	27558	0.511	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	102.000%
10) 1,1,2,2-Tetrachloroeth...	10.728	84	6396	0.582	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	116.000%
Target Compounds						
6) Trichloroethene	6.520	95	623	0.024	ug/L	91
12) 1,2,3-Trichloropropane	10.797	75	565	0.038	ug/L #	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112525\
Data File : VU063795.D
Acq On : 25 Nov 2025 12:08
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK013

Quant Time: Nov 26 03:32:58 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM112525.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 26 03:25:40 2025
Response via : Initial Calibration

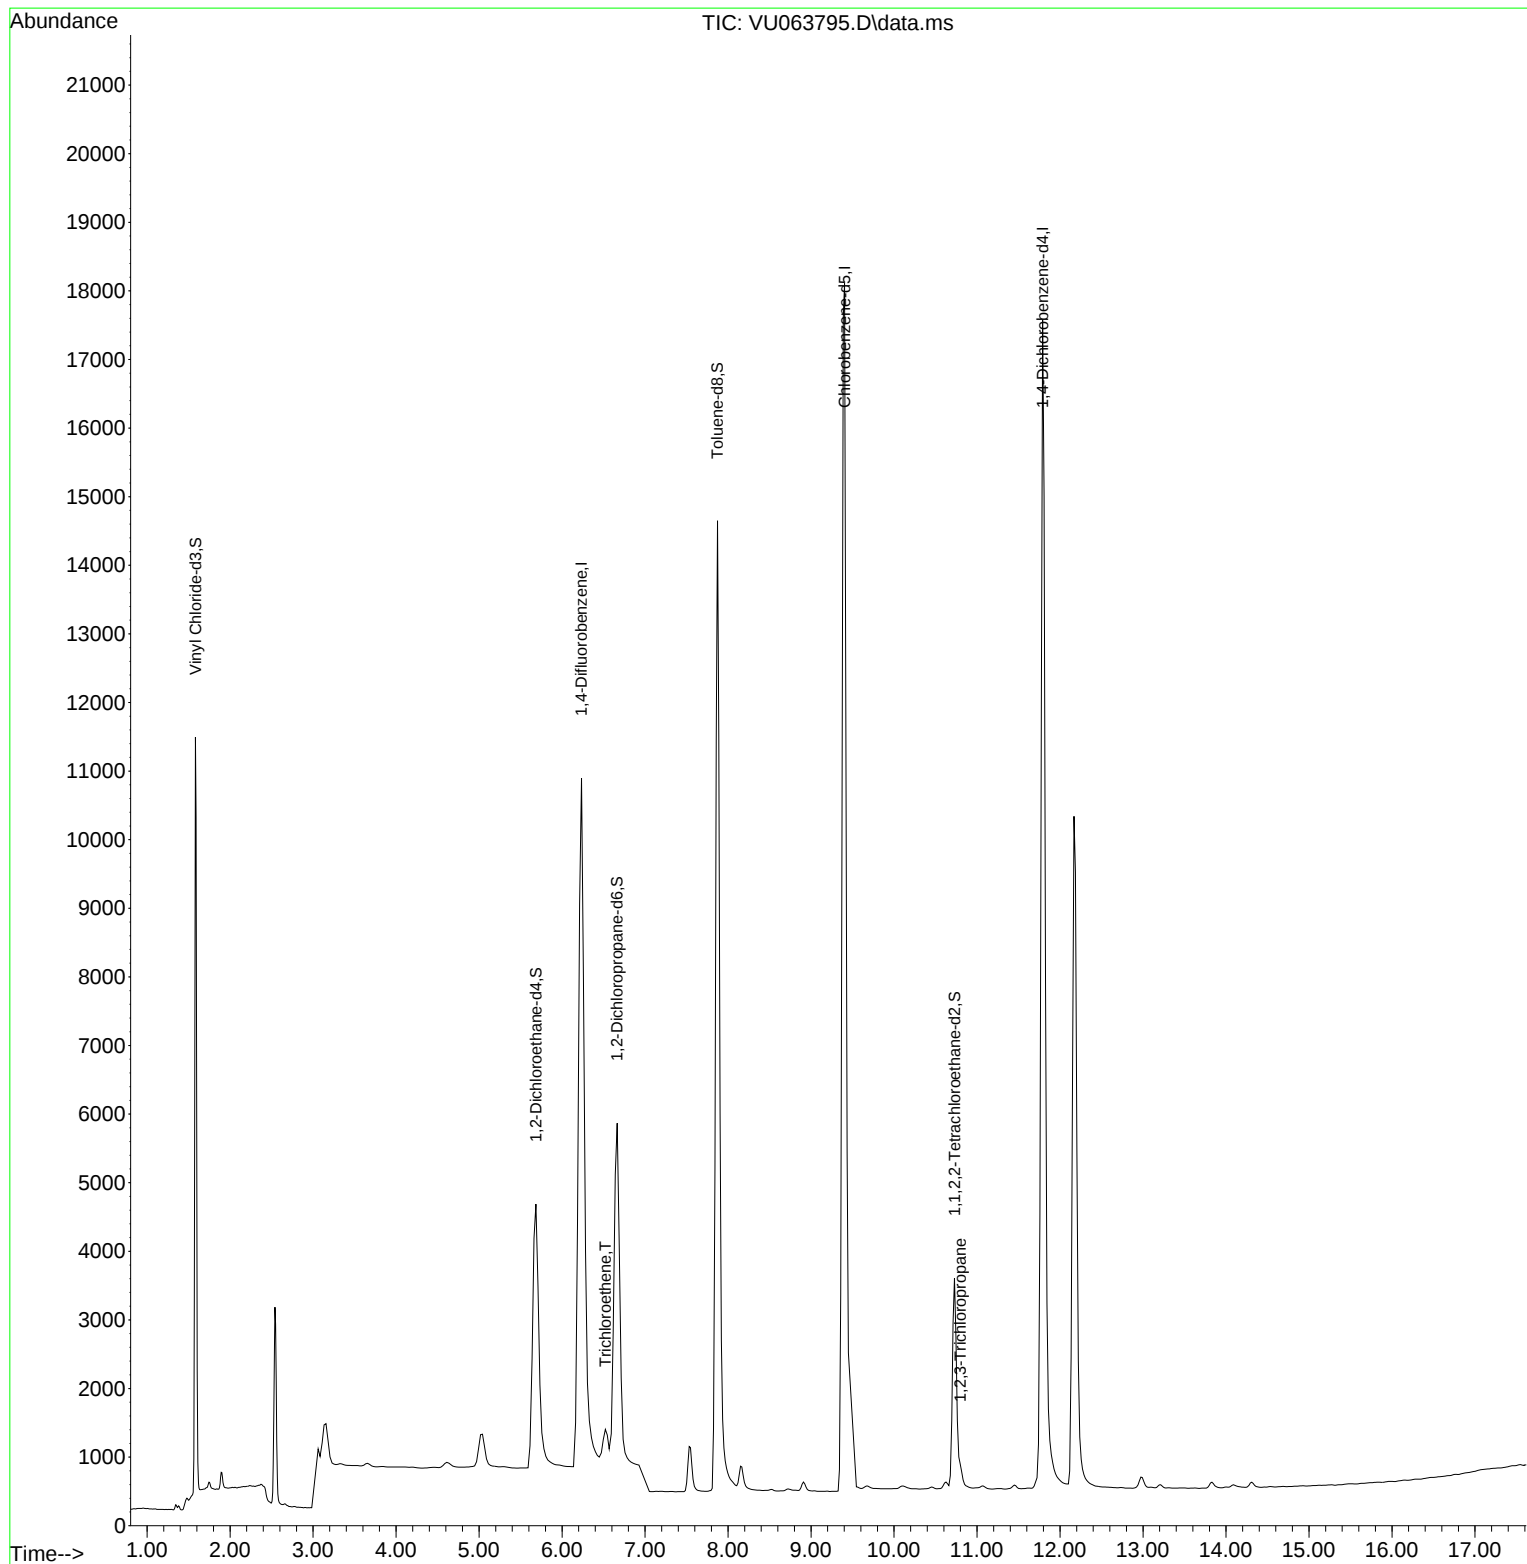

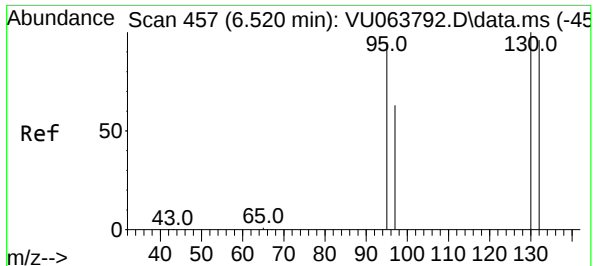

#6

Trichloroethene

Concen: 0.024 ug/L

RT: 6.520 min Scan# 457

Delta R.T. 0.000 min

Lab File: VU063795.D


Acq: 25 Nov 2025 12:08

Instrument :

MSVOA_U

ClientSampleId :

VIBLK013

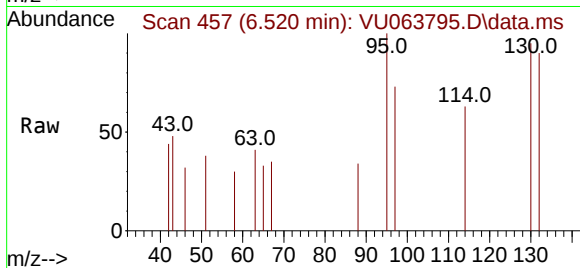

Tgt Ion: 95 Resp: 623




Ion Ratio Lower Upper

95 100

97 73.0 46.7 86.7

132 90.3 70.1 130.3

130 95.1 73.1 135.7

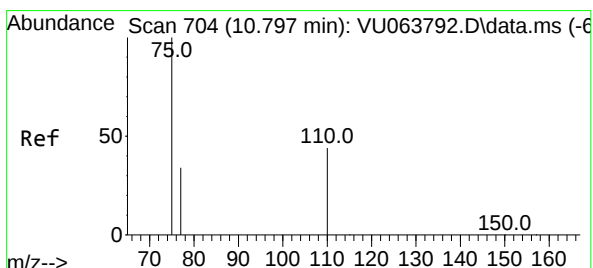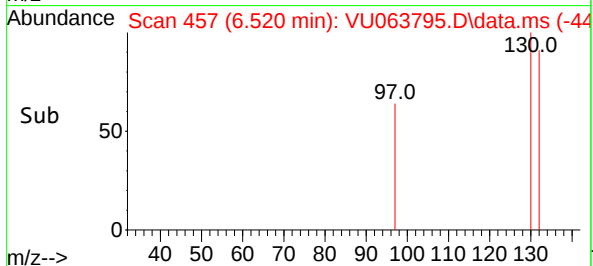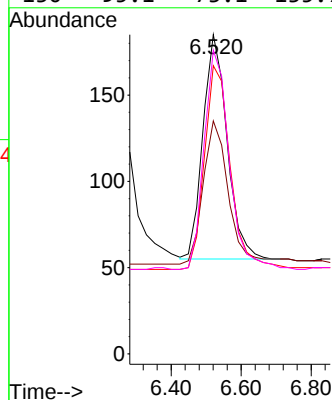

#12

1,2,3-Trichloropropane

Concen: 0.038 ug/L

RT: 10.797 min Scan# 704

Delta R.T. 0.000 min

Lab File: VU063795.D

Acq: 25 Nov 2025 12:08

Tgt Ion: 75 Resp: 565

Ion Ratio Lower Upper

75 100

110 39.6 32.9 49.3

77 49.7 27.3 40.9#

