

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU112618\
 Data File : VU028334.D
 Acq On : 26 Nov 2018 13:09
 Operator : MD/SY
 Sample : VU1126WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU1126WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U0112618DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.077	590	592	595	rVB2	2223	1308	1.12%	0.318%
2	4.003	876	880	884	rBV4	1146	1216	1.05%	0.295%
3	4.250	951	957	960	rBV5	1675	2158	1.86%	0.524%
4	4.668	1077	1087	1096	rBV7	4044	8603	7.40%	2.090%
5	4.987	1184	1186	1194	rVB7	1604	1639	1.41%	0.398%
6	5.742	1405	1421	1440	rBV2	55421	116315	100.00%	28.264%
7	6.186	1555	1559	1564	rBV5	1339	1226	1.05%	0.298%
8	6.762	1734	1738	1745	rVB4	1525	1520	1.31%	0.369%
9	7.713	2025	2034	2036	rBV5	985	1417	1.22%	0.344%
10	7.893	2082	2090	2094	rBV4	1003	1516	1.30%	0.368%
11	7.929	2094	2101	2104	rBV4	978	1209	1.04%	0.294%
12	8.231	2187	2195	2201	rBV7	2098	3225	2.77%	0.784%
13	8.469	2263	2269	2272	rBV4	1253	1537	1.32%	0.373%
14	8.626	2308	2318	2325	rBV9	2774	4576	3.93%	1.112%
15	9.122	2466	2472	2478	rBV5	1541	1880	1.62%	0.457%
16	9.372	2544	2550	2552	rBV4	1930	1790	1.54%	0.435%
17	9.790	2673	2680	2688	rVB6	2468	3934	3.38%	0.956%
18	10.032	2752	2755	2762	rVB5	2048	2327	2.00%	0.565%
19	10.308	2830	2841	2856	rBV	47981	78456	67.45%	19.064%
20	10.459	2877	2888	2893	rBV6	1127	1789	1.54%	0.435%
21	10.591	2924	2929	2936	rVB7	1448	2004	1.72%	0.487%
22	10.771	2979	2985	2986	rBV3	1327	1184	1.02%	0.288%
23	11.096	3082	3086	3094	rBV6	1383	1835	1.58%	0.446%
24	11.154	3098	3104	3108	rVB6	1320	1542	1.33%	0.375%
25	11.224	3124	3126	3134	rVB5	937	1225	1.05%	0.298%
26	11.421	3180	3187	3194	rBV6	3056	3687	3.17%	0.896%
27	11.482	3198	3206	3207	rBV4	2578	2577	2.22%	0.626%
28	11.745	3278	3288	3299	rBV5	2926	5080	4.37%	1.234%
29	11.861	3313	3324	3343	rBV2	59811	107632	92.53%	26.154%
30	12.575	3537	3546	3553	rBV7	3039	4653	4.00%	1.131%
31	13.118	3704	3715	3723	rBV6	2452	4515	3.88%	1.097%
32	13.504	3827	3835	3844	rBV6	5259	7802	6.71%	1.896%
33	13.745	3903	3910	3918	rBV3	5395	8550	7.35%	2.078%
34	13.990	3974	3986	4001	rVB9	6382	12750	10.96%	3.098%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU112618\
Data File : VU028334.D
Acq On : 26 Nov 2018 13:09
Operator : MD/SY
Sample : VU1126WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1126WBL01

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U0112618DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER

35	14.134	4021	4031	4033	rbV4	1242	1789	1.54%	0.435%
36	14.279	4065	4076	4085	rvB3	3064	5733	4.93%	1.393%
37	15.533	4461	4466	4469	rbV4	1502	1333	1.15%	0.324%


Sum of corrected areas: 411532

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU112618\
Data File : VU028334.D
Acq On : 26 Nov 2018 13:09
Operator : MD/SY
Sample : VU1126WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1126WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U0112618DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

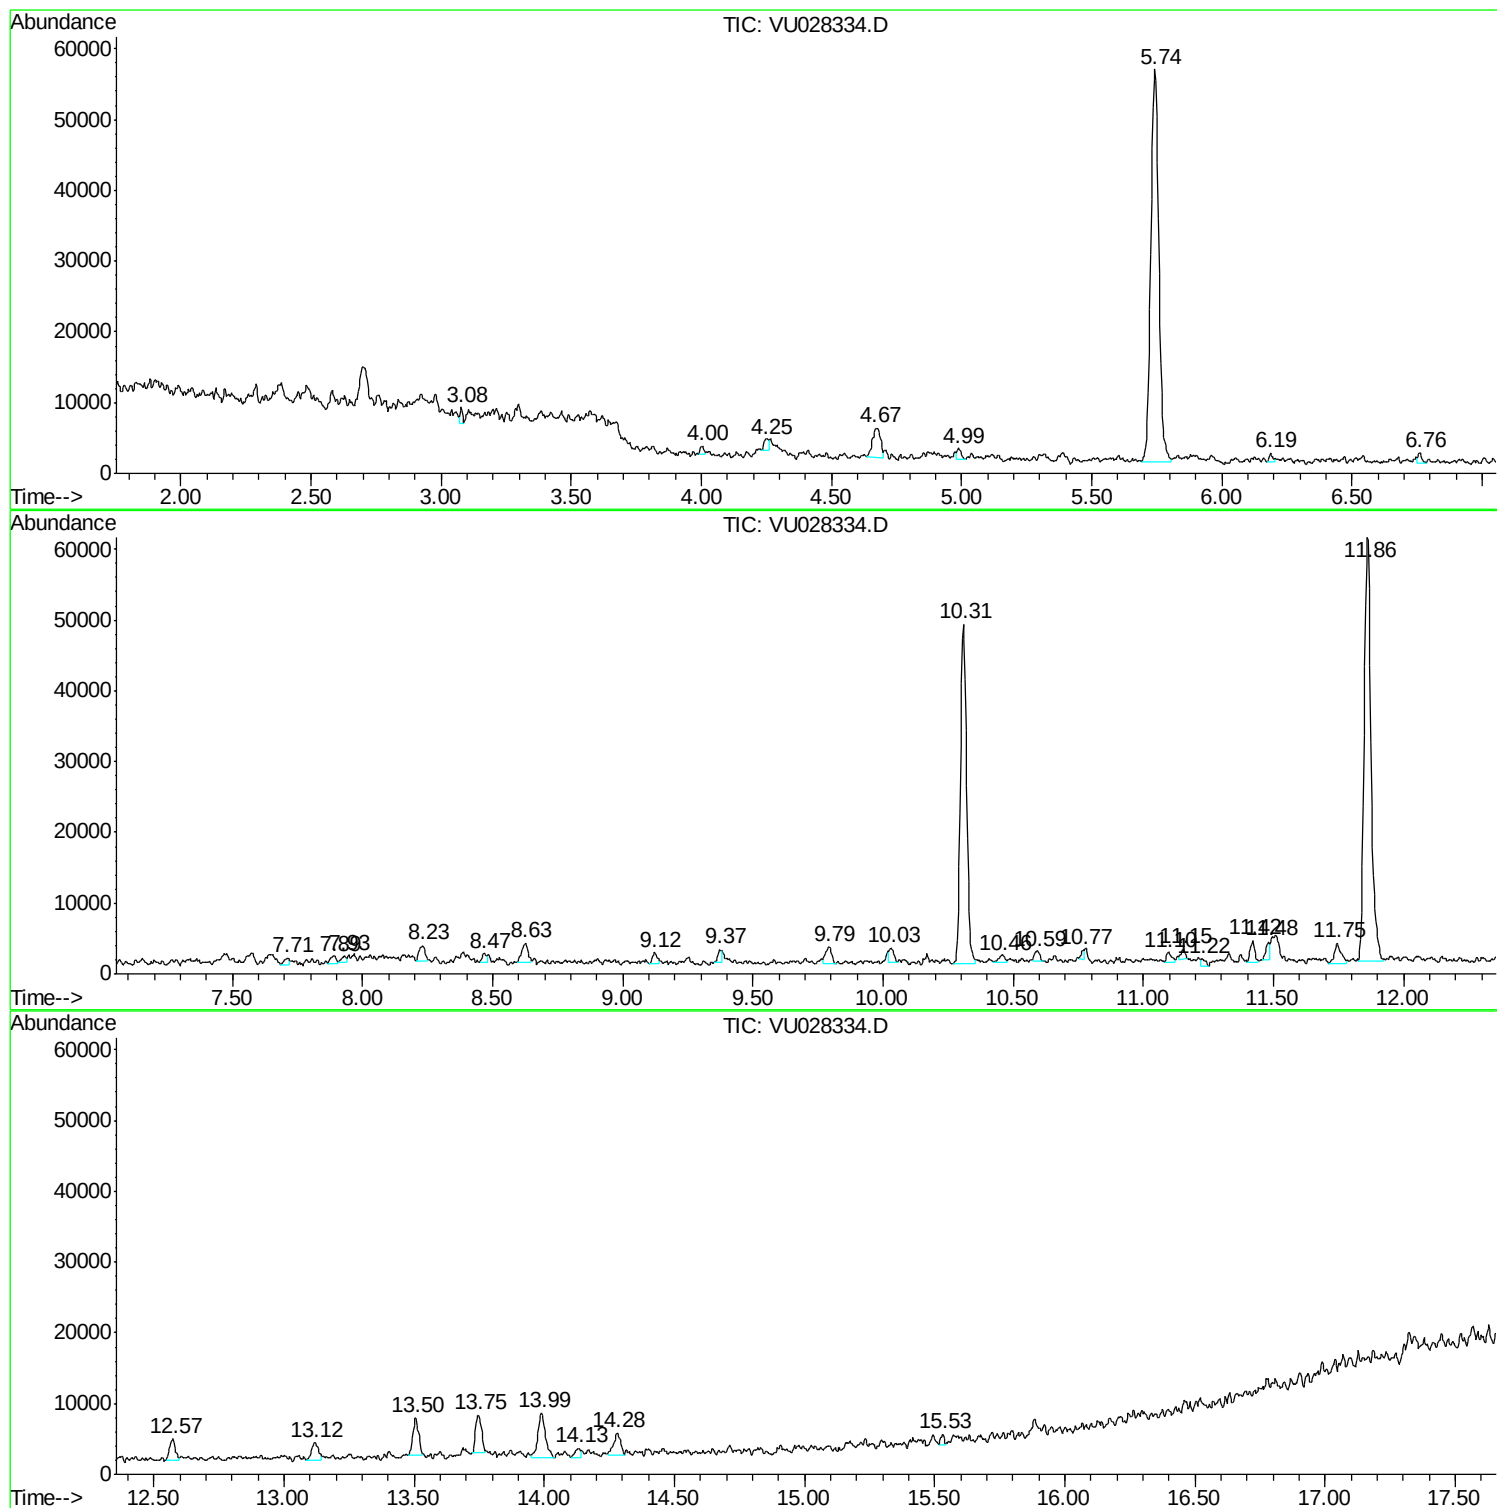

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU112618\
Data File : VU028334.D
Acq On : 26 Nov 2018 13:09
Operator : MD/SY
Sample : VU1126WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1126WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U0112618DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU112618\
Data File : VU028334.D
Acq On : 26 Nov 2018 13:09
Operator : MD/SY
Sample : VU1126WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU1126WBL01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\524U0112618DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc