


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU112618\
 Data File : VU028326.D
 Acq On : 26 Nov 2018 08:35
 Operator : MD/SY
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\524U112618DW.M
 Title : METHOD 524.2 VOLATILES DRINKING WATER
 Last Update : Tue Nov 27 01:03:50 2018

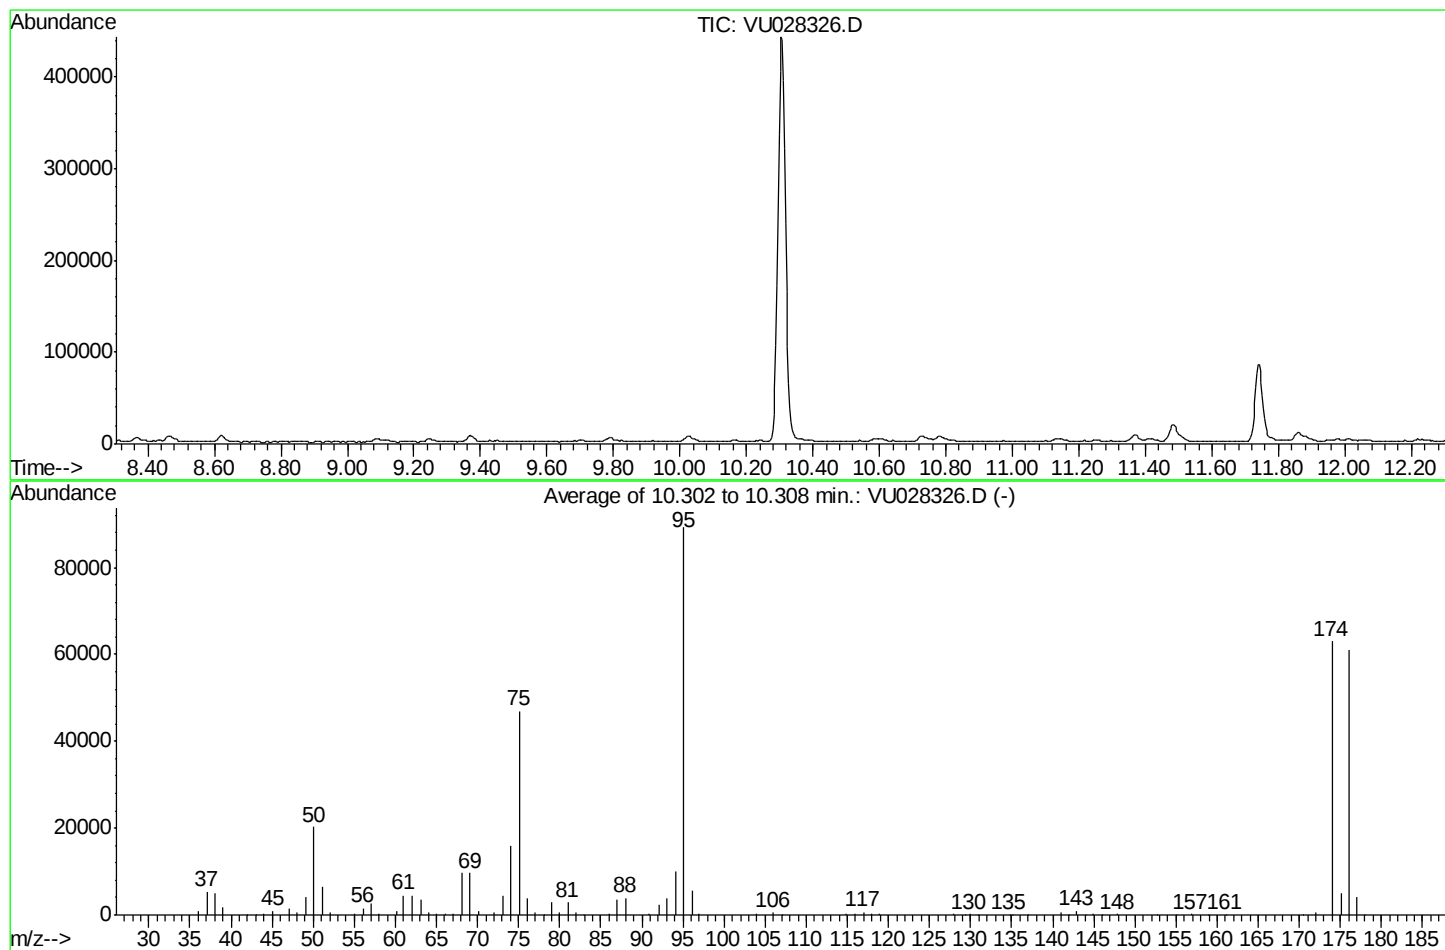

AutoFind: Scans 2839, 2840, 2841; Background Corrected with Scan 2826

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	20272	PASS
75	95	30	60	52.6	46978	PASS
95	95	100	100	100.0	89269	PASS
96	95	5	9	6.4	5752	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	70.6	63050	PASS
175	174	5	9	7.8	4934	PASS
176	174	95	101	96.8	61016	PASS
177	176	5	9	6.8	4152	PASS