

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\U112619\
 Data File : VU035852.D
 Acq On : 26 Nov 2019 12:50
 Operator : JC/SP
 Sample : K5992-05DL 100X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GARE6DL

Quant Time: Nov 27 02:01:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Nov 27 01:18:55 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	238763	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	273681	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	102016	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	166351	5.33	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	106.60%
7) Chloroethane-d5	1.93	69	149049	5.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	110.40%
11) 1,1-Dichloroethene-d2	2.59	63	201549	3.48	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.60%
20) 2-Butanone-d5	4.70	46	388105	53.77	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	107.54%
24) Chloroform-d	5.11	84	258474	4.89	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.80%
26) 1,2-Dichloroethane-d4	5.75	65	144588	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.60%
32) Benzene-d6	5.77	84	501061	4.80	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.00%
36) 1,2-Dichloropropane-d6	6.73	67	174180	4.95	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.00%
41) Toluene-d8	7.93	98	405998	4.21	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.20%
43) trans-1,3-Dichloropropene-	8.22	79	61101	4.46	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.20%
46) 2-Hexanone-d5	8.68	63	283854	51.58	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	103.16%
57) 1,1,2,2-Tetrachloroethane-	10.78	84	136391	4.60	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.00%
64) 1,2-Dichlorobenzene-d4	12.22	152	118288	5.34	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.80%

Target Compounds


					Qvalue
5) Vinyl chloride	1.62	62	34396	0.863 ug/L	90
12) 1,1-Dichloroethene	2.60	96	5184	0.209 ug/L #	1
18) trans-1,2-Dichloroethene	3.39	96	4587	0.188 ug/L	93
22) cis-1,2-Dichloroethene	4.72	96	321797	11.805 ug/L	98
34) Trichloroethene	6.58	95	347741	12.415 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU112619\
Data File : VU035852.D
Acq On : 26 Nov 2019 12:50
Operator : JC/SP
Sample : K5992-05DL 100X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GARE6DL

Quant Time: Nov 27 02:01:25 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 27 01:18:55 2019
Response via : Initial Calibration

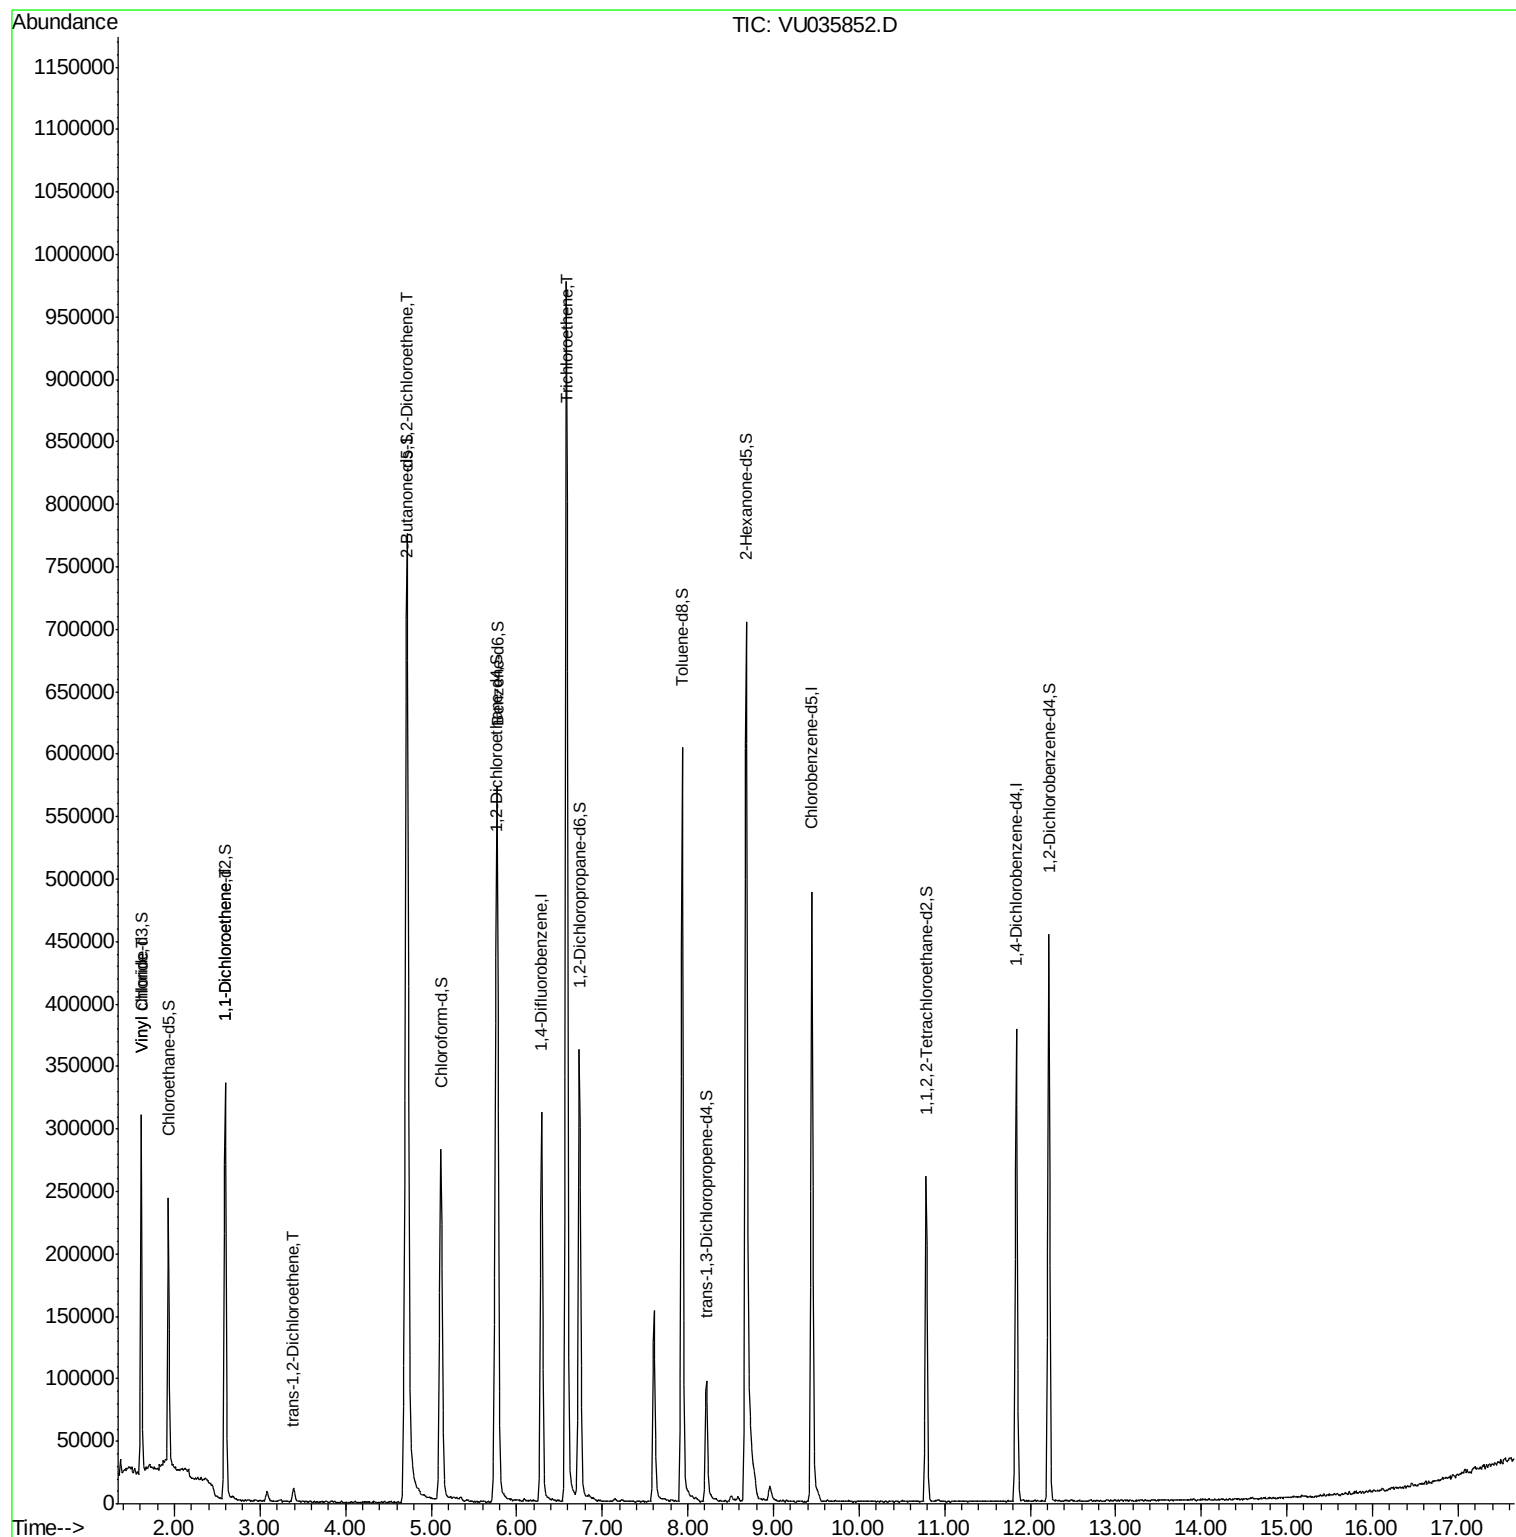

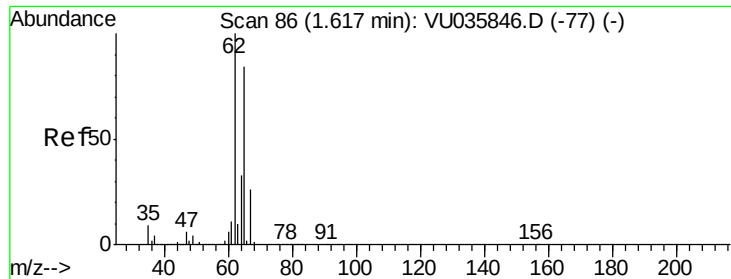

#5

Vinyl chloride

Concen: 0.863 ug/L

RT: 1.62 min Scan# 86

Delta R.T. 0.00 min

Lab File: VU035852.D

Acq: 26 Nov 2019 12:50

Instrument :

MSVOA_U

ClientSampleId :





GARE6DL

Tgt Ion: 62 Resp: 34396

Ion Ratio Lower Upper

62 100

64 38.0 22.5 41.9

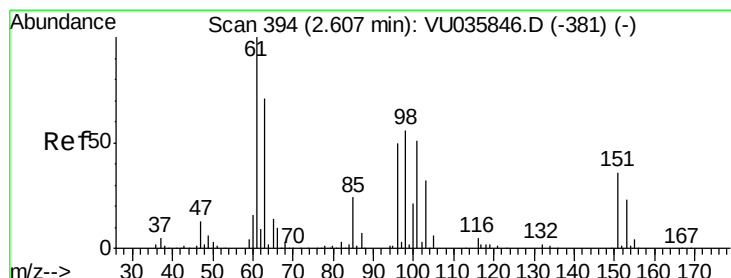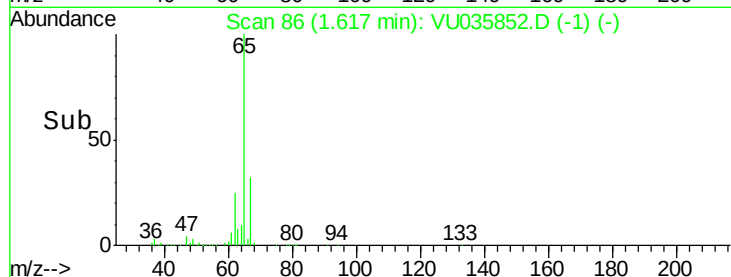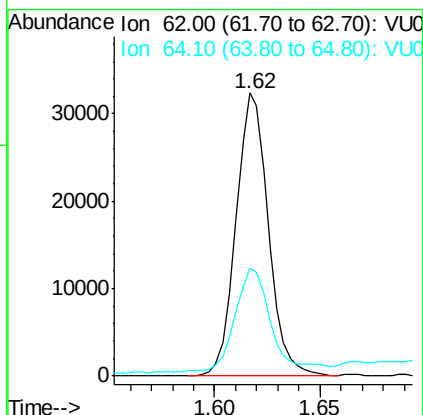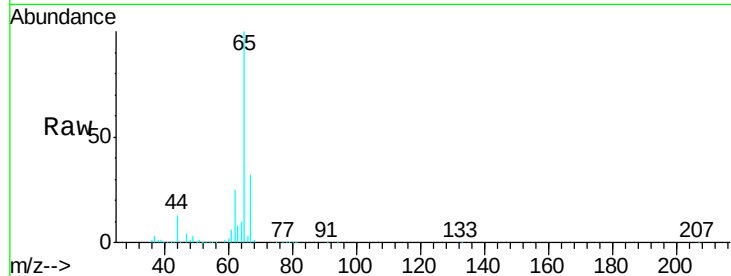

#12

1,1-Dichloroethene

Concen: 0.209 ug/L

RT: 2.60 min Scan# 393

Delta R.T. -0.00 min

Lab File: VU035852.D

Acq: 26 Nov 2019 12:50




Tgt Ion: 96 Resp: 5184


Ion Ratio Lower Upper

96 100

61 462.6 139.3 258.7#

63 2841.8 93.7 174.1#

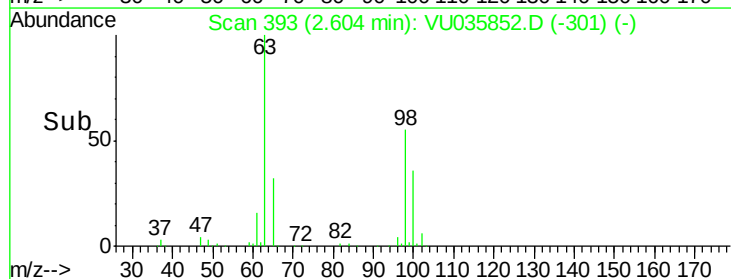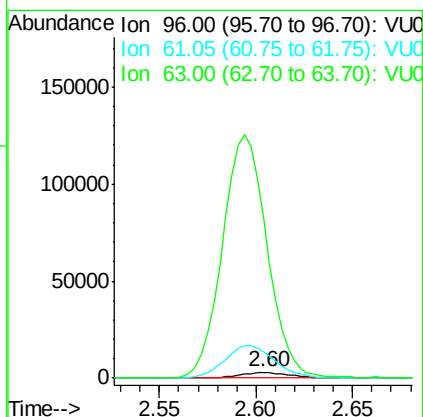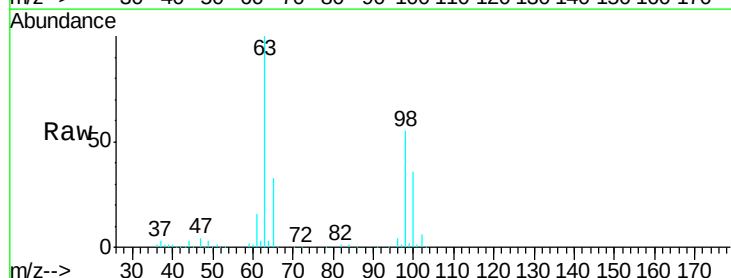

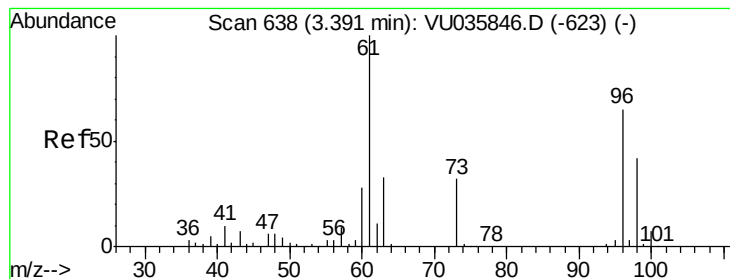

#18

trans-1,2-Dichloroethene

Concen: 0.188 ug/L

RT: 3.39 min Scan# 639

Delta R.T. 0.00 min

Lab File: VU035852.D

Acq: 26 Nov 2019 12:50

Instrument :

MSVOA_U

ClientSampleId :

GARE6DL


Tgt Ion: 96 Resp: 4587

Ion Ratio Lower Upper

96 100

61 148.1 111.1 206.3




98 64.0 43.1 80.1

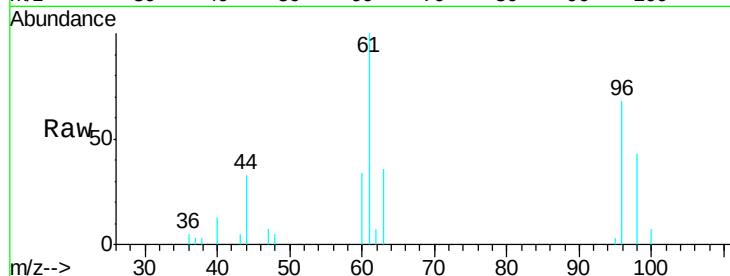

Abundance Ion 96.00 (95.70 to 96.70): VU035846.D (-623) (-)

Ion 61.05 (60.75 to 61.75): VU035846.D (-623) (-)

Ion 97.95 (97.65 to 98.65): VU035846.D (-623) (-)

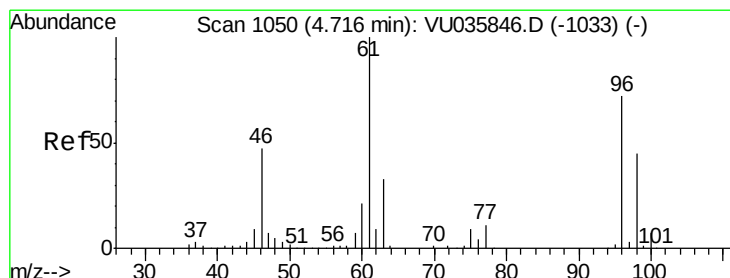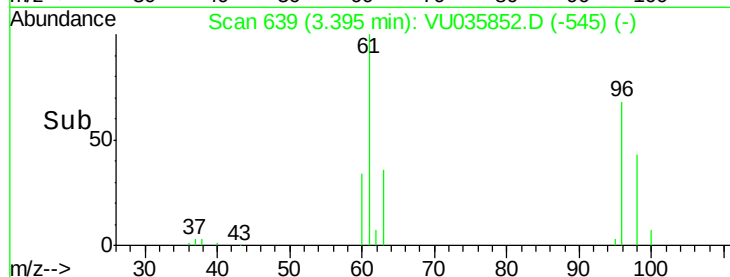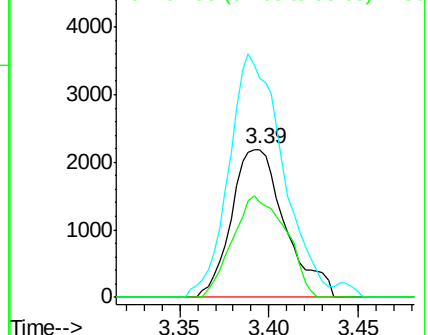

#22

cis-1,2-Dichloroethene

Concen: 11.805 ug/L

RT: 4.72 min Scan# 1051

Delta R.T. 0.00 min

Lab File: VU035852.D

Acq: 26 Nov 2019 12:50


Tgt Ion: 96 Resp: 321797

Ion Ratio Lower Upper

96 100

61 137.4 98.1 182.1



68 0.0 0.0 0.0

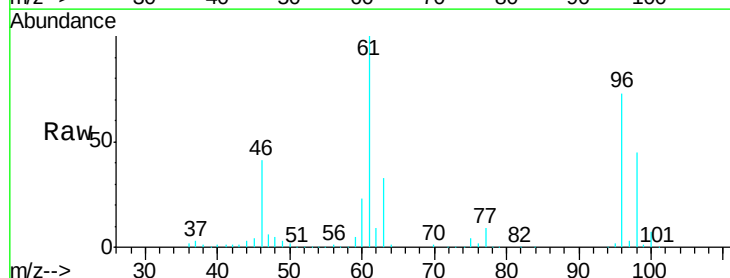


Abundance Ion 96.00 (95.70 to 96.70): VU035846.D (-1033) (-)

Ion 61.05 (60.75 to 61.75): VU035846.D (-1033) (-)

Ion 68.15 (67.85 to 68.85): VU035846.D (-1033) (-)

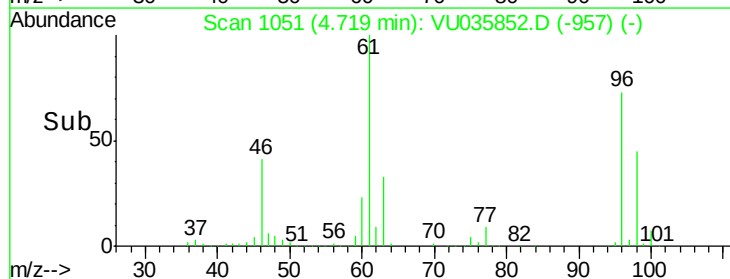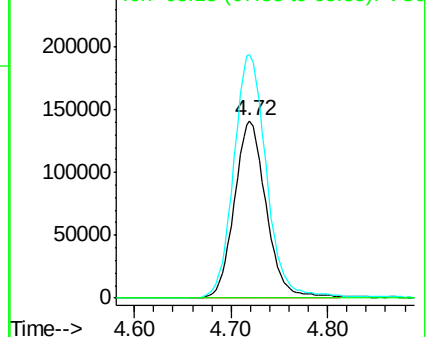

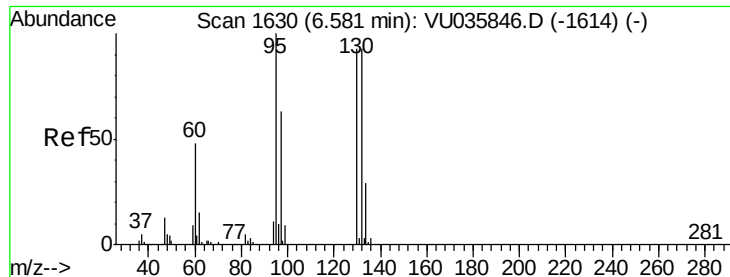

#34

Trichloroethene

Concen: 12.415 ug/L

RT: 6.58 min Scan# 1630

Delta R.T. 0.00 min

Lab File: VU035852.D

Acq: 26 Nov 2019 12:50

Instrument :

MSVOA_U

ClientSampleId :

GARE6DL

Tgt Ion: 95 Resp: 347741



Ion Ratio Lower Upper

95 100

97 62.3 45.1 83.9

132 87.9 61.9 114.9

130 90.8 66.3 123.1

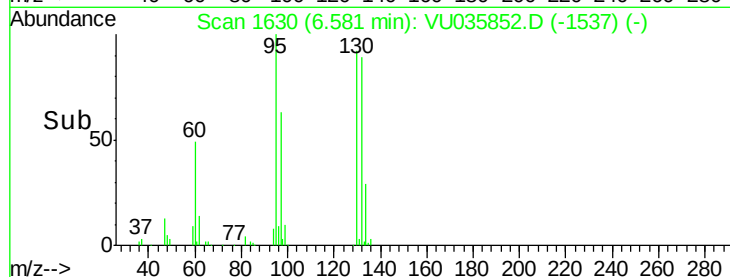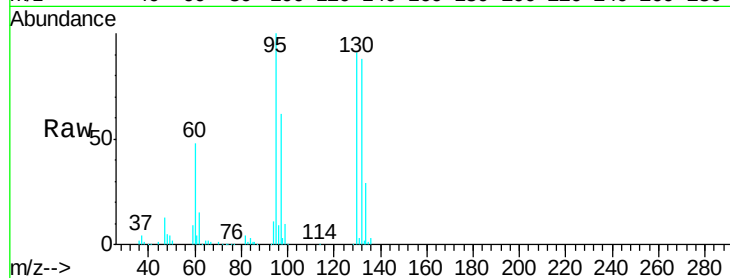

Abundance Ion 95.00 (94.70 to 95.70): VU0

Ion 96.95 (96.65 to 97.65): VU0

Ion 131.95 (131.65 to 132.65): V

Ion 129.95 (129.65 to 130.65): V

