

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU112619\
 Data File : VU035871.D
 Acq On : 26 Nov 2019 20:56
 Operator : JC/SP
 Sample : K6057-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AA3

Quant Time: Nov 27 04:16:08 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed Nov 27 03:16:13 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	222111	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	256860	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	73540	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.62	65	140834	4.85	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.00%
7) Chloroethane-d5	1.93	69	131343	5.23	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	104.60%
11) 1,1-Dichloroethene-d2	2.59	63	175892	3.26	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	65.20%
20) 2-Butanone-d5	4.69	46	270254	40.25	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	80.50%
24) Chloroform-d	5.12	84	214440	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.20%
26) 1,2-Dichloroethane-d4	5.75	65	127609	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.60%
32) Benzene-d6	5.77	84	449478	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.80%
36) 1,2-Dichloropropane-d6	6.74	67	154956	4.69	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	93.80%
41) Toluene-d8	7.93	98	349851	3.87	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	77.40%
43) trans-1,3-Dichloropropene-	8.21	79	47051	3.66	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.20%
46) 2-Hexanone-d5	8.69	63	228275	44.20	ug/L	0.01
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.40%
57) 1,1,2,2-Tetrachloroethane-	10.79	84	117360	4.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.40%
64) 1,2-Dichlorobenzene-d4	12.22	152	83985	5.26	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	105.20%


Target Compounds					Qvalue
13) Acetone	2.67	43	15162	2.571 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU112619\
Data File : VU035871.D
Acq On : 26 Nov 2019 20:56
Operator : JC/SP
Sample : K6057-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AA3

Quant Time: Nov 27 04:16:08 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed Nov 27 03:16:13 2019
Response via : Initial Calibration

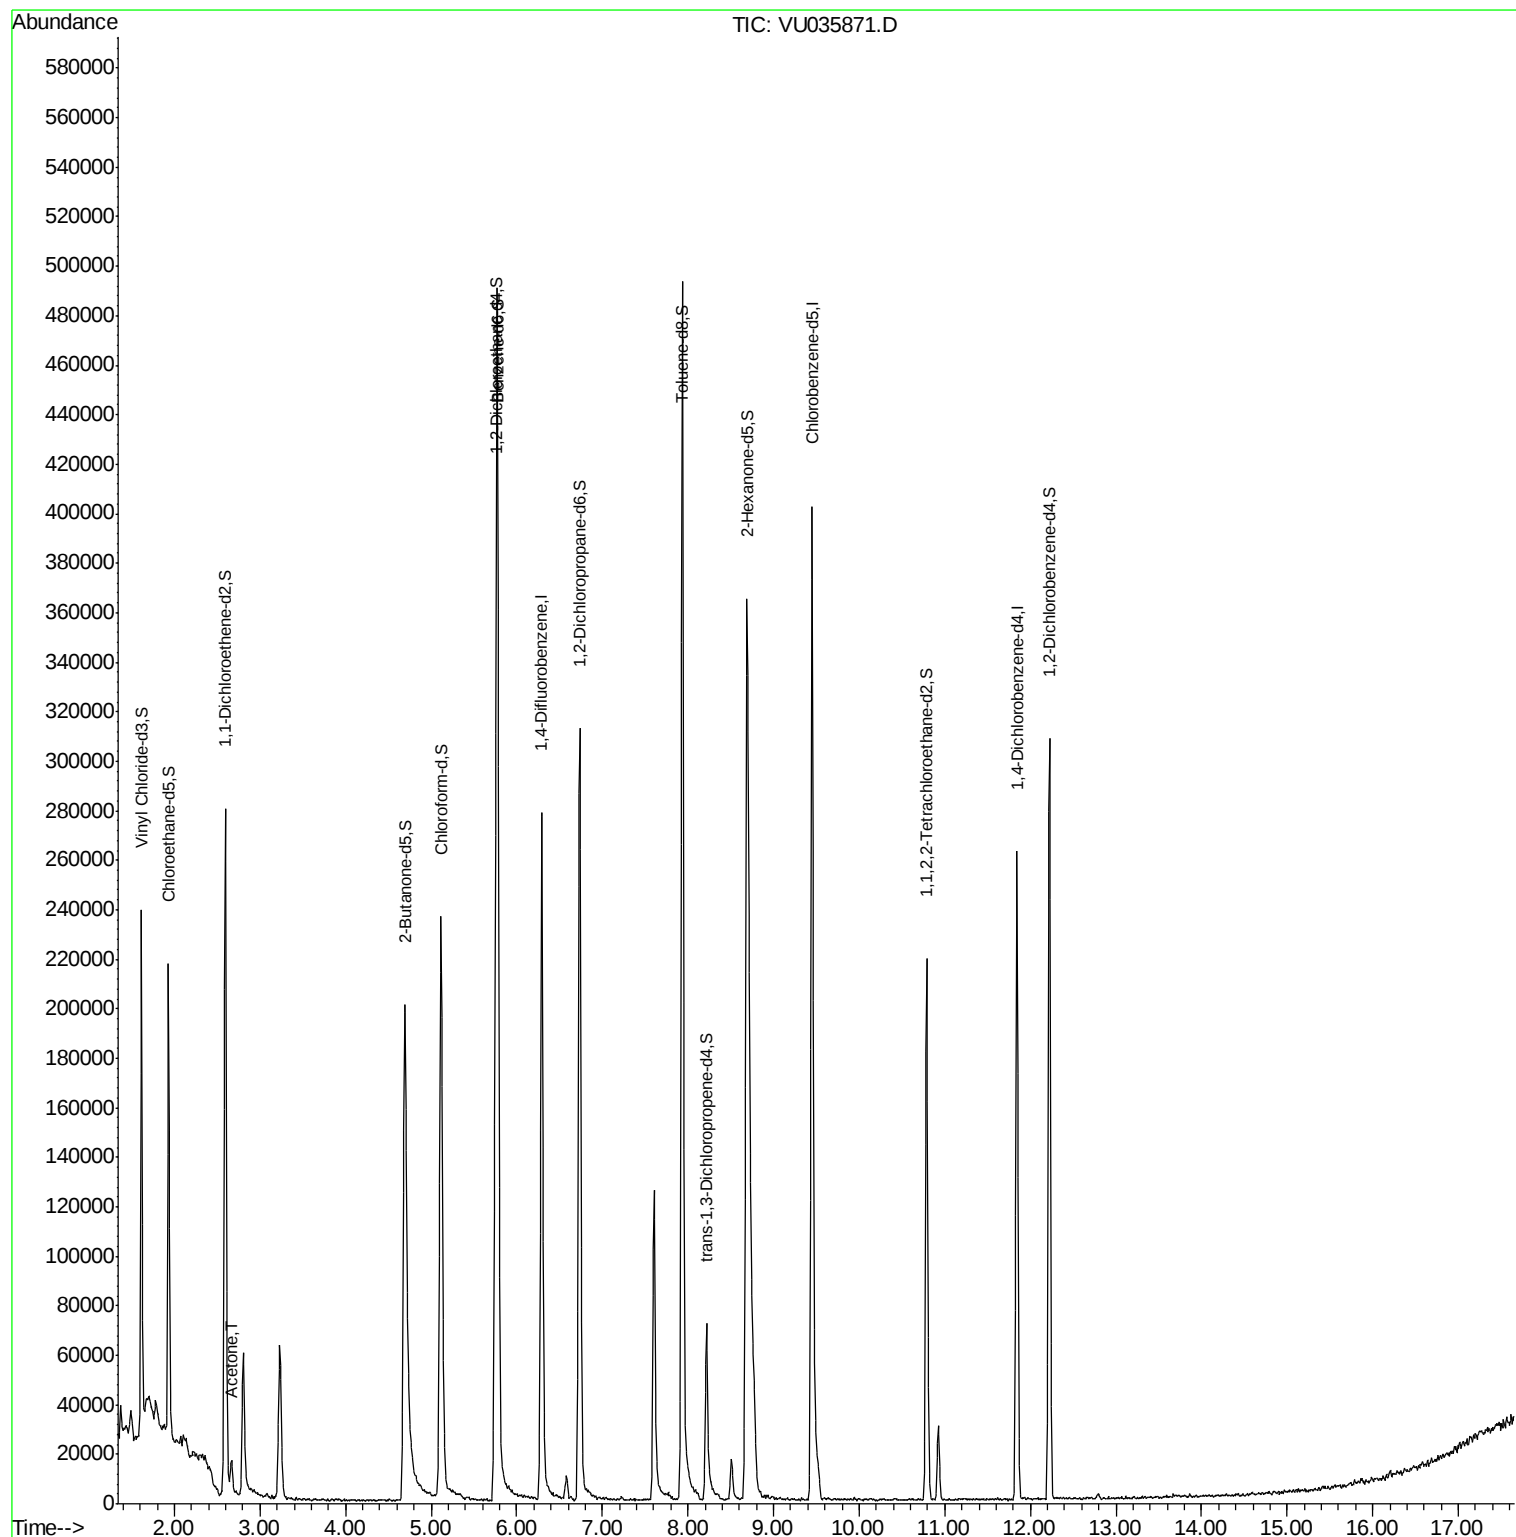

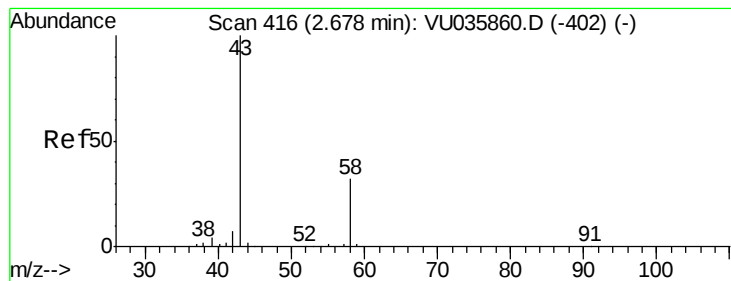

#13

Acetone

Concen: 2.571 ug/L

RT: 2.67 min Scan# 413

Delta R.T. -0.01 min

Lab File: VU035871.D

Acq: 26 Nov 2019 20:56

Instrument :

MSVOA_U

ClientSampleId :

C0AA3

Tgt Ion: 43 Resp: 15162

Ion Ratio Lower Upper

43 100

58 33.9 0.0 61.2

