


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU112619\
 Data File : VU035845.D
 Acq On : 26 Nov 2019 08:44
 Operator : JC/SP
 Sample : BFB06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB06

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed Nov 27 18:31:03 2019

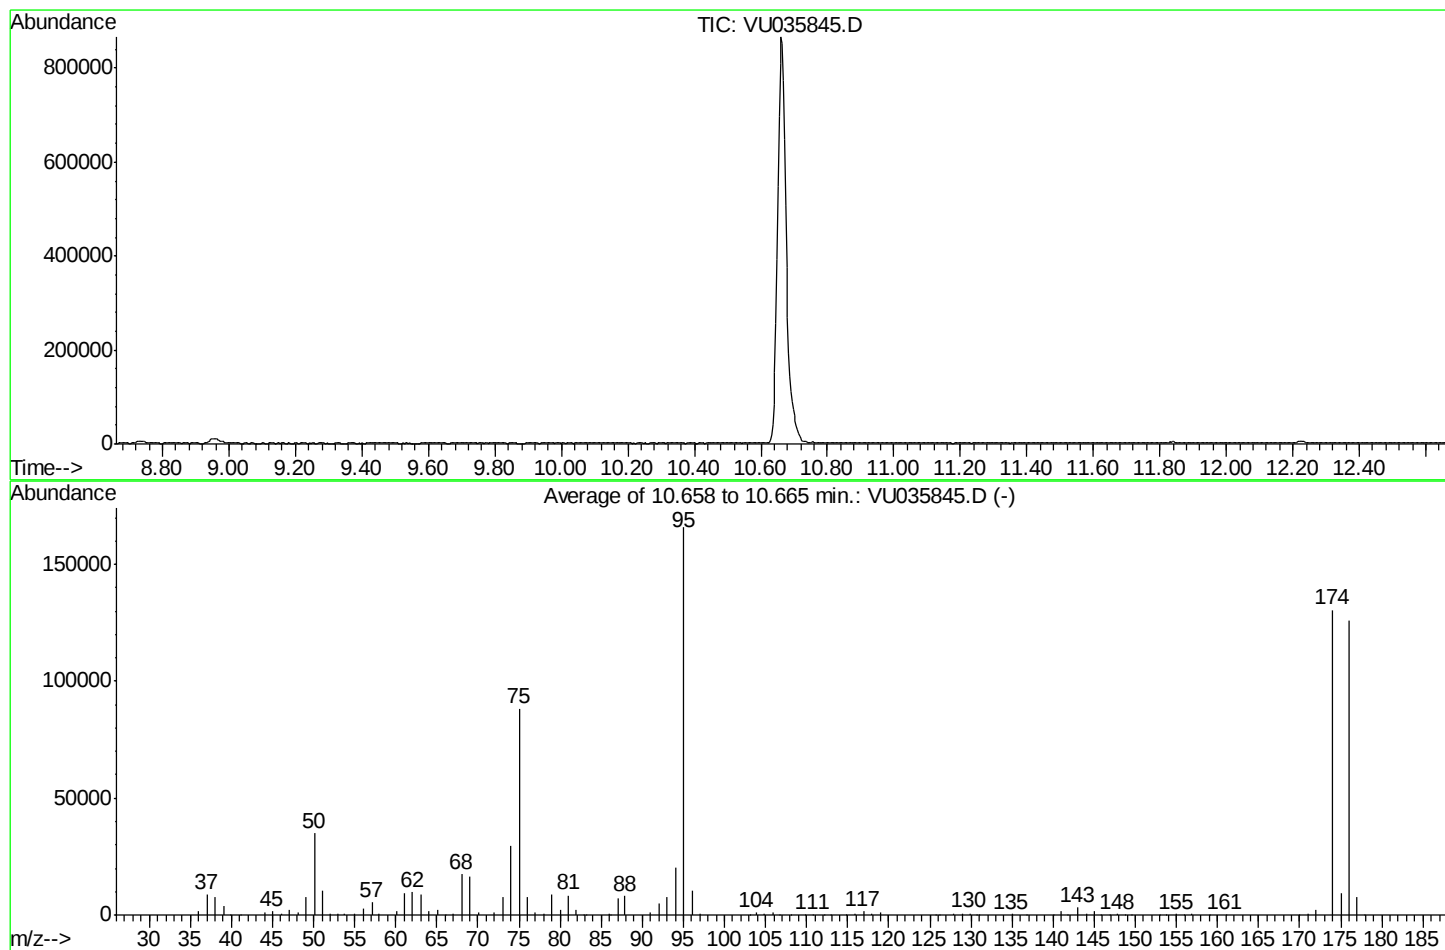

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	34917	PASS
75	95	30	80	53.2	88168	PASS
95	95	100	100	100.0	165824	PASS
96	95	5	9	6.3	10383	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.7	130541	PASS
175	174	5	9	7.0	9143	PASS
176	174	95	101	96.7	126173	PASS
177	176	5	9	6.2	7829	PASS

m/z	Abundance
36.00	1934.0
37.00	8976.0
38.00	8069.0
39.10	3674.0
40.00	617.0
41.10	106.0
44.10	2287.0
45.00	1680.0
46.10	552.0
47.00	2494.0
48.00	1404.0
49.10	8044.0
50.10	36032.0
51.00	10907.0
52.00	526.0
53.00	408.0
53.80	392.0
55.00	615.0
56.00	2541.0
57.10	5448.0
58.00	360.0
60.10	1892.0
61.00	9879.0
62.00	10003.0
63.00	8818.0
64.00	1836.0
65.10	2137.0
66.00	125.0
66.90	503.0
68.00	17848.0
69.00	16864.0
70.10	1342.0
72.00	1368.0
73.00	8029.0
74.00	30344.0
75.00	90096.0
76.10	7786.0
77.00	1079.0
78.00	753.0
79.00	8790.0
80.00	2188.0
81.00	8769.0
81.90	2067.0
82.80	133.0
85.90	507.0
87.00	7517.0
87.90	8645.0
90.90	881.0
92.00	4999.0
93.00	7763.0
94.00	20696.0
95.00	170624.0
96.00	10685.0
97.10	516.0
103.10	101.0
103.90	966.0
104.80	306.0
105.90	933.0
106.70	193.0
108.10	153.0
109.80	151.0
110.80	199.0
114.80	195.0
116.00	725.0
116.90	1498.0
117.80	613.0
119.00	1123.0
125.70	138.0
127.90	602.0
128.90	344.0
129.90	801.0
130.70	244.0
135.00	337.0
136.70	269.0
139.90	110.0
141.00	1687.0
141.80	283.0
143.00	3217.0
144.10	349.0
144.90	1439.0
145.90	254.0
147.00	111.0
147.90	302.0
148.70	104.0
152.90	176.0
153.80	183.0
155.10	431.0
155.90	133.0
156.90	391.0
159.00	206.0
161.00	193.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

170.90	734.0
171.90	2354.0
174.00	134144.0
175.00	9392.0
176.00	129544.0
177.00	8000.0
177.90	184.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

m/z	Abundance
36.00	1965.0
37.00	8445.0
38.00	7430.0
39.10	3054.0
39.90	554.0
41.10	123.0
44.00	2082.0
45.00	1542.0
46.00	455.0
47.00	2278.0
48.10	1266.0
49.10	7561.0
50.10	34224.0
51.10	10481.0
52.00	529.0
53.00	453.0
53.80	246.0
55.00	524.0
56.00	2476.0
57.10	5203.0
58.00	287.0
60.10	1816.0
61.00	9296.0
62.00	9890.0
63.00	8164.0
64.00	1735.0
65.10	2077.0
66.10	114.0
66.90	546.0
68.00	16640.0
69.00	16504.0
70.00	1427.0
72.00	1128.0
73.10	7694.0
74.00	28712.0
75.00	85928.0
76.10	7406.0
77.00	910.0
77.90	635.0
79.00	8402.0
80.00	2044.0
81.00	7750.0
81.90	1895.0
83.10	127.0
87.00	7091.0
87.90	7498.0
90.90	780.0
92.00	4689.0
93.00	7422.0
94.00	19968.0
95.10	159040.0
96.00	10208.0
97.10	504.0
103.90	839.0
104.80	312.0
105.90	832.0
106.80	181.0
108.10	105.0
109.80	116.0
110.80	156.0
112.90	115.0
114.80	176.0
116.00	764.0
116.90	1464.0
117.90	684.0
118.90	1103.0
125.70	105.0
126.20	103.0
127.90	468.0
129.00	492.0
129.80	632.0
130.70	215.0
131.00	229.0
135.00	309.0
136.70	236.0
140.00	184.0
141.00	1718.0
141.90	296.0
143.00	3155.0
144.10	273.0
144.90	1477.0
145.90	219.0
147.00	140.0
147.80	339.0
153.80	144.0
155.00	350.0
156.90	381.0
159.00	188.0
161.00	192.0
170.00	119.0
170.90	701.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

171.90	2203.0
174.00	123016.0
175.00	9053.0
176.00	119256.0
177.00	7821.0
177.90	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

m/z	Abundance
39.90	378.0
41.90	132.0
44.00	1092.0
51.00	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

m/z	Abundance
36.00	1758.0
37.00	8558.0
38.00	7878.0
39.10	4045.0
40.00	671.0
44.10	2447.0
45.00	1688.0
46.00	599.0
47.00	2383.0
48.00	1313.0
49.00	7747.0
50.10	34496.0
51.10	10395.0
52.00	513.0
52.90	354.0
53.80	394.0
55.00	583.0
56.10	2533.0
57.10	5226.0
58.00	377.0
60.10	1789.0
61.00	9391.0
62.10	9355.0
63.10	8704.0
64.10	1760.0
65.10	1925.0
66.00	166.0
66.90	488.0
68.00	18072.0
69.00	16370.0
70.10	1161.0
72.00	1408.0
73.00	7778.0
74.00	30040.0
75.10	88480.0
76.00	7462.0
77.00	1097.0
78.00	864.0
79.00	8369.0
80.00	2210.0
81.00	8681.0
81.90	2059.0
82.80	188.0
85.90	503.0
86.20	502.0
87.00	7514.0
87.90	8188.0
90.90	866.0
92.00	4958.0
93.00	7513.0
94.10	19408.0
95.00	167808.0
96.10	10256.0
97.00	425.0
103.10	143.0
103.90	1005.0
104.80	274.0
105.90	935.0
106.70	183.0
108.10	159.0
109.70	179.0
110.80	208.0
112.10	125.0
114.80	218.0
115.90	557.0
116.90	1456.0
117.80	626.0
119.00	1176.0
125.70	103.0
127.90	590.0
128.90	235.0
129.90	778.0
130.70	217.0
131.00	191.0
135.00	297.0
136.70	250.0
141.00	1434.0
141.70	251.0
143.00	2993.0
144.10	344.0
145.00	1303.0
145.80	304.0
146.90	100.0
147.90	363.0
149.60	174.0
153.00	232.0
153.80	181.0
155.10	449.0
155.90	208.0
156.90	324.0
159.00	199.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06

161.00	187.0
171.00	747.0
171.90	2314.0
174.00	134464.0
175.00	8986.0
176.00	129720.0
177.00	7666.0
177.80	202.0

Instrument :
MSVOA_U
ClientSampleId :
BFB06