


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112621\
 Data File : VU046008.D
 Acq On : 26 Nov 2021 09:37
 Operator : SY/MD
 Sample : BFB032
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB032

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111521WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Nov 26 23:26:55 2021

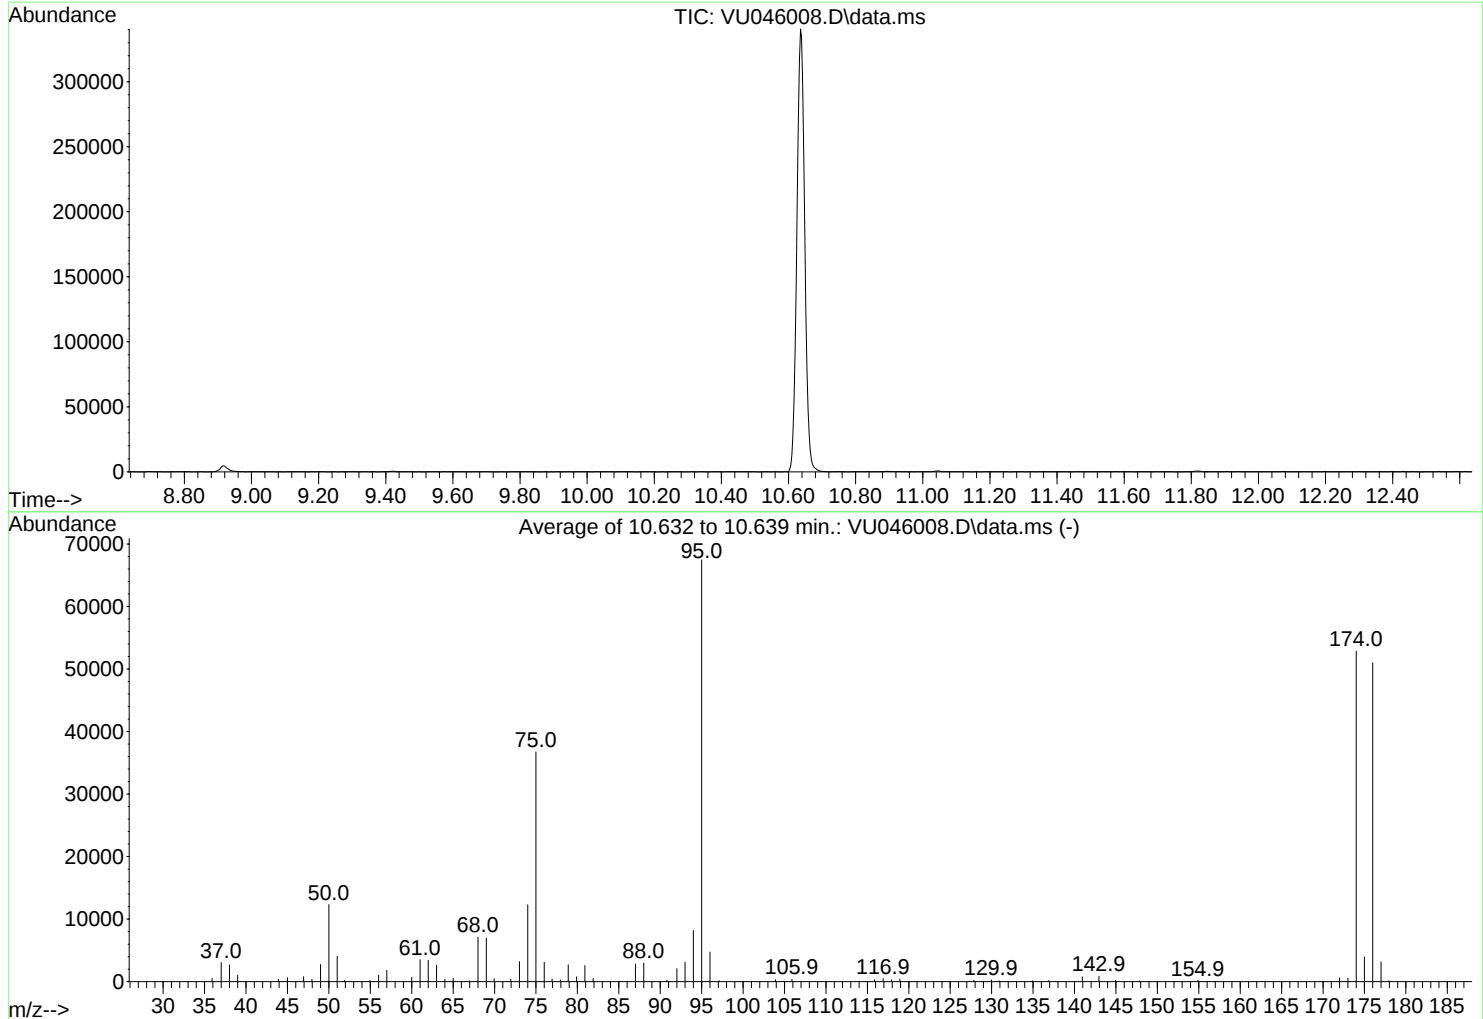

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2877

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	12330	PASS
75	95	30	80	54.5	36741	PASS
95	95	100	100	100.0	67461	PASS
96	95	5	9	7.0	4745	PASS
173	174	0.00	2	1.1	566	PASS
174	95	50	120	78.3	52840	PASS
175	174	5	9	7.4	3933	PASS
176	174	95	101	96.5	51013	PASS
177	176	5	9	6.2	3163	PASS

m/z	Abundance
43.90	104.0

Instrument :
MSVOA_U
ClientSampleId :
BFB032

m/z	Abundance
35.90	511.0
37.00	3002.0
38.00	2676.0
39.00	1001.0
40.00	100.0
43.90	507.0
45.00	650.0
47.00	856.0
47.90	313.0
49.00	2616.0
50.00	11938.0
51.00	4018.0
51.90	164.0
55.00	170.0
56.00	1049.0
57.00	1734.0
60.00	685.0
61.00	3248.0
62.00	3284.0
63.00	2613.0
64.00	344.0
65.00	528.0
67.00	176.0
68.00	7059.0
69.00	6782.0
70.00	421.0
72.00	366.0
73.00	3157.0
74.00	11833.0
75.00	34984.0
76.00	3005.0
76.90	411.0
78.00	272.0
78.90	2497.0
79.90	761.0
80.90	2505.0
81.90	554.0
87.00	2671.0
88.00	2832.0
90.80	264.0
92.00	2015.0
93.00	2972.0
94.00	7890.0
95.00	64800.0
96.00	4741.0
97.10	165.0
103.90	292.0
105.90	345.0
115.80	309.0
116.90	468.0
117.90	274.0
118.90	435.0
127.80	227.0
129.90	315.0
130.90	128.0
134.90	116.0
136.90	149.0
141.00	699.0
143.00	885.0
143.90	100.0
144.90	195.0
147.80	115.0
154.90	209.0
158.90	112.0
172.00	582.0
173.00	497.0
174.00	50080.0
175.00	3749.0
176.00	48168.0
177.00	2941.0
178.00	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB032

m/z	Abundance
35.90	555.0
37.00	3159.0
38.00	2782.0
39.00	1067.0
44.00	489.0
45.00	660.0
47.00	813.0
48.00	397.0
49.00	2784.0
50.00	12730.0
51.00	4154.0
51.90	187.0
54.90	174.0
56.00	1035.0
57.00	1867.0
60.00	700.0
61.00	3574.0
62.00	3497.0
63.00	2709.0
64.00	401.0
65.00	559.0
67.00	169.0
68.00	7340.0
69.00	7215.0
70.00	475.0
71.90	394.0
73.00	3256.0
74.00	12669.0
75.00	37984.0
76.00	3247.0
77.00	454.0
78.00	294.0
78.90	2809.0
79.90	794.0
80.90	2668.0
81.90	515.0
87.00	2910.0
88.00	3079.0
90.80	261.0
92.00	2119.0
93.00	3195.0
94.00	8368.0
95.00	69560.0
96.00	4923.0
97.10	161.0
103.90	315.0
104.90	103.0
105.90	385.0
115.90	331.0
116.90	502.0
117.90	319.0
118.90	475.0
127.80	239.0
128.80	112.0
129.90	311.0
130.90	125.0
134.90	130.0
136.90	182.0
141.00	805.0
143.00	874.0
145.00	196.0
147.90	128.0
154.90	219.0
157.00	122.0
158.90	111.0
172.00	625.0
173.00	589.0
174.00	54368.0
175.00	4066.0
176.00	52392.0
177.00	3179.0
178.00	135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB032

m/z	Abundance
35.90	521.0
37.00	2966.0
38.00	2596.0
39.00	1019.0
44.00	446.0
45.00	573.0
46.90	722.0
47.90	464.0
49.00	2787.0
50.00	12322.0
51.00	3956.0
51.90	187.0
54.90	161.0
56.00	995.0
57.00	1850.0
60.00	674.0
61.00	3698.0
62.00	3464.0
63.00	2626.0
64.00	435.0
65.00	494.0
66.90	142.0
68.00	6974.0
69.00	6922.0
69.90	485.0
71.90	414.0
73.00	3155.0
74.00	12362.0
75.00	37256.0
76.00	3026.0
77.00	482.0
77.90	288.0
78.90	2767.0
79.90	743.0
80.90	2577.0
81.90	465.0
87.00	2907.0
88.00	3004.0
90.80	241.0
92.00	2119.0
93.00	3169.0
94.00	8299.0
95.00	68024.0
96.00	4572.0
97.10	133.0
103.90	334.0
104.90	103.0
105.90	380.0
115.90	297.0
116.90	520.0
117.90	327.0
118.90	443.0
127.90	252.0
130.00	260.0
130.90	106.0
134.90	153.0
136.90	195.0
140.90	838.0
142.90	849.0
145.00	212.0
147.90	120.0
154.90	191.0
156.90	129.0
172.00	564.0
173.00	611.0
174.00	54072.0
175.00	3984.0
176.00	52480.0
177.00	3369.0
177.90	102.0

Instrument :
MSVOA_U
ClientSampleId :
BFB032