


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112718\
Data File : VU028341.D
Acq On : 27 Nov 2018 17:15
Operator : MD/SY
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\82U110218W.M
Title : SW846 8260
Last Update : Fri Nov 02 02:28:20 2018

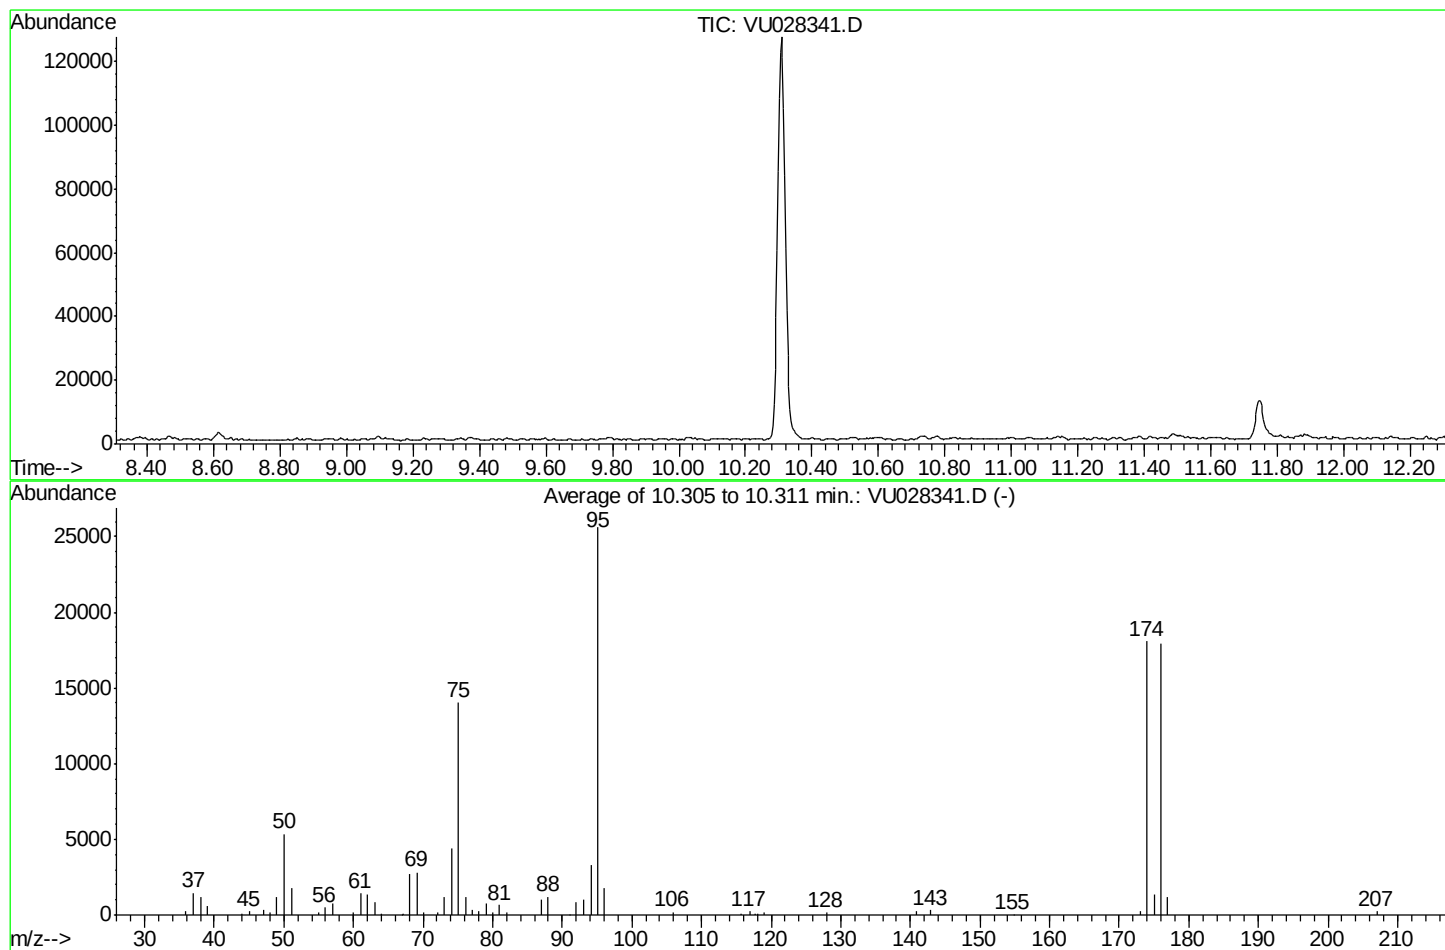

AutoFind: Scans 2840, 2841, 2842; Background Corrected with Scan 2828

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	5361	PASS
75	95	30	60	54.7	14023	PASS
95	95	100	100	100.0	25613	PASS
96	95	5	9	6.9	1770	PASS
173	174	0.00	2	1.3	238	PASS
174	95	50	100	70.7	18098	PASS
175	174	5	9	7.5	1360	PASS
176	174	95	101	99.2	17954	PASS
177	176	5	9	6.4	1151	PASS