

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U112719\
 Data File : VU035887.D
 Acq On : 27 Nov 2019 11:20
 Operator : JC/SP
 Sample : K6057-04
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AA3

Quant Time: Nov 29 03:40:56 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Nov 28 04:57:50 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.29	114	224911	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	262523	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	72856	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.62	65	136266	4.64	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	92.80%
7) Chloroethane-d5	1.93	69	128936	5.07	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	101.40%
11) 1,1-Dichloroethene-d2	2.60	63	170188	3.12	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.40%
20) 2-Butanone-d5	4.69	46	270479	39.78	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	79.56%
24) Chloroform-d	5.11	84	219290	4.41	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.20%
26) 1,2-Dichloroethane-d4	5.75	65	127324	4.56	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.20%
32) Benzene-d6	5.77	84	438471	4.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.60%
36) 1,2-Dichloropropane-d6	6.74	67	150057	4.45	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.00%
41) Toluene-d8	7.93	98	343020	3.71	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	74.20%
43) trans-1,3-Dichloropropene-	8.22	79	49942	3.80	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	76.00%
46) 2-Hexanone-d5	8.70	63	214008	40.54	ug/L	0.02
Spiked Amount	50.000	Range	45 - 130	Recovery	=	81.08%
57) 1,1,2,2-Tetrachloroethane-	10.79	84	118971	4.19	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	83.80%
64) 1,2-Dichlorobenzene-d4	12.22	152	77644	4.91	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.20%


Target Compounds					Ovalue
13) Acetone	2.67	43	10928	1.830 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU112719\
Data File : VU035887.D
Acq On : 27 Nov 2019 11:20
Operator : JC/SP
Sample : K6057-04
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AA3

Quant Time: Nov 29 03:40:56 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Nov 28 04:57:50 2019
Response via : Initial Calibration

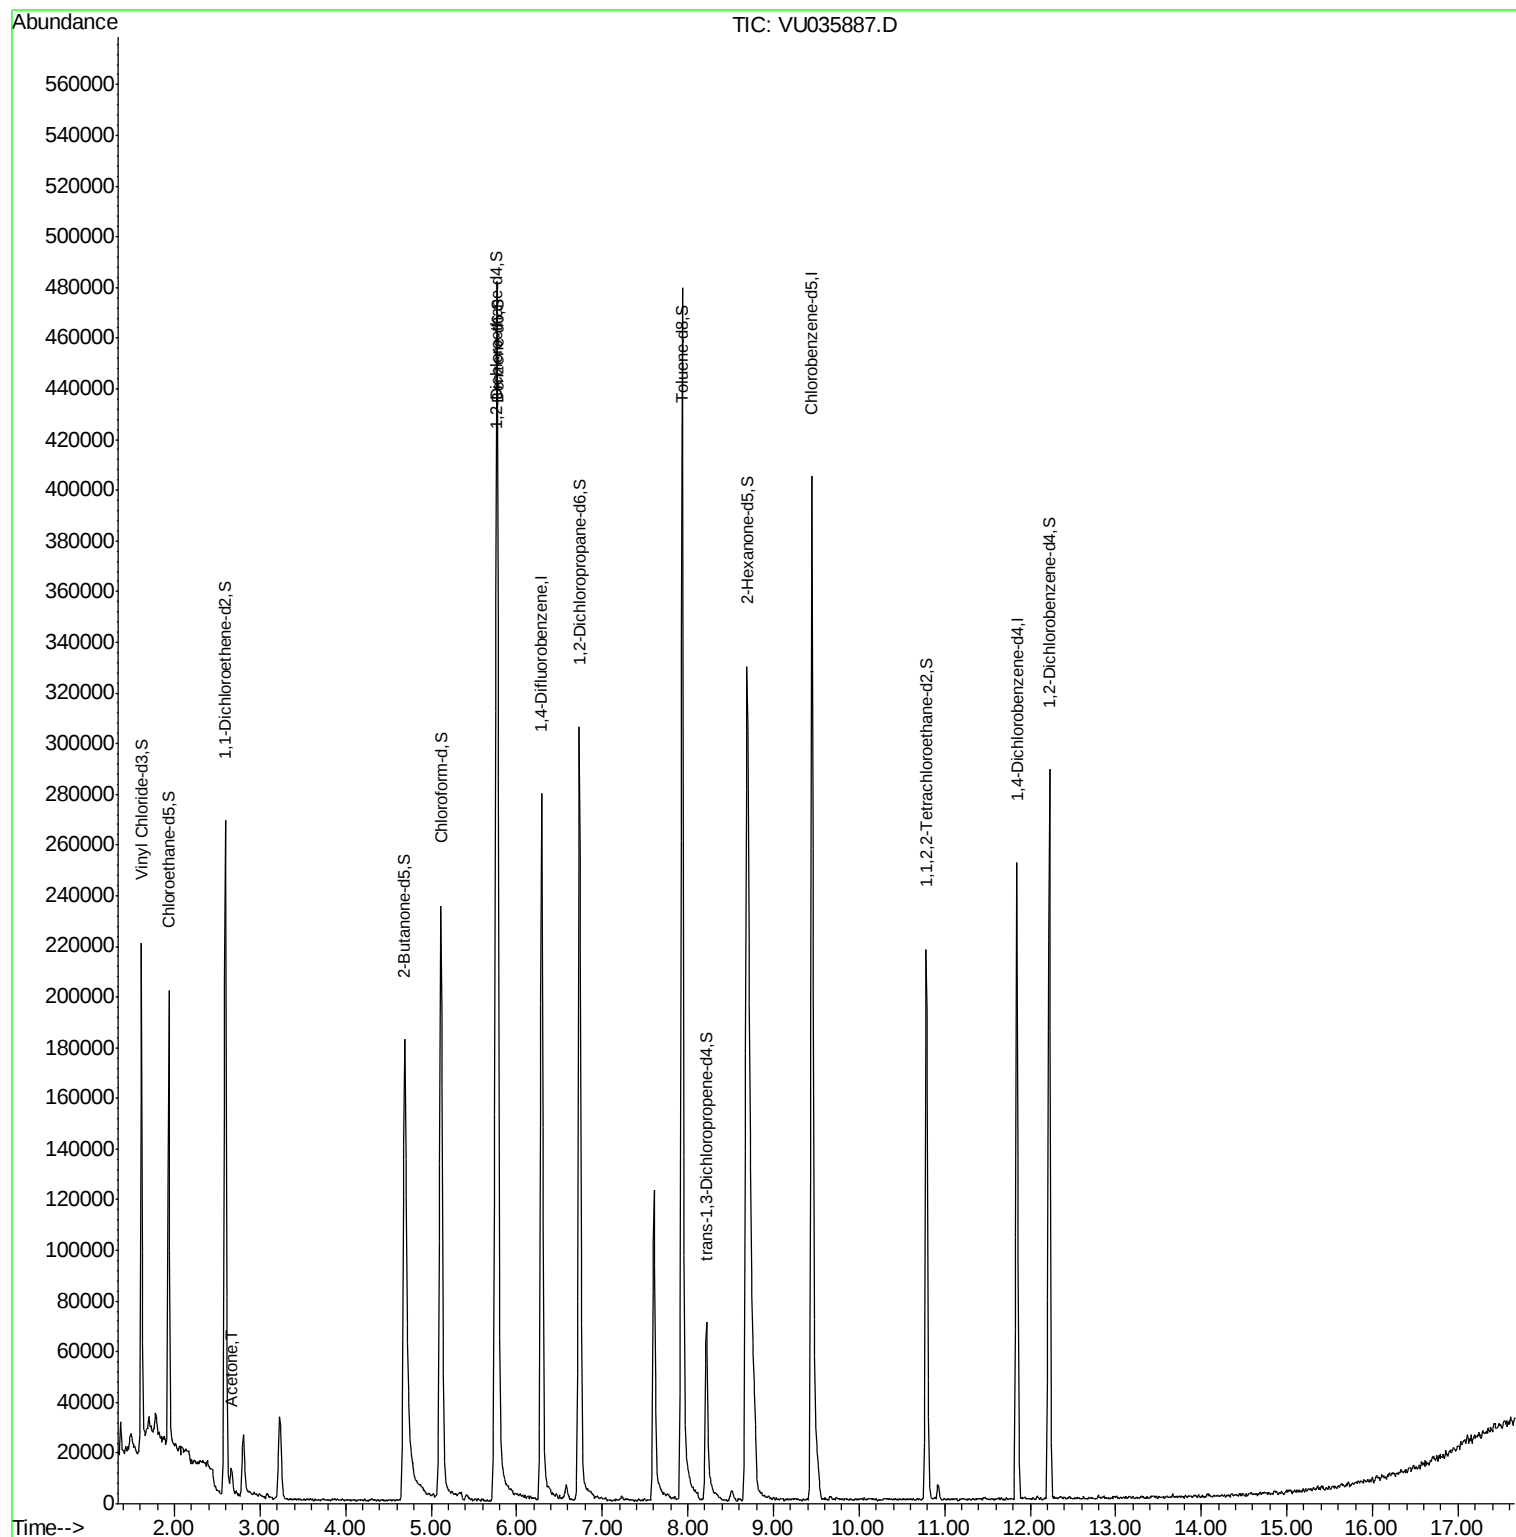

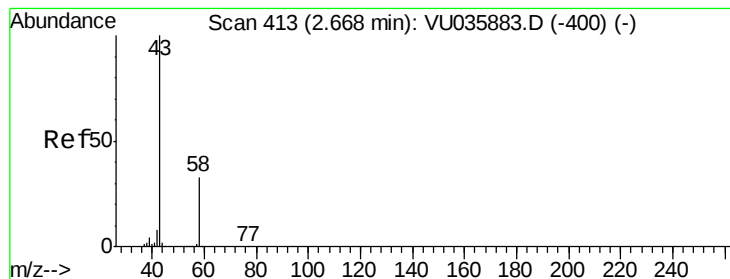

#13

Acetone

Concen: 1.830 ug/L

RT: 2.67 min Scan# 413

Delta R.T. 0.00 min

Lab File: VU035887.D

Acq: 27 Nov 2019 11:20

Instrument :

MSVOA_U

ClientSampleId :

C0AA3

Tot Ion: 43 Resp: 10928

Ion Ratio Lower Upper

43 100

58 35.3 0.0 61.2

