

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U112719\
 Data File : VU035897.D
 Acq On : 27 Nov 2019 15:21
 Operator : JC/SP
 Sample : K6057-11
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AB0

Quant Time: Nov 29 04:07:42 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Nov 28 04:57:50 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.30	114	234950	5.00	ug/L	0.00
28) Chlorobenzene-d5	9.45	117	268203	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.84	152	74690	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.62	65	130713	4.26	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.20%
7) Chloroethane-d5	1.93	69	124594	4.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.80%
11) 1,1-Dichloroethene-d2	2.60	63	165356	2.90	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	58.00%#
20) 2-Butanone-d5	4.69	46	335844	47.28	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	94.56%
24) Chloroform-d	5.12	84	223679	4.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.00%
26) 1,2-Dichloroethane-d4	5.75	65	127343	4.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.20%
32) Benzene-d6	5.77	84	440202	4.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.00%
36) 1,2-Dichloropropane-d6	6.74	67	150141	4.35	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.00%
41) Toluene-d8	7.93	98	339689	3.60	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	72.00%
43) trans-1,3-Dichloropropene-	8.21	79	49419	3.68	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	73.60%
46) 2-Hexanone-d5	8.69	63	259676	48.15	ug/L	0.01
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.30%
57) 1,1,2,2-Tetrachloroethane-	10.79	84	126663	4.36	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	87.20%
64) 1,2-Dichlorobenzene-d4	12.22	152	81023	4.99	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.80%


Target Compounds					Ovalue
13) Acetone	2.67	43	17009	2.727 ug/L	96
14) Carbon disulfide	2.83	76	32796	0.404 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU112719\
Data File : VU035897.D
Acq On : 27 Nov 2019 15:21
Operator : JC/SP
Sample : K6057-11
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AB0

Quant Time: Nov 29 04:07:42 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Nov 28 04:57:50 2019
Response via : Initial Calibration

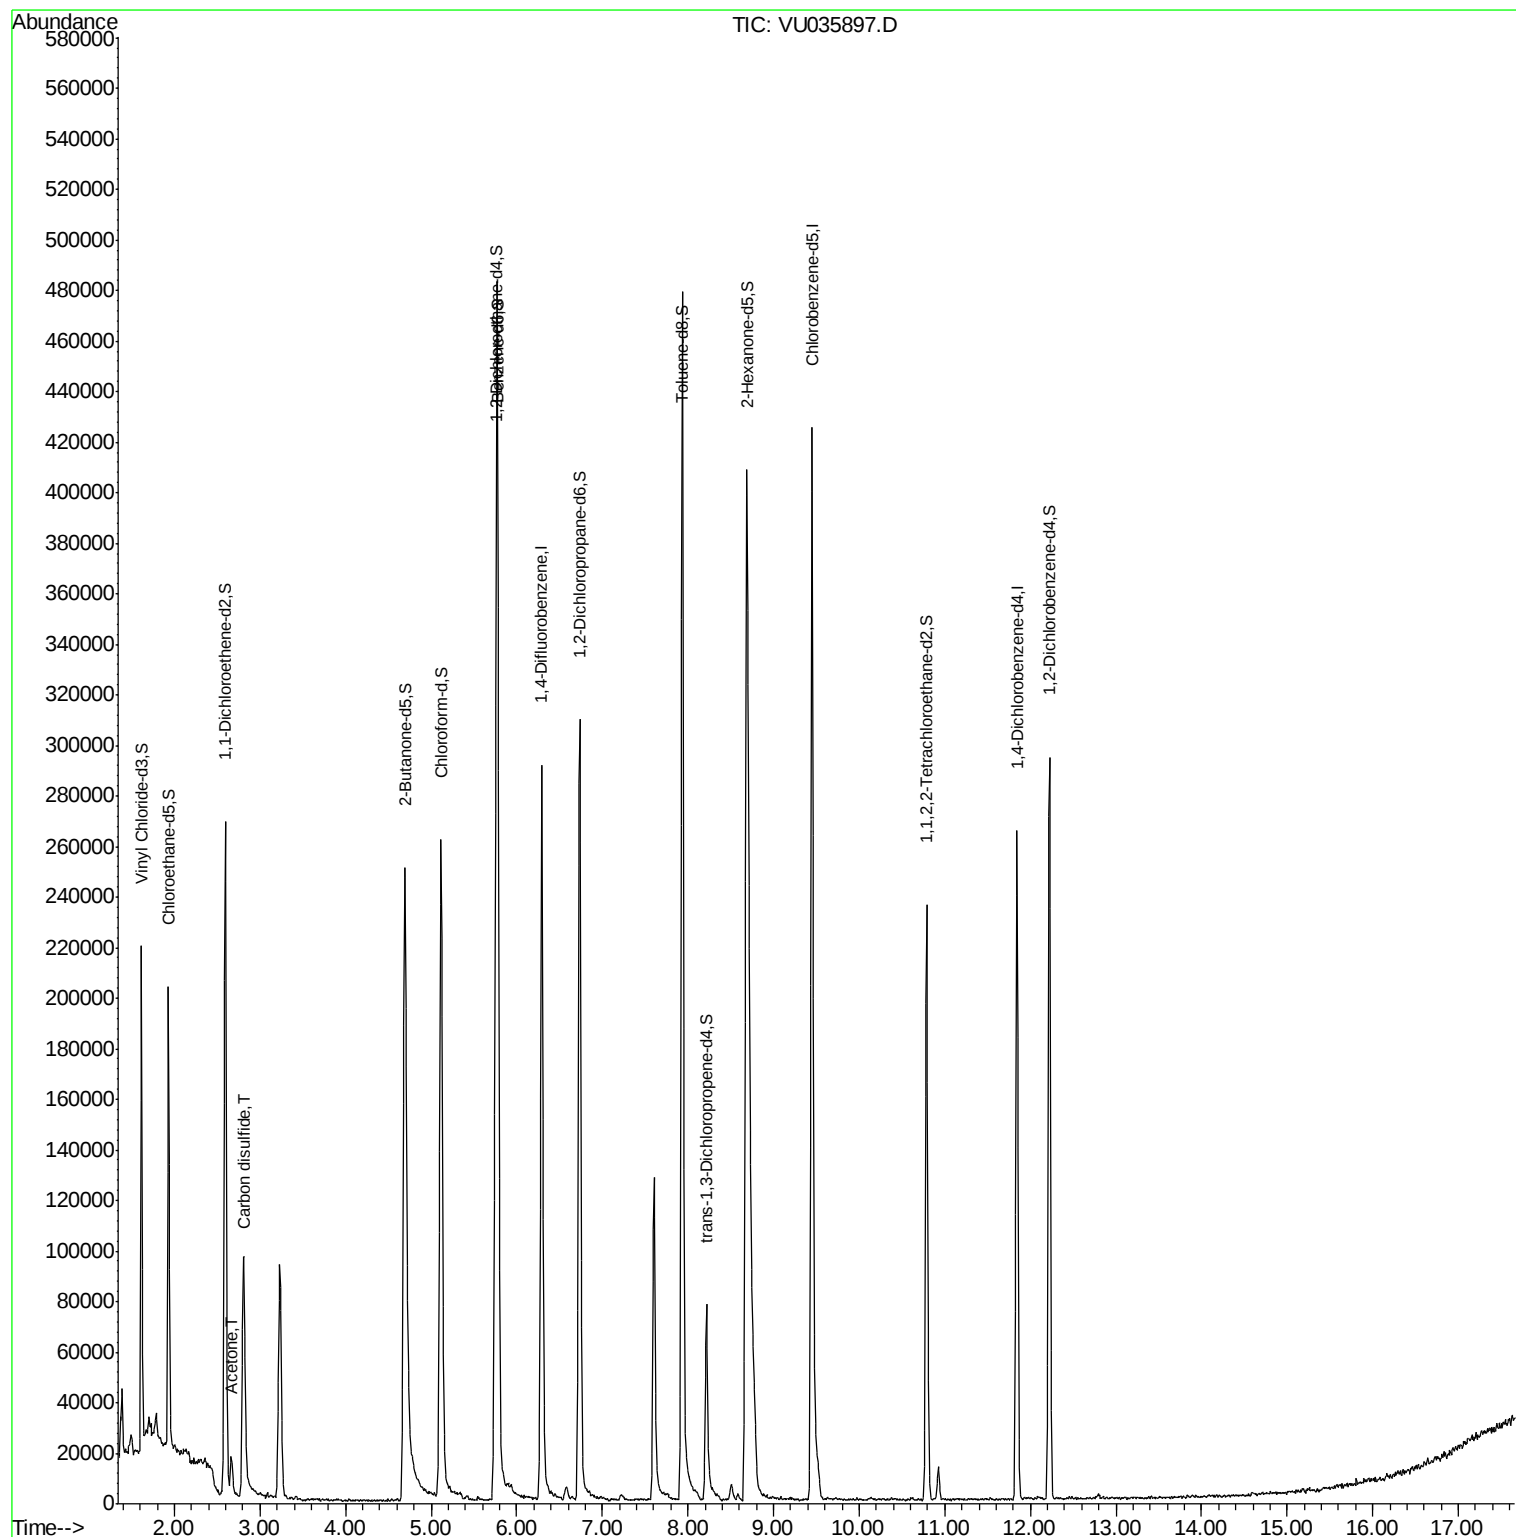

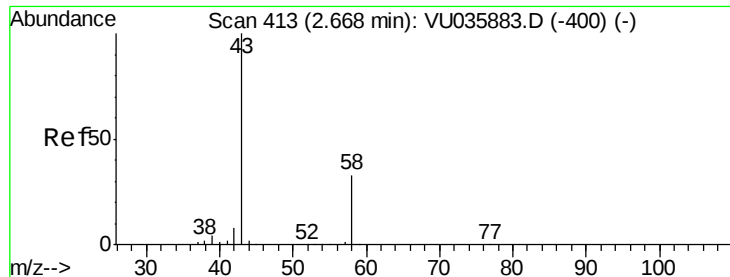

#13

Acetone

Concen: 2.727 ug/L

RT: 2.67 min Scan# 413

Delta R.T. 0.00 min

Lab File: VU035897.D

Acq: 27 Nov 2019 15:21

Instrument :

MSVOA_U

ClientSampleId :


C0AB0

Tot Ion: 43 Resp: 17009

Ion Ratio Lower Upper




43 100

58 32.9 0.0 61.2

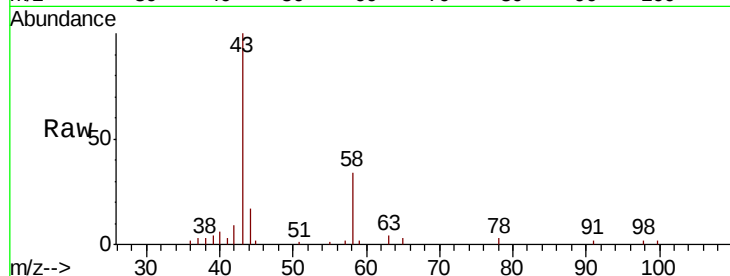

Abundance Ion 43.05 (42.75 to 43.75): VU035897.D (-320) (-)

Ion 58.05 (57.75 to 58.75): VU035897.D (-320) (-)

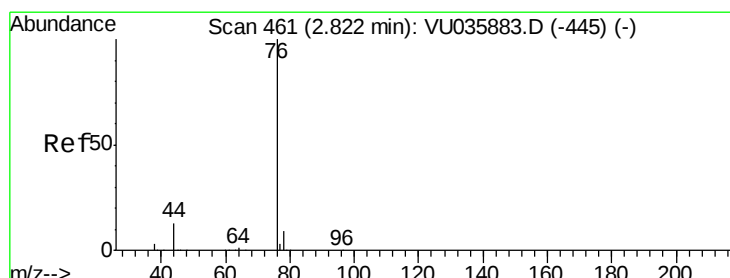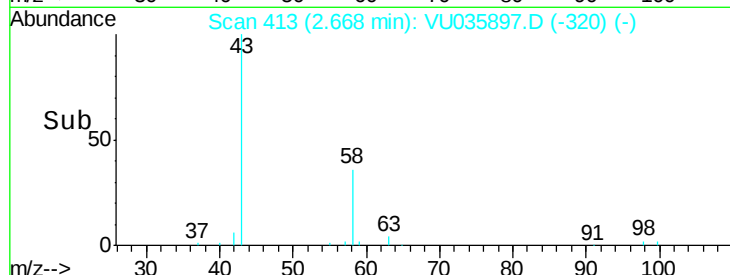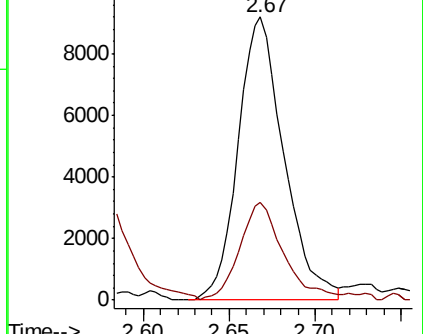

#14

Carbon disulfide

Concen: 0.404 ug/L

RT: 2.83 min Scan# 462

Delta R.T. 0.00 min

Lab File: VU035897.D


Acq: 27 Nov 2019 15:21

Tgt Ion: 76 Resp: 32796

Ion Ratio Lower Upper

76 100

78 8.7 7.3 10.9

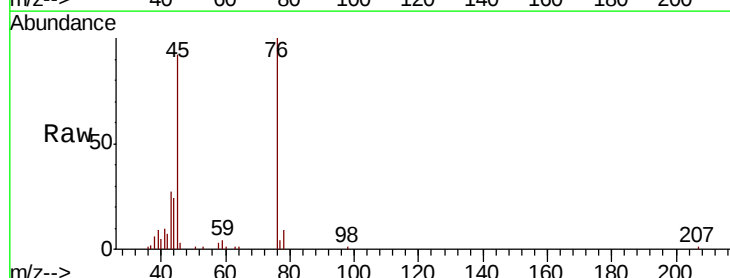

Abundance Ion 76.05 (75.75 to 76.75): VU035897.D (-368) (-)

Ion 78.00 (77.70 to 78.70): VU035897.D (-368) (-)

