


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU112719\
Data File : VU035882.D
Acq On : 27 Nov 2019 08:37
Operator : JC/SP
Sample : BFB07
Misc : 25.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB07

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR112119WMA.M
Title : TRACE VOA SOM01.0
Last Update : Thu Nov 28 04:57:50 2019

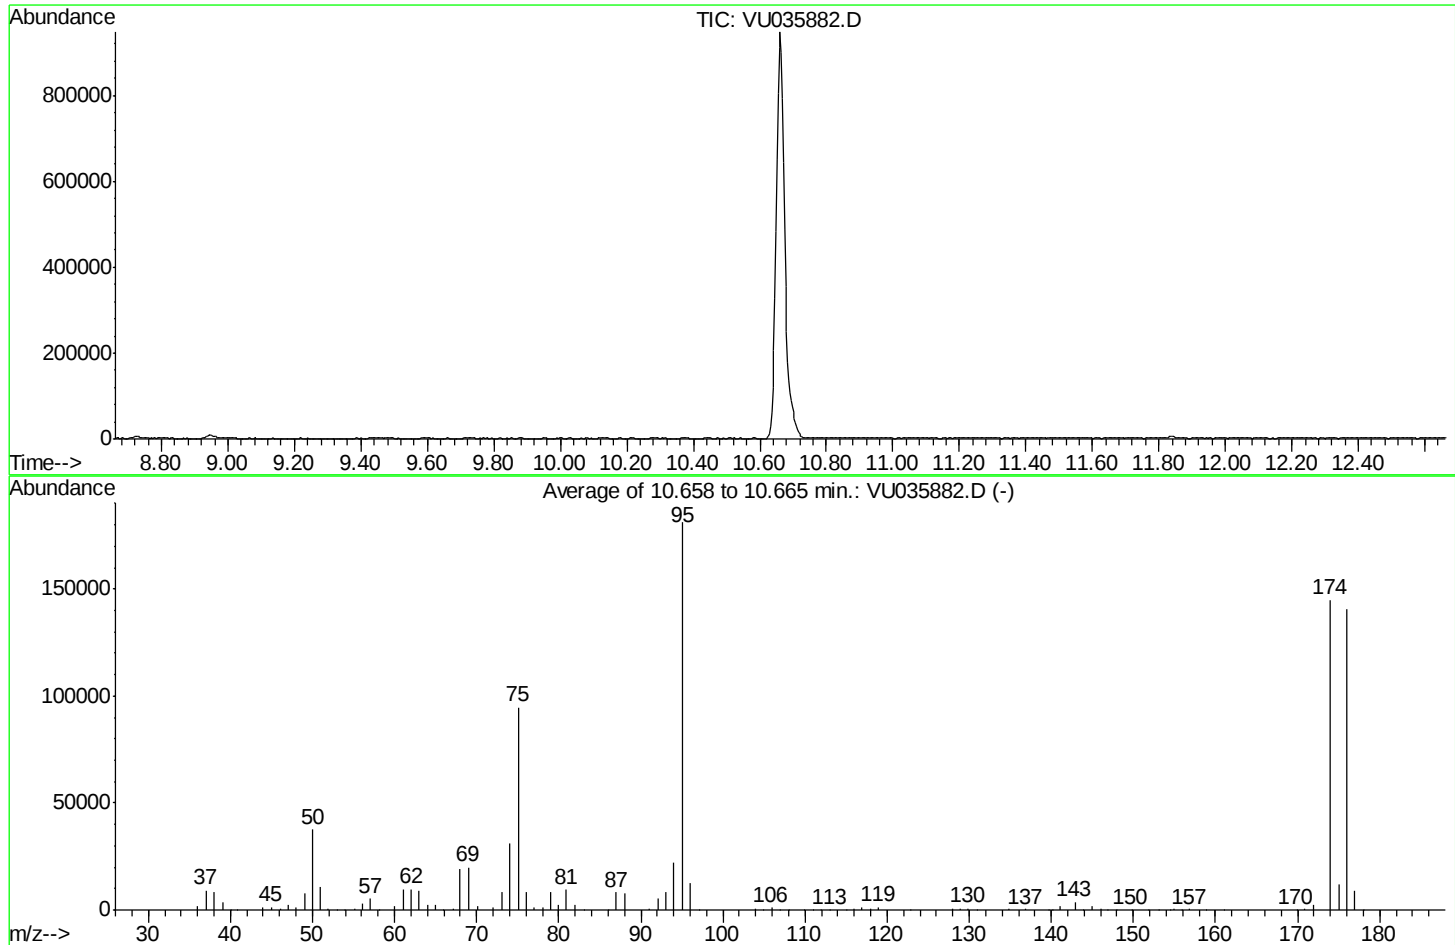

AutoFind: Scans 2898, 2899, 2900; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	37538	PASS
75	95	30	80	52.2	94597	PASS
95	95	100	100	100.0	181162	PASS
96	95	5	9	6.9	12410	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	79.9	144768	PASS
175	174	5	9	8.1	11735	PASS
176	174	95	101	97.3	140800	PASS
177	176	5	9	6.4	9047	PASS

m/z	Abundance
36.00	1754.0
37.00	9018.0
38.00	8843.0
39.00	3659.0
39.90	717.0
40.80	230.0
44.00	2157.0
45.00	1216.0
46.00	374.0
47.10	2624.0
48.00	1409.0
49.10	7776.0
50.10	37240.0
51.00	10751.0
52.00	480.0
53.00	311.0
53.90	316.0
55.10	658.0
56.00	3294.0
57.10	5357.0
58.00	312.0
60.00	1709.0
61.00	9416.0
62.00	9909.0
63.00	9190.0
64.00	2189.0
65.00	2087.0
66.00	259.0
67.10	538.0
68.00	19400.0
69.00	20504.0
70.10	1651.0
71.90	1057.0
73.10	8416.0
74.00	31080.0
75.00	94088.0
76.10	8415.0
77.00	1425.0
78.00	1012.0
79.00	8466.0
80.00	2082.0
80.90	9188.0
81.90	2303.0
83.00	164.0
86.00	215.0
87.00	8375.0
88.00	7164.0
91.00	924.0
92.10	5152.0
93.10	8250.0
94.00	21768.0
95.10	180864.0
96.00	12292.0
97.00	267.0
103.90	824.0
104.90	241.0
106.00	843.0
106.90	194.0
108.00	100.0
110.90	171.0
111.90	164.0
113.00	201.0
115.90	862.0
116.90	1429.0
118.00	685.0
119.00	1420.0
122.80	116.0
127.90	574.0
128.90	356.0
129.90	673.0
131.00	337.0
134.90	369.0
136.90	276.0
140.10	196.0
141.00	1636.0
142.90	3819.0
143.90	257.0
145.00	2081.0
146.00	311.0
148.00	258.0
149.70	283.0
151.80	159.0
153.00	192.0
154.90	407.0
155.90	126.0
156.80	440.0
158.80	302.0
161.00	241.0
169.90	238.0
170.80	589.0
172.00	2193.0
174.00	142144.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

175.00	11637.0
176.00	137728.0
177.00	9043.0
178.00	189.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

m/z	Abundance
36.00	1712.0
37.00	9339.0
38.00	9055.0
39.10	3776.0
40.00	707.0
40.90	189.0
44.00	2161.0
45.00	1375.0
46.10	362.0
47.10	2576.0
48.00	1443.0
49.00	7770.0
50.00	38856.0
51.00	10810.0
51.90	463.0
53.00	310.0
53.90	245.0
55.10	626.0
56.10	3267.0
57.00	5595.0
58.10	311.0
60.00	1756.0
61.00	10171.0
62.10	10007.0
63.00	9521.0
64.00	2204.0
65.00	2298.0
65.90	221.0
67.10	615.0
68.00	19872.0
69.00	20448.0
70.00	1780.0
72.00	1207.0
73.10	8538.0
74.00	31832.0
75.00	97072.0
76.10	8548.0
77.10	1331.0
78.00	1037.0
79.00	9069.0
80.00	2285.0
81.00	9651.0
81.90	2188.0
83.00	190.0
86.00	329.0
87.00	8450.0
88.00	7969.0
91.00	968.0
92.10	5651.0
93.00	8903.0
94.00	22904.0
95.10	186048.0
96.00	12772.0
97.10	323.0
103.90	985.0
104.90	250.0
105.90	1027.0
106.90	128.0
108.10	174.0
110.90	147.0
111.90	166.0
113.00	212.0
115.00	141.0
115.90	774.0
116.90	1413.0
118.00	780.0
119.00	1467.0
128.00	649.0
128.90	376.0
129.90	676.0
130.90	332.0
134.80	337.0
136.90	387.0
139.70	158.0
140.00	186.0
141.00	1624.0
142.90	4024.0
143.80	259.0
144.90	2085.0
146.00	384.0
146.80	109.0
148.00	252.0
149.80	343.0
151.80	133.0
153.00	278.0
154.40	188.0
154.90	419.0
155.90	181.0
156.90	457.0
158.80	319.0
161.00	122.0
169.90	231.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

170.90	630.0
172.00	2479.0
174.00	148992.0
175.00	12236.0
176.00	144704.0
177.00	9313.0
178.00	218.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

m/z	Abundance
36.00	1618.0
37.00	8641.0
38.00	8163.0
39.10	3601.0
40.10	765.0
40.90	120.0
44.00	1950.0
45.00	1367.0
46.10	378.0
47.10	2379.0
47.90	1201.0
49.00	7271.0
50.00	36520.0
51.00	10150.0
51.90	463.0
53.00	276.0
53.80	171.0
55.10	570.0
56.10	2990.0
57.10	5090.0
58.10	235.0
60.00	1793.0
61.00	9619.0
62.10	9563.0
63.00	8779.0
64.00	2089.0
65.00	2231.0
65.90	198.0
67.10	639.0
68.00	18952.0
69.00	18664.0
70.00	1754.0
72.00	1282.0
73.10	7998.0
74.00	30352.0
75.10	92632.0
76.10	7726.0
77.10	1268.0
78.00	916.0
78.90	8549.0
80.00	2277.0
81.00	9199.0
81.90	2055.0
83.00	185.0
86.00	381.0
87.00	7556.0
88.00	7568.0
90.90	761.0
92.10	5524.0
93.00	8708.0
94.00	21744.0
95.10	176576.0
96.00	12168.0
97.10	349.0
103.90	918.0
105.00	246.0
105.90	1012.0
106.80	118.0
108.00	202.0
109.90	127.0
110.90	106.0
111.80	147.0
113.10	229.0
114.90	221.0
115.90	617.0
116.90	1404.0
118.00	738.0
119.00	1490.0
128.00	655.0
128.90	314.0
129.90	633.0
130.90	223.0
134.80	311.0
136.90	450.0
139.70	152.0
140.00	158.0
141.00	1599.0
142.90	3764.0
143.80	247.0
144.90	1929.0
146.00	337.0
146.80	127.0
148.00	279.0
149.80	315.0
151.80	110.0
153.00	271.0
155.00	373.0
155.90	195.0
156.90	363.0
158.80	301.0
169.90	199.0
170.90	645.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

172.00	2547.0
174.00	143168.0
175.00	11334.0
176.00	139968.0
177.00	8785.0
178.00	242.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07

Scan 2884 (10.613 min): VU035882.D
BFB07

m/z	Abundance
40.00	490.0
44.00	880.0

Instrument :
MSVOA_U
ClientSampleId :
BFB07