
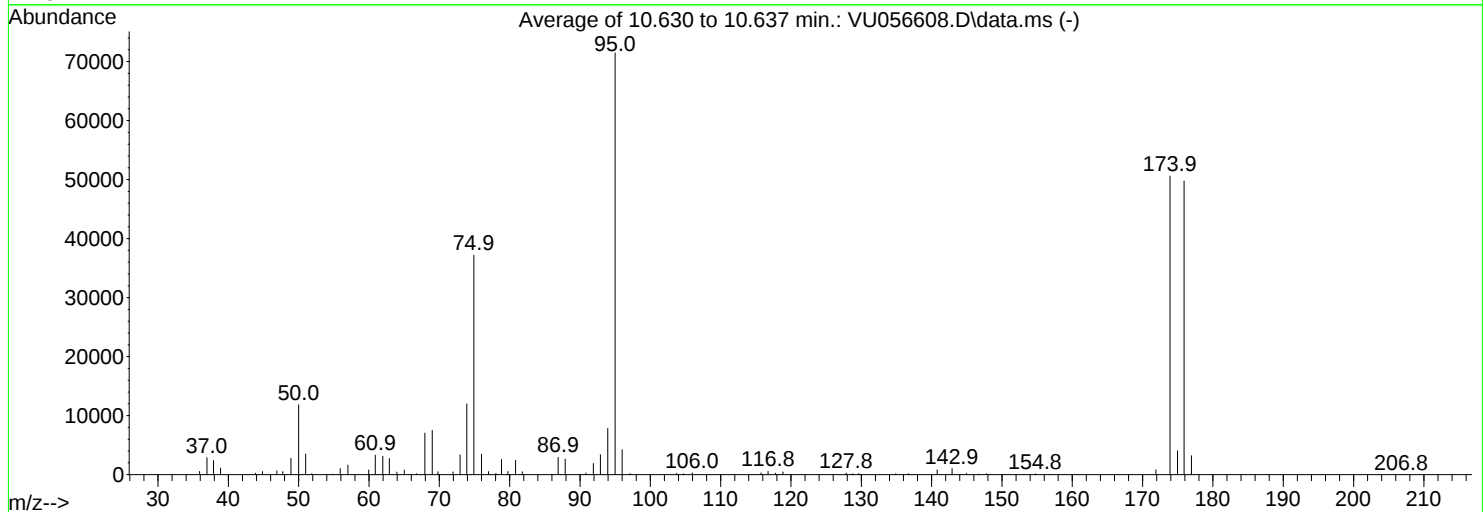


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112723\
Data File : VU056608.D
Acq On : 27 Nov 2023 09:37
Operator : MD/SY
Sample : BFB082
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB082

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Nov 27 22:31:27 2023

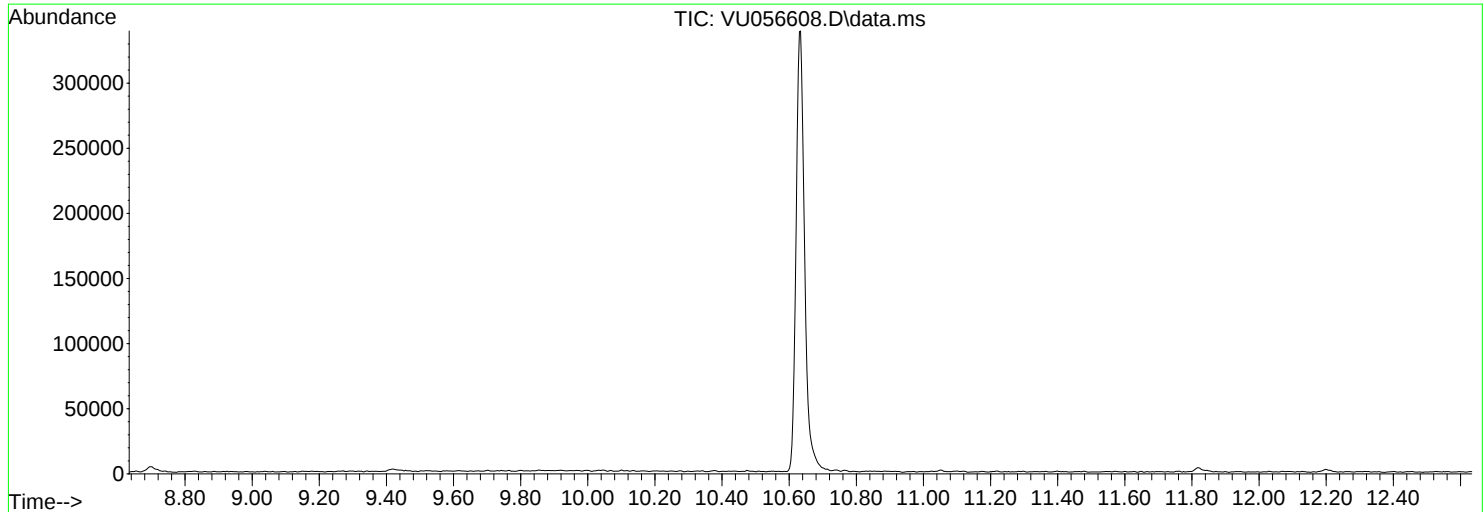

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2891

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.6	11860	PASS
75	95	30	80	52.0	37173	PASS
95	95	100	100	100.0	71475	PASS
96	95	5	9	5.9	4230	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.8	50605	PASS
175	174	5	9	8.0	4029	PASS
176	174	95	101	98.3	49749	PASS
177	176	5	9	6.4	3206	PASS

m/z	Abundance
35.90	1048.0
37.80	422.0
39.90	147.0
43.80	352.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082

m/z	Abundance
36.00	1749.0
36.90	3109.0
38.00	3161.0
38.90	1212.0
39.80	168.0
43.90	558.0
44.90	527.0
47.00	846.0
47.70	521.0
48.90	2813.0
50.00	12064.0
51.00	3701.0
51.90	152.0
54.90	164.0
55.90	1081.0
57.00	1767.0
60.00	946.0
60.90	3536.0
62.00	3209.0
62.90	2839.0
63.90	487.0
65.00	864.0
66.80	180.0
68.00	7039.0
69.00	7997.0
69.80	554.0
72.00	535.0
73.00	3714.0
73.90	12217.0
74.90	38048.0
76.00	3434.0
77.00	456.0
78.00	364.0
78.90	2664.0
79.70	580.0
80.90	2623.0
81.80	516.0
86.00	101.0
86.90	2868.0
87.90	2843.0
90.90	268.0
91.90	2131.0
92.90	3588.0
93.90	8220.0
95.00	72872.0
96.00	4247.0
97.10	158.0
103.80	318.0
104.70	164.0
105.90	287.0
114.90	118.0
115.70	312.0
116.80	596.0
117.80	275.0
118.90	502.0
127.90	279.0
128.80	132.0
129.60	292.0
134.90	126.0
136.80	137.0
140.80	760.0
142.90	1137.0
144.90	213.0
147.80	193.0
154.70	136.0
160.80	101.0
171.90	824.0
173.90	51304.0
175.00	3994.0
175.90	50472.0
176.90	3158.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082

m/z	Abundance
36.00	1654.0
36.90	2971.0
37.90	2883.0
38.90	1152.0
39.80	177.0
43.90	639.0
44.90	538.0
46.90	595.0
47.80	499.0
48.90	2909.0
50.00	12309.0
51.00	3507.0
51.90	144.0
54.80	120.0
55.90	1053.0
57.00	1666.0
60.00	808.0
60.90	3452.0
62.00	3148.0
62.90	2910.0
63.90	445.0
65.00	814.0
66.70	176.0
67.90	7304.0
69.00	7810.0
69.80	504.0
72.00	486.0
72.90	3518.0
73.90	12385.0
74.90	38200.0
76.00	3549.0
77.00	576.0
78.10	323.0
78.90	2606.0
79.80	555.0
80.90	2475.0
81.80	530.0
86.00	128.0
86.90	3104.0
87.90	2676.0
90.80	257.0
91.90	1991.0
92.90	3528.0
93.90	7913.0
95.00	73416.0
96.00	4294.0
97.10	217.0
103.70	239.0
104.70	157.0
106.00	294.0
115.80	308.0
116.80	574.0
117.80	245.0
118.80	476.0
127.90	272.0
128.80	195.0
129.70	258.0
134.90	185.0
136.80	174.0
140.80	875.0
142.90	1042.0
144.90	218.0
146.70	115.0
147.80	177.0
154.70	147.0
171.90	845.0
173.90	51944.0
174.90	4217.0
175.90	50840.0
177.00	3254.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082

m/z	Abundance
36.00	1414.0
37.00	2552.0
37.90	2432.0
38.90	1017.0
39.80	208.0
43.90	635.0
44.80	462.0
46.00	102.0
46.80	507.0
47.80	520.0
48.90	2600.0
50.00	11207.0
51.00	3273.0
51.80	161.0
55.90	1008.0
57.00	1443.0
59.90	644.0
60.90	2933.0
61.90	3020.0
62.90	2485.0
64.00	389.0
65.00	634.0
66.70	125.0
67.90	6779.0
69.00	6739.0
69.80	445.0
71.90	367.0
72.90	2877.0
73.90	11351.0
74.90	35272.0
76.00	3314.0
77.00	538.0
78.80	2369.0
79.80	495.0
80.80	2139.0
81.80	436.0
86.90	2828.0
87.90	2367.0
90.80	270.0
91.90	1616.0
92.90	3091.0
94.00	7304.0
95.00	68136.0
96.00	4150.0
97.10	193.0
103.80	178.0
104.70	104.0
105.90	287.0
115.80	313.0
116.70	507.0
117.80	196.0
118.80	434.0
127.80	261.0
128.80	202.0
129.90	207.0
134.90	199.0
136.70	165.0
140.80	818.0
142.90	894.0
145.00	201.0
146.70	115.0
147.80	136.0
154.80	135.0
156.80	142.0
171.90	801.0
173.90	48568.0
174.90	3877.0
175.90	47936.0
177.00	3206.0
206.80	105.0

Instrument :
MSVOA_U
ClientSampleId :
BFB082