

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052142.D
 Acq On : 28 Nov 2022 12:43
 Operator : JC/MD
 Sample : VU1128WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK034

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

Signal : TIC: VU052142.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	96	rBV	246788	286965	16.21%	2.182%
2	1.906	167	176	197	rBV	172953	260677	14.72%	1.982%
3	2.417	333	335	338	rBV3	972	575	0.03%	0.004%
4	2.565	368	381	398	rBV	378842	615773	34.78%	4.683%
5	2.784	445	449	450	rBV3	795	496	0.03%	0.004%
6	2.851	466	470	475	rBV2	873	894	0.05%	0.007%
7	2.925	490	493	499	rVB2	566	525	0.03%	0.004%
8	2.964	499	505	508	rBV4	710	784	0.04%	0.006%
9	3.044	519	530	546	rVB6	5590	12969	0.73%	0.099%
10	3.141	556	560	562	rBV2	643	535	0.03%	0.004%
11	3.179	564	572	589	rVB3	4634	10282	0.58%	0.078%
12	3.260	595	597	602	rVB2	657	512	0.03%	0.004%
13	3.292	602	607	610	rBV	668	631	0.04%	0.005%
14	3.314	611	614	618	rVB2	608	466	0.03%	0.004%
15	3.443	647	654	658	rBV3	516	603	0.03%	0.005%
16	3.501	668	672	678	rVV3	378	434	0.02%	0.003%
17	3.543	680	685	691	rVB3	651	680	0.04%	0.005%
18	3.623	706	710	714	rVB2	603	519	0.03%	0.004%
19	3.870	782	787	790	rBV2	568	468	0.03%	0.004%
20	4.015	829	832	834	rBV2	524	382	0.02%	0.003%
21	4.057	840	845	848	rBV2	373	350	0.02%	0.003%
22	4.385	940	947	950	rBV2	430	521	0.03%	0.004%
23	4.472	970	974	981	rBV2	510	580	0.03%	0.004%
24	4.539	992	995	998	rBV	458	358	0.02%	0.003%
25	4.616	1008	1019	1060	rBV	170216	416931	23.55%	3.171%
26	5.060	1140	1157	1181	rBV	316126	693337	39.16%	5.272%
27	5.198	1198	1200	1206	rBV4	437	382	0.02%	0.003%
28	5.292	1218	1229	1230	rBV3	1460	1852	0.10%	0.014%
29	5.362	1248	1251	1258	rVB3	763	847	0.05%	0.006%
30	5.449	1274	1278	1283	rVV	505	386	0.02%	0.003%
31	5.523	1298	1301	1305	rBV3	662	468	0.03%	0.004%
32	5.722	1341	1363	1386	rBV2	656098	1770419	100.00%	13.463%
33	6.018	1449	1455	1457	rBV3	561	615	0.03%	0.005%
34	6.112	1478	1484	1487	rBV3	410	474	0.03%	0.004%
35	6.247	1512	1526	1555	rBV	547664	1044569	59.00%	7.943%
36	6.446	1585	1588	1591	rVB2	715	553	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052142.D
 Acq On : 28 Nov 2022 12:43
 Operator : JC/MD
 Sample : VU1128WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK034

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

37	6.523	1608	1612	1613	rBV3	1158	794	0.04%	0.006%
38	6.687	1649	1663	1693	rBV	407052	800676	45.23%	6.089%
39	6.809	1698	1701	1709	rVB4	1320	1295	0.07%	0.010%
40	7.066	1778	1781	1787	rVB3	424	408	0.02%	0.003%
41	7.105	1787	1793	1795	rBV	487	382	0.02%	0.003%
42	7.253	1832	1839	1847	rBV2	505	849	0.05%	0.006%
43	7.375	1873	1877	1883	rBV3	693	734	0.04%	0.006%
44	7.562	1923	1935	1956	rBV2	202082	356193	20.12%	2.709%
45	7.697	1972	1977	1979	rBV2	643	451	0.03%	0.003%
46	7.774	1996	2001	2004	rBV3	573	597	0.03%	0.005%
47	7.796	2004	2008	2015	rVB4	981	1071	0.06%	0.008%
48	7.835	2015	2020	2023	rBV	584	526	0.03%	0.004%
49	7.896	2023	2039	2066	rBV	765490	1332902	75.29%	10.136%
50	8.176	2115	2126	2150	rBV	141645	239974	13.55%	1.825%
51	8.510	2228	2230	2238	rVB3	487	400	0.02%	0.003%
52	8.546	2238	2241	2242	rBV	611	350	0.02%	0.003%
53	8.555	2242	2244	2248	rVB3	799	517	0.03%	0.004%
54	8.629	2255	2267	2302	rBV	485664	898417	50.75%	6.832%
55	9.057	2395	2400	2404	rVB2	539	444	0.03%	0.003%
56	9.308	2475	2478	2484	rBV2	496	628	0.04%	0.005%
57	9.414	2498	2511	2537	rBV	788188	1297150	73.27%	9.864%
58	9.562	2554	2557	2558	rBV	813	407	0.02%	0.003%
59	9.632	2577	2579	2583	rVB3	677	402	0.02%	0.003%
60	9.658	2583	2587	2592	rVB2	941	871	0.05%	0.007%
61	9.690	2592	2597	2599	rBV3	1121	1103	0.06%	0.008%
62	9.838	2640	2643	2647	rVV3	427	378	0.02%	0.003%
63	10.263	2771	2775	2778	rBV2	405	376	0.02%	0.003%
64	10.388	2807	2814	2816	rBV2	406	482	0.03%	0.004%
65	10.574	2869	2872	2877	rBV2	393	423	0.02%	0.003%
66	10.632	2885	2890	2891	rBV	599	441	0.02%	0.003%
67	10.751	2914	2927	2949	rBV	592892	970001	54.79%	7.376%
68	10.896	2969	2972	2983	rVB4	824	1130	0.06%	0.009%
69	11.092	3030	3033	3036	rBV3	556	417	0.02%	0.003%
70	11.208	3064	3069	3073	rBV2	606	549	0.03%	0.004%
71	11.330	3100	3107	3109	rBV2	545	709	0.04%	0.005%
72	11.410	3128	3132	3137	rBV3	574	524	0.03%	0.004%
73	11.433	3137	3139	3146	rVB2	437	379	0.02%	0.003%
74	11.468	3146	3150	3154	rBV3	844	781	0.04%	0.006%
75	11.603	3188	3192	3198	rVB3	482	511	0.03%	0.004%
76	11.664	3203	3211	3216	rBV2	542	881	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052142.D
 Acq On : 28 Nov 2022 12:43
 Operator : JC/MD
 Sample : VU1128WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK034

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

77	11.748	3231	3237	3240	rBV3	845	944	0.05%	0.007%
78	11.809	3244	3256	3274	rBV	635729	1005232	56.78%	7.644%
79	11.954	3299	3301	3305	rVB3	1167	584	0.03%	0.004%
80	11.973	3305	3307	3312	rBV3	468	351	0.02%	0.003%
81	12.192	3361	3375	3402	rBV	642666	1077705	60.87%	8.195%
82	12.545	3479	3485	3494	rVB2	673	1054	0.06%	0.008%
83	13.143	3667	3671	3674	rBV3	449	390	0.02%	0.003%
84	13.195	3684	3687	3689	rBV2	603	385	0.02%	0.003%
85	13.227	3691	3697	3704	rVB6	1660	2280	0.13%	0.017%
86	13.307	3719	3722	3726	rBV3	447	377	0.02%	0.003%
87	13.407	3750	3753	3758	rVB3	629	563	0.03%	0.004%
88	13.507	3780	3784	3788	rVB2	658	544	0.03%	0.004%
89	13.606	3811	3815	3820	rVV2	569	495	0.03%	0.004%
90	13.664	3826	3833	3837	rBV3	777	792	0.04%	0.006%
91	13.696	3837	3843	3847	rBV4	607	778	0.04%	0.006%
92	13.822	3878	3882	3883	rBV2	499	370	0.02%	0.003%
93	13.848	3884	3890	3896	rVV4	2054	2500	0.14%	0.019%
94	14.002	3935	3938	3943	rBV3	470	549	0.03%	0.004%
95	14.089	3958	3965	3975	rBV5	3466	6328	0.36%	0.048%
96	14.211	4000	4003	4006	rBV3	692	449	0.03%	0.003%
97	14.330	4034	4040	4041	rBV4	2681	2272	0.13%	0.017%
98	14.577	4114	4117	4123	rBV4	953	953	0.05%	0.007%
99	14.831	4194	4196	4201	rBV3	550	434	0.02%	0.003%
100	15.581	4426	4429	4431	rBV3	749	482	0.03%	0.004%




Sum of corrected areas: 13150146

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052142.D
Acq On : 28 Nov 2022 12:43
Operator : JC/MD
Sample : VU1128WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK034

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

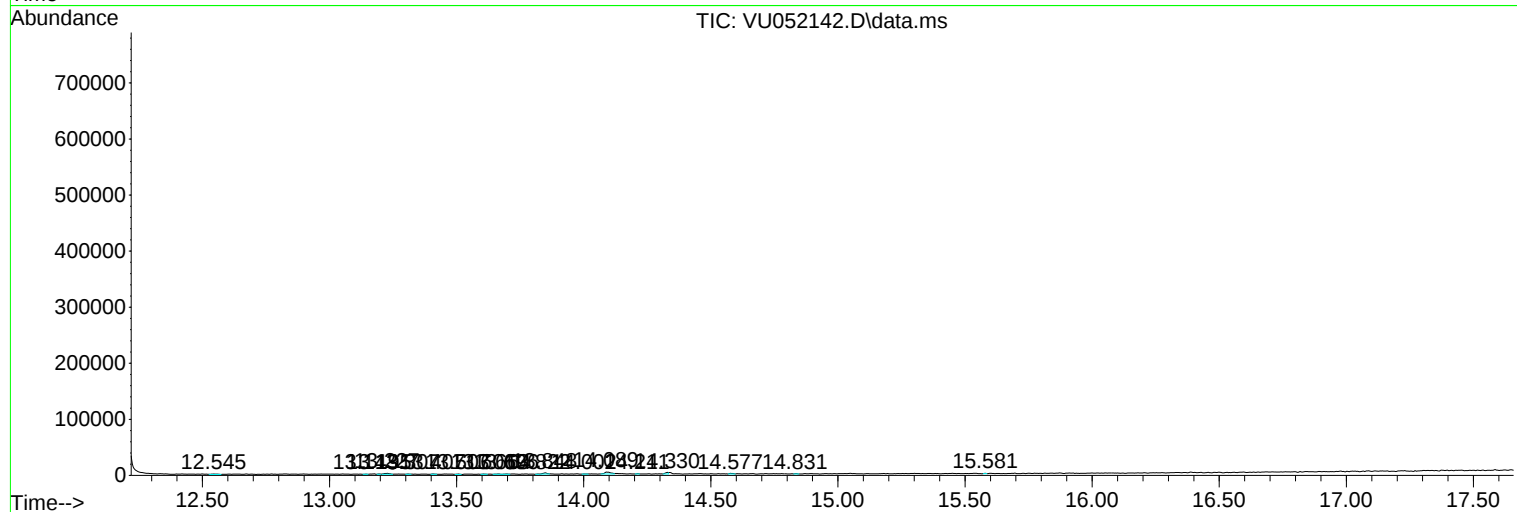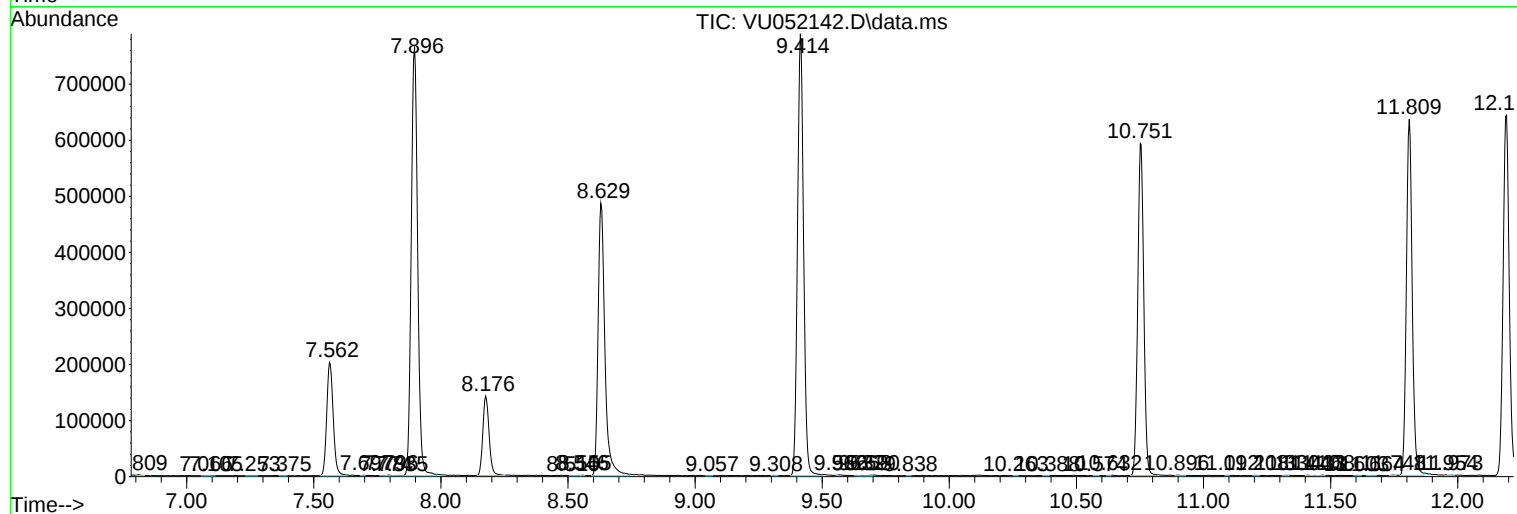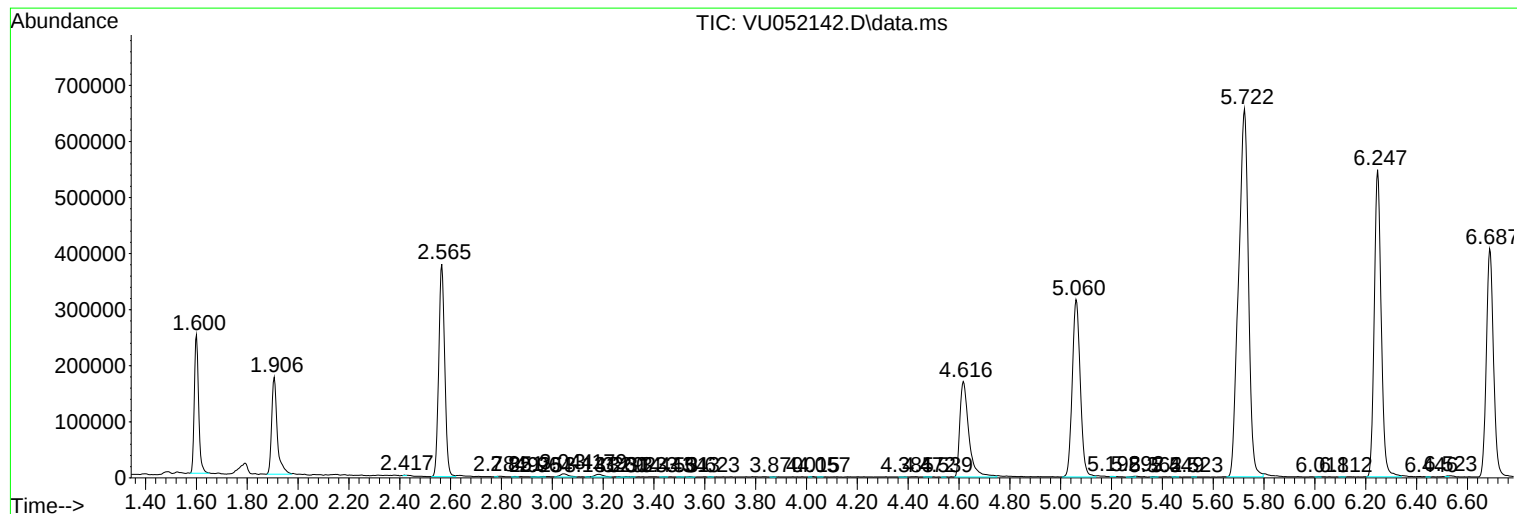

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052142.D
Acq On : 28 Nov 2022 12:43
Operator : JC/MD
Sample : VU1128WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK034

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052142.D
Acq On : 28 Nov 2022 12:43
Operator : JC/MD
Sample : VU1128WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK034

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc