

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052143.D
 Acq On : 28 Nov 2022 13:21
 Operator : JC/MD
 Sample : N5785-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COL76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

Signal : TIC: VU052143.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	34	42	50	rBV3	10671	20603	1.28%	0.170%
2	1.597	73	80	99	rVB	214755	255654	15.84%	2.112%
3	1.800	126	143	144	rBV7	20704	39457	2.45%	0.326%
4	1.896	165	173	184	rBV	149822	210951	13.07%	1.743%
5	2.562	368	380	394	rBV	330907	537408	33.31%	4.440%
6	2.803	453	455	461	rVB3	925	706	0.04%	0.006%
7	2.880	476	479	482	rBV2	682	465	0.03%	0.004%
8	2.970	502	507	518	rVB3	914	1542	0.10%	0.013%
9	3.044	518	530	538	rBV5	2314	4369	0.27%	0.036%
10	3.186	561	574	586	rBV	5877	12356	0.77%	0.102%
11	3.292	600	607	611	rVB3	517	725	0.04%	0.006%
12	3.321	611	616	620	rBV2	366	420	0.03%	0.003%
13	3.513	673	676	681	rVB	458	390	0.02%	0.003%
14	3.787	758	761	766	rBV2	467	389	0.02%	0.003%
15	3.983	818	822	825	rBV2	503	420	0.03%	0.003%
16	4.192	883	887	894	rVB2	510	611	0.04%	0.005%
17	4.231	894	899	902	rBV2	462	409	0.03%	0.003%
18	4.394	944	950	953	rBV2	404	413	0.03%	0.003%
19	4.616	1008	1019	1049	rBV2	144769	351636	21.79%	2.905%
20	4.976	1126	1131	1133	rBV2	549	446	0.03%	0.004%
21	5.060	1141	1157	1186	rBV	286911	630260	39.06%	5.207%
22	5.166	1186	1190	1193	rVB3	727	627	0.04%	0.005%
23	5.288	1225	1228	1237	rVB4	1170	1513	0.09%	0.012%
24	5.369	1250	1253	1257	rVV2	738	519	0.03%	0.004%
25	5.488	1285	1290	1296	rBV2	357	461	0.03%	0.004%
26	5.520	1296	1300	1306	rBV	445	441	0.03%	0.004%
27	5.722	1341	1363	1396	rBV2	592909	1613528	100.00%	13.330%
28	6.034	1455	1460	1462	rBV	430	453	0.03%	0.004%
29	6.095	1471	1479	1481	rBV2	739	638	0.04%	0.005%
30	6.128	1481	1489	1493	rVV3	705	953	0.06%	0.008%
31	6.247	1505	1526	1555	rBV	518276	980477	60.77%	8.100%
32	6.472	1590	1596	1601	rBV3	851	1168	0.07%	0.010%
33	6.539	1615	1617	1621	rVB7	1477	725	0.04%	0.006%
34	6.578	1626	1629	1632	rBV2	715	544	0.03%	0.004%
35	6.687	1646	1663	1691	rBV	370922	728485	45.15%	6.018%
36	7.166	1807	1812	1813	rBV2	586	490	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052143.D
 Acq On : 28 Nov 2022 13:21
 Operator : JC/MD
 Sample : N5785-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COL76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

37	7.208	1822	1825	1831	rVB3	647	512	0.03%	0.004%
38	7.250	1835	1838	1841	rVB2	657	405	0.03%	0.003%
39	7.295	1848	1852	1855	rBV2	553	489	0.03%	0.004%
40	7.382	1873	1879	1882	rBV2	398	401	0.02%	0.003%
41	7.433	1889	1895	1898	rBV2	478	497	0.03%	0.004%
42	7.562	1923	1935	1953	rBV	185563	325439	20.17%	2.689%
43	7.793	2002	2007	2010	rBV2	857	913	0.06%	0.008%
44	7.896	2022	2039	2066	rBV	694779	1206624	74.78%	9.968%
45	8.102	2099	2103	2106	rBV2	549	444	0.03%	0.004%
46	8.179	2115	2127	2146	rBV	132107	221680	13.74%	1.831%
47	8.359	2180	2183	2186	rBV2	706	493	0.03%	0.004%
48	8.468	2208	2217	2231	rVB4	3289	5240	0.32%	0.043%
49	8.542	2237	2240	2242	rBV3	630	458	0.03%	0.004%
50	8.632	2256	2268	2300	rBV	426930	795421	49.30%	6.571%
51	8.825	2326	2328	2332	rVB4	659	391	0.02%	0.003%
52	8.873	2337	2343	2348	rBV4	669	829	0.05%	0.007%
53	9.025	2383	2390	2392	rBV2	424	470	0.03%	0.004%
54	9.211	2444	2448	2454	rVB2	423	429	0.03%	0.004%
55	9.417	2499	2512	2531	rBV	736550	1218511	75.52%	10.067%
56	9.558	2552	2556	2559	rBV4	428	487	0.03%	0.004%
57	9.648	2581	2584	2587	rVV3	751	536	0.03%	0.004%
58	9.764	2615	2620	2623	rBV	456	434	0.03%	0.004%
59	9.986	2681	2689	2690	rBV	426	364	0.02%	0.003%
60	10.105	2722	2726	2728	rBV2	574	413	0.03%	0.003%
61	10.166	2741	2745	2750	rBV2	529	512	0.03%	0.004%
62	10.574	2866	2872	2875	rBV2	523	503	0.03%	0.004%
63	10.645	2890	2894	2898	rVB3	784	660	0.04%	0.005%
64	10.754	2914	2928	2953	rVV	560836	903969	56.02%	7.468%
65	10.889	2965	2970	2977	rVB3	2834	3366	0.21%	0.028%
66	10.963	2991	2993	3000	rVB	622	506	0.03%	0.004%
67	10.999	3000	3004	3007	rBV	504	433	0.03%	0.004%
68	11.089	3025	3032	3035	rBV4	675	873	0.05%	0.007%
69	11.140	3044	3048	3052	rBV2	341	422	0.03%	0.003%
70	11.179	3057	3060	3065	rVV3	581	608	0.04%	0.005%
71	11.208	3065	3069	3071	rVV	620	503	0.03%	0.004%
72	11.233	3075	3077	3084	rVV2	570	612	0.04%	0.005%
73	11.266	3084	3087	3091	rVV3	573	486	0.03%	0.004%
74	11.365	3108	3118	3121	rBV3	509	695	0.04%	0.006%
75	11.410	3130	3132	3137	rVB3	736	549	0.03%	0.005%
76	11.465	3145	3149	3150	rBV	768	540	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052143.D
 Acq On : 28 Nov 2022 13:21
 Operator : JC/MD
 Sample : N5785-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L76

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

77	11.748	3230	3237	3244	rBV4	1469	1917	0.12%	0.016%
78	11.812	3244	3257	3286	rBV	595908	960929	59.55%	7.939%
79	12.063	3327	3335	3351	rBV3	16269	32941	2.04%	0.272%
80	12.192	3362	3375	3408	rBV	608448	991588	61.45%	8.192%
81	12.394	3435	3438	3444	rBV3	586	606	0.04%	0.005%
82	12.581	3493	3496	3499	rVB2	556	376	0.02%	0.003%
83	12.632	3509	3512	3515	rBV2	596	462	0.03%	0.004%
84	12.764	3550	3553	3558	rVB4	714	629	0.04%	0.005%
85	12.918	3598	3601	3603	rBV	524	386	0.02%	0.003%
86	13.085	3648	3653	3657	rBV3	480	536	0.03%	0.004%
87	13.227	3689	3697	3706	rBV5	1463	2567	0.16%	0.021%
88	13.388	3744	3747	3753	rBV2	514	538	0.03%	0.004%
89	13.458	3763	3769	3772	rBV3	560	535	0.03%	0.004%
90	13.552	3795	3798	3803	rBV2	559	434	0.03%	0.004%
91	13.735	3852	3855	3858	rBV3	582	522	0.03%	0.004%
92	13.851	3884	3891	3895	rBV6	1620	2211	0.14%	0.018%
93	14.095	3959	3967	3968	rBV4	2496	2543	0.16%	0.021%
94	14.269	4017	4021	4025	rVB3	594	489	0.03%	0.004%
95	14.330	4036	4040	4046	rBV5	2035	2627	0.16%	0.022%
96	15.674	4455	4458	4463	rBV4	797	648	0.04%	0.005%
97	15.700	4463	4466	4469	rBV2	864	695	0.04%	0.006%
98	15.735	4474	4477	4479	rBV3	904	607	0.04%	0.005%
99	15.889	4522	4525	4529	rVB4	1270	851	0.05%	0.007%
100	16.153	4604	4607	4610	rBV4	1106	998	0.06%	0.008%




Sum of corrected areas: 12104404

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052143.D
Acq On : 28 Nov 2022 13:21
Operator : JC/MD
Sample : N5785-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COL76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

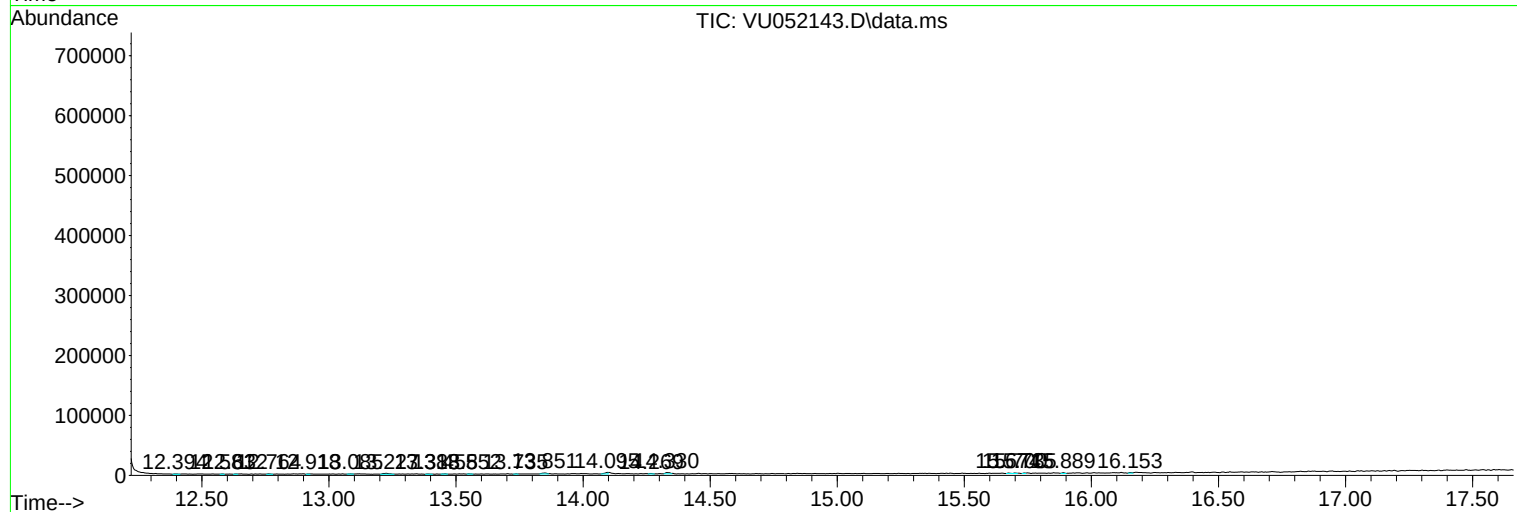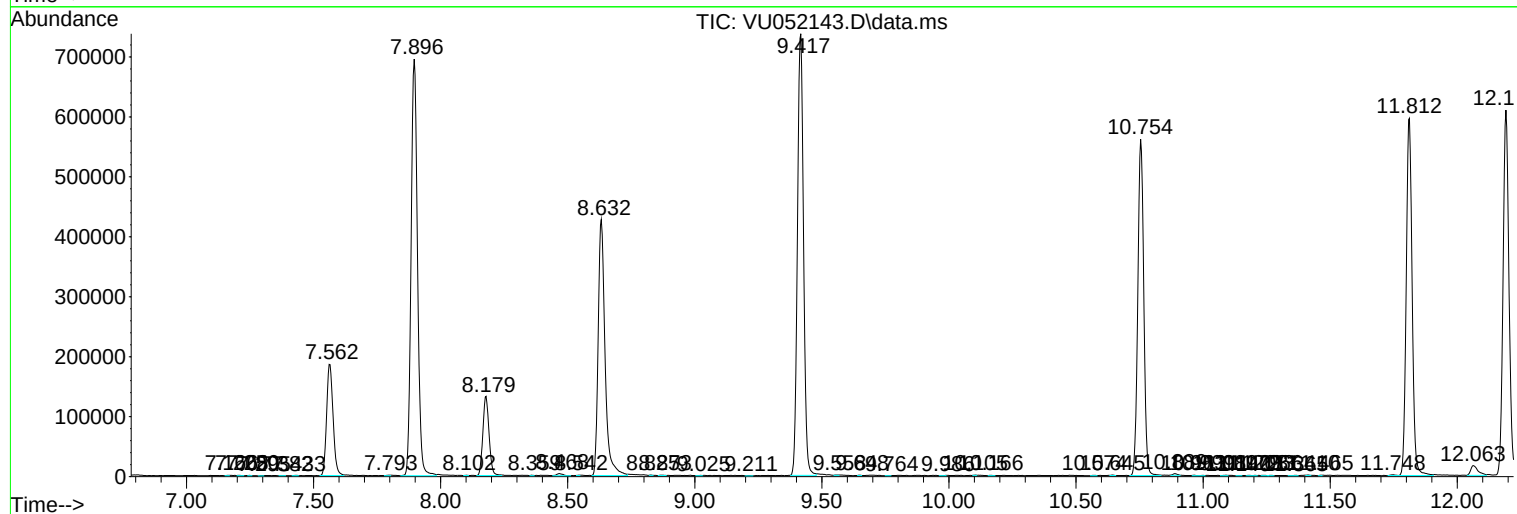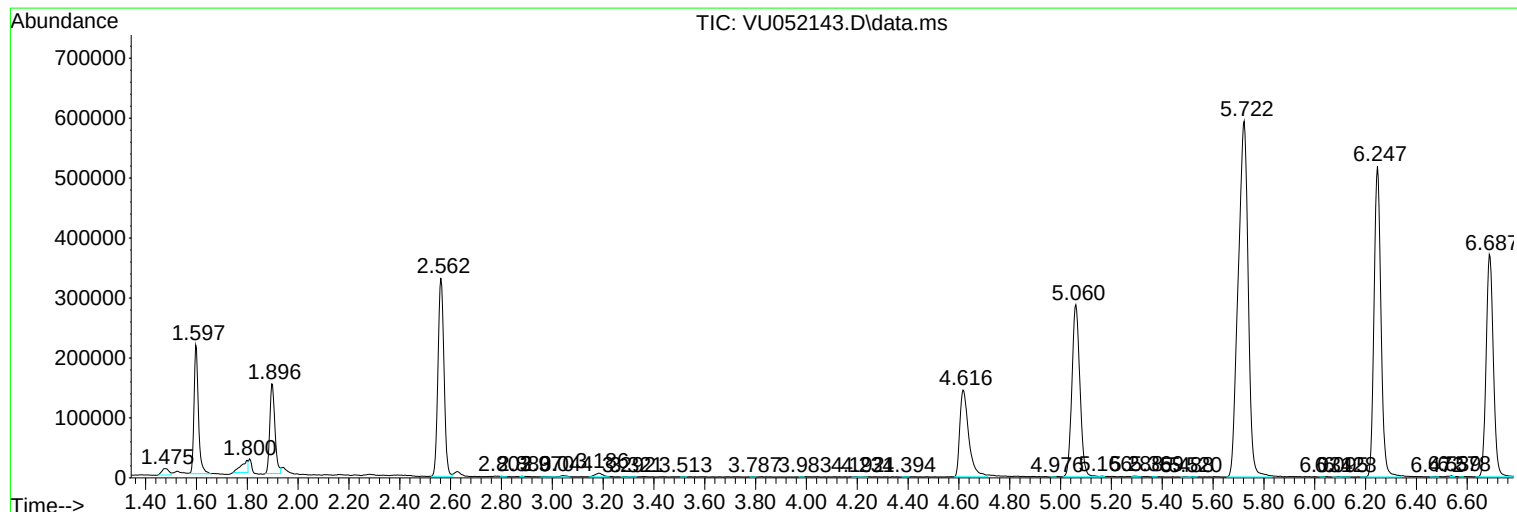

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052143.D
Acq On : 28 Nov 2022 13:21
Operator : JC/MD
Sample : N5785-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052143.D
Acq On : 28 Nov 2022 13:21
Operator : JC/MD
Sample : N5785-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L76

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------