

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052144.D
 Acq On : 28 Nov 2022 13:43
 Operator : JC/MD
 Sample : N5785-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COL70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M

Title : VOC Analysis

Signal : TIC: VU052144.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	35	44	51	rBV3	10149	19755	0.95%	0.137%
2	1.523	53	57	66	rVV2	7057	9389	0.45%	0.065%
3	1.597	73	80	97	rVB	222705	261175	12.50%	1.811%
4	1.900	166	174	205	rVB	154121	241780	11.57%	1.677%
5	2.562	368	380	393	rBV	337516	542740	25.97%	3.764%
6	2.758	437	441	443	rBV2	445	401	0.02%	0.003%
7	2.787	444	450	456	rVV5	1191	1609	0.08%	0.011%
8	2.813	456	458	464	rVB3	646	611	0.03%	0.004%
9	2.919	488	491	493	rBV2	500	359	0.02%	0.002%
10	3.038	522	528	531	rBV4	1320	1515	0.07%	0.011%
11	3.183	558	573	596	rVB	70373	168886	8.08%	1.171%
12	3.295	604	608	611	rBV	568	400	0.02%	0.003%
13	3.369	627	631	633	rBV2	511	400	0.02%	0.003%
14	3.469	656	662	664	rBV2	487	440	0.02%	0.003%
15	3.530	674	681	687	rBV	608	753	0.04%	0.005%
16	3.752	747	750	753	rVV	584	409	0.02%	0.003%
17	3.771	753	756	763	rVV3	398	438	0.02%	0.003%
18	3.826	769	773	776	rBV2	638	489	0.02%	0.003%
19	4.031	834	837	844	rVB	582	458	0.02%	0.003%
20	4.173	876	881	884	rVB3	413	398	0.02%	0.003%
21	4.218	891	895	899	rBV2	559	626	0.03%	0.004%
22	4.289	915	917	925	rVB2	650	639	0.03%	0.004%
23	4.617	1006	1019	1050	rBV	159861	394452	18.87%	2.736%
24	4.810	1077	1079	1083	rVB4	639	417	0.02%	0.003%
25	5.060	1141	1157	1182	rBV	287612	634478	30.35%	4.400%
26	5.266	1217	1221	1223	rBV2	524	464	0.02%	0.003%
27	5.292	1223	1229	1236	rVB5	1284	2026	0.10%	0.014%
28	5.366	1247	1252	1254	rBV3	798	631	0.03%	0.004%
29	5.584	1316	1320	1324	rBV2	456	368	0.02%	0.003%
30	5.617	1324	1330	1336	rVB2	269	376	0.02%	0.003%
31	5.723	1341	1363	1397	rBV2	598832	1641523	78.53%	11.385%
32	5.883	1410	1413	1416	rBV2	503	347	0.02%	0.002%
33	6.070	1469	1471	1476	rVB3	712	544	0.03%	0.004%
34	6.105	1476	1482	1484	rBV3	460	550	0.03%	0.004%
35	6.157	1495	1498	1502	rBV2	484	362	0.02%	0.003%
36	6.247	1512	1526	1555	rBV	486789	932539	44.61%	6.468%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052144.D
 Acq On : 28 Nov 2022 13:43
 Operator : JC/MD
 Sample : N5785-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COL70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

37	6.530	1612	1614	1617	rVB2	686	397	0.02%	0.003%
38	6.565	1622	1625	1628	rBV	478	355	0.02%	0.002%
39	6.588	1628	1632	1636	rBV4	693	829	0.04%	0.006%
40	6.687	1649	1663	1685	rVV	376299	731155	34.98%	5.071%
41	6.858	1713	1716	1719	rVB	585	373	0.02%	0.003%
42	6.887	1723	1725	1730	rBV2	352	387	0.02%	0.003%
43	6.983	1752	1755	1759	rVV2	612	559	0.03%	0.004%
44	7.121	1796	1798	1805	rVB3	551	545	0.03%	0.004%
45	7.173	1810	1814	1816	rBV2	459	376	0.02%	0.003%
46	7.340	1863	1866	1871	rVB2	394	365	0.02%	0.003%
47	7.424	1889	1892	1897	rBV2	519	466	0.02%	0.003%
48	7.462	1897	1904	1906	rBV2	509	521	0.02%	0.004%
49	7.562	1923	1935	1954	rBV	185255	327619	15.67%	2.272%
50	7.671	1967	1969	1975	rVB3	571	495	0.02%	0.003%
51	7.700	1975	1978	1981	rBV2	686	505	0.02%	0.004%
52	7.787	2000	2005	2007	rBV4	621	659	0.03%	0.005%
53	7.896	2024	2039	2061	rBV	697770	1207950	57.79%	8.378%
54	8.176	2115	2126	2145	rBV	133168	225632	10.79%	1.565%
55	8.356	2178	2182	2185	rVB4	560	358	0.02%	0.002%
56	8.375	2185	2188	2192	rBV3	540	579	0.03%	0.004%
57	8.465	2211	2216	2218	rBV3	1543	1443	0.07%	0.010%
58	8.552	2239	2243	2248	rVB5	660	528	0.03%	0.004%
59	8.629	2255	2267	2301	rBV	445786	830632	39.74%	5.761%
60	9.034	2388	2393	2400	rBV2	378	508	0.02%	0.004%
61	9.092	2408	2411	2414	rBV2	551	366	0.02%	0.003%
62	9.112	2414	2417	2424	rVB2	453	492	0.02%	0.003%
63	9.163	2429	2433	2438	rVB2	359	415	0.02%	0.003%
64	9.414	2498	2511	2536	rVV	708524	1307889	62.57%	9.071%
65	9.758	2614	2618	2621	rBV2	643	541	0.03%	0.004%
66	10.256	2769	2773	2775	rBV2	553	364	0.02%	0.003%
67	10.433	2821	2828	2829	rBV	425	398	0.02%	0.003%
68	10.562	2864	2868	2873	rBV	530	404	0.02%	0.003%
69	10.755	2914	2928	2948	rBV	562110	904239	43.26%	6.271%
70	10.890	2965	2970	2974	rBV3	1621	1585	0.08%	0.011%
71	11.185	3057	3062	3066	rBV2	369	413	0.02%	0.003%
72	11.227	3070	3075	3078	rVV3	575	598	0.03%	0.004%
73	11.349	3110	3113	3116	rVB2	666	481	0.02%	0.003%
74	11.520	3162	3166	3171	rVB3	580	457	0.02%	0.003%
75	11.552	3171	3176	3181	rBV2	635	674	0.03%	0.005%
76	11.581	3182	3185	3191	rVV3	310	389	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052144.D
 Acq On : 28 Nov 2022 13:43
 Operator : JC/MD
 Sample : N5785-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COL70

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

77	11.639	3200	3203	3207	rBV2	488	350	0.02%	0.002%
78	11.745	3225	3236	3245	rBV2	59393	97907	4.68%	0.679%
79	11.809	3245	3256	3280	rVB	585490	1022684	48.93%	7.093%
80	12.060	3320	3334	3353	rBV3	17319	36058	1.73%	0.250%
81	12.202	3361	3378	3408	rBV2	862106	2090236	100.00%	14.497%
82	12.359	3424	3427	3433	rBV2	824	684	0.03%	0.005%
83	12.536	3480	3482	3491	rVB2	568	596	0.03%	0.004%
84	12.578	3491	3495	3498	rBV2	533	510	0.02%	0.004%
85	12.825	3564	3572	3580	rBV2	611	1007	0.05%	0.007%
86	12.883	3586	3590	3593	rBV3	570	508	0.02%	0.004%
87	13.054	3640	3643	3646	rBV3	478	380	0.02%	0.003%
88	13.163	3668	3677	3680	rBV2	718	1098	0.05%	0.008%
89	13.208	3681	3691	3706	rVV2	15091	26654	1.28%	0.185%
90	13.327	3724	3728	3729	rBV2	592	417	0.02%	0.003%
91	13.513	3781	3786	3789	rBV	903	787	0.04%	0.005%
92	13.603	3810	3814	3816	rBV2	595	467	0.02%	0.003%
93	13.838	3875	3887	3909	rVV	234451	373801	17.88%	2.592%
94	14.047	3950	3952	3957	rBV2	457	477	0.02%	0.003%
95	14.230	4007	4009	4012	rBV2	466	391	0.02%	0.003%
96	14.327	4027	4039	4058	rBV	170374	287977	13.78%	1.997%
97	14.423	4067	4069	4074	rBV3	650	550	0.03%	0.004%
98	14.732	4157	4165	4176	rBV7	4741	8703	0.42%	0.060%
99	14.944	4228	4231	4235	rBV3	677	563	0.03%	0.004%
100	15.996	4550	4558	4571	rBV3	29927	50130	2.40%	0.348%




Sum of corrected areas: 14418623

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052144.D
Acq On : 28 Nov 2022 13:43
Operator : JC/MD
Sample : N5785-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COL70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

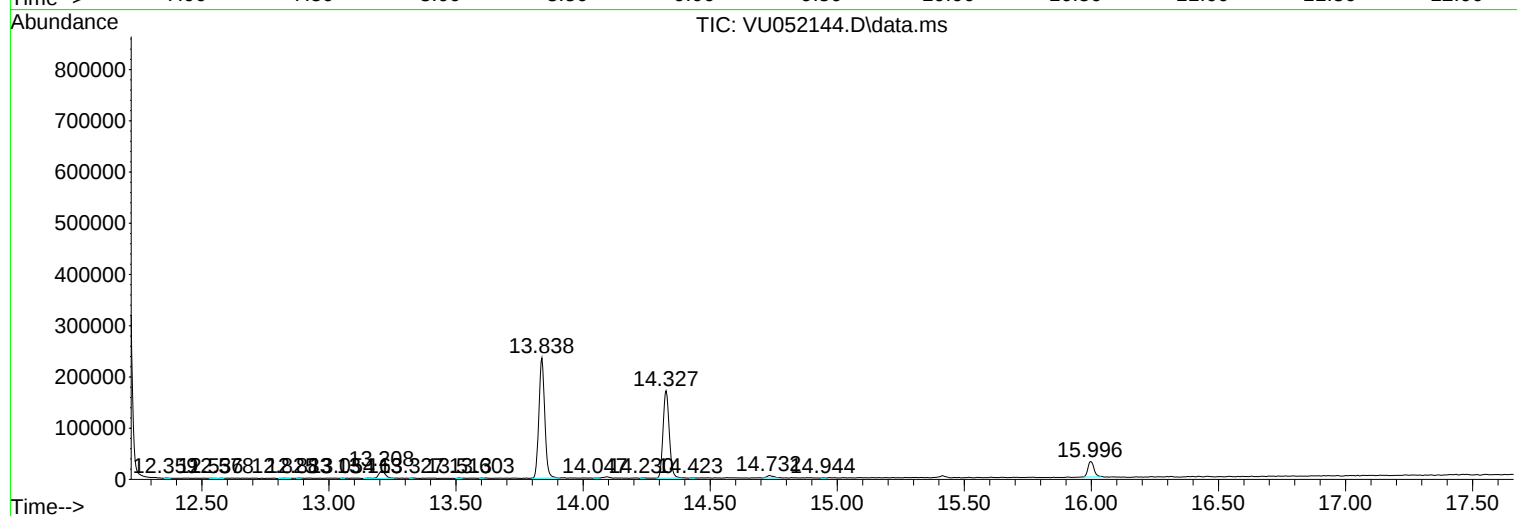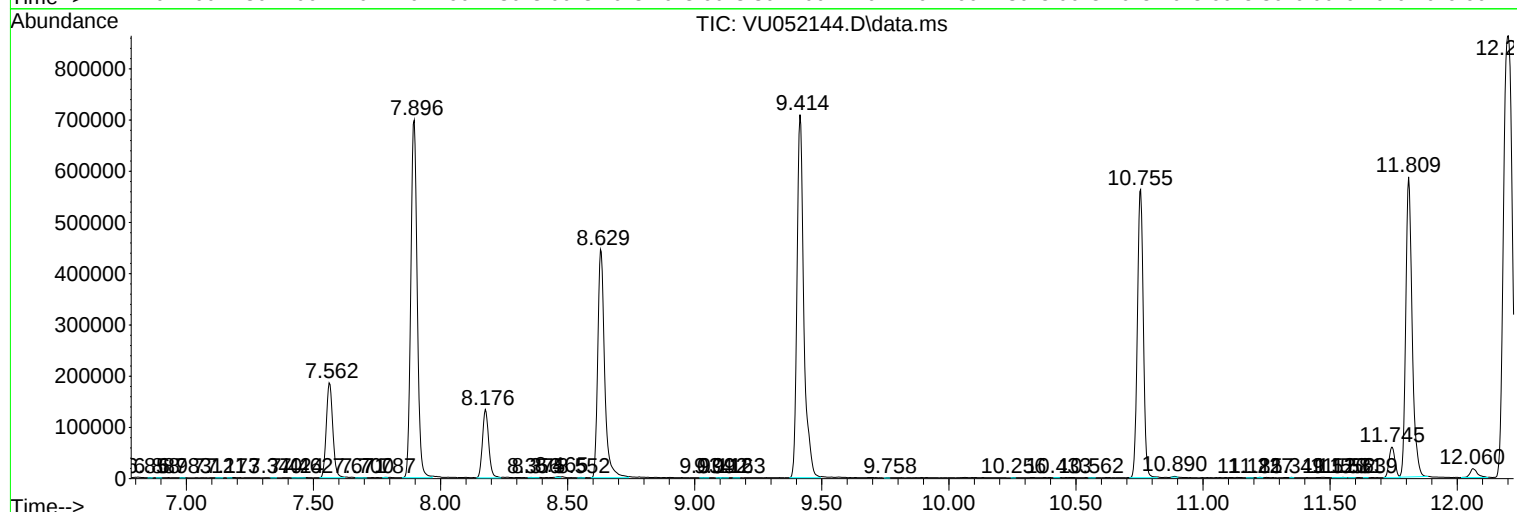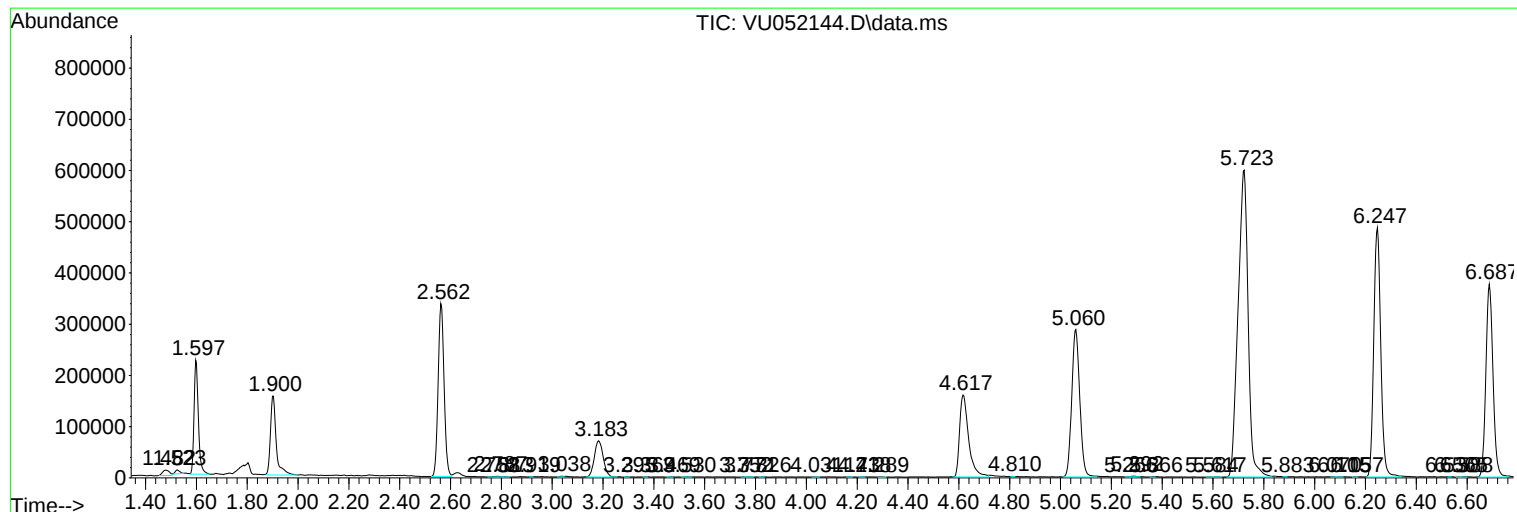

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052144.D
Acq On : 28 Nov 2022 13:43
Operator : JC/MD
Sample : N5785-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052144.D
Acq On : 28 Nov 2022 13:43
Operator : JC/MD
Sample : N5785-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L70

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------