

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052145.D
 Acq On : 28 Nov 2022 14:10
 Operator : JC/MD
 Sample : N5785-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COL72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

Signal : TIC: VU052145.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	74	80	99	rVB	219259	261864	16.11%	2.157%
2	1.906	168	176	203	rVB	154785	239346	14.73%	1.971%
3	2.565	369	381	397	rBV	327972	534852	32.91%	4.405%
4	3.102	542	548	550	rBV2	334	356	0.02%	0.003%
5	3.183	559	573	594	rVB	56808	132843	8.17%	1.094%
6	3.321	613	616	620	rBV2	454	338	0.02%	0.003%
7	3.430	641	650	652	rBV2	522	694	0.04%	0.006%
8	3.543	681	685	688	rBV2	289	216	0.01%	0.002%
9	3.575	692	695	699	rBV	601	374	0.02%	0.003%
10	3.768	749	755	760	rBV2	497	608	0.04%	0.005%
11	3.842	776	778	782	rBV2	218	170	0.01%	0.001%
12	3.893	790	794	796	rBV2	408	391	0.02%	0.003%
13	3.961	811	815	817	rBV2	334	206	0.01%	0.002%
14	3.977	817	820	823	rVV	511	340	0.02%	0.003%
15	4.002	826	828	831	rVB	308	136	0.01%	0.001%
16	4.038	836	839	842	rBV	437	262	0.02%	0.002%
17	4.186	882	885	887	rBV2	550	315	0.02%	0.003%
18	4.228	893	898	899	rBV2	343	320	0.02%	0.003%
19	4.276	909	913	916	rBV	373	283	0.02%	0.002%
20	4.334	927	931	934	rBV2	427	314	0.02%	0.003%
21	4.433	959	962	964	rBV2	322	161	0.01%	0.001%
22	4.459	965	970	973	rBV2	538	486	0.03%	0.004%
23	4.501	979	983	984	rBV	329	207	0.01%	0.002%
24	4.527	988	991	995	rBV2	330	342	0.02%	0.003%
25	4.617	1007	1019	1053	rBV	164662	407261	25.06%	3.354%
26	5.060	1142	1157	1180	rBV2	290006	632523	38.92%	5.209%
27	5.279	1222	1225	1226	rBV3	899	531	0.03%	0.004%
28	5.366	1247	1252	1255	rBV4	751	808	0.05%	0.007%
29	5.488	1286	1290	1297	rVB2	553	516	0.03%	0.004%
30	5.520	1297	1300	1304	rBV2	356	244	0.02%	0.002%
31	5.546	1304	1308	1312	rBV2	365	359	0.02%	0.003%
32	5.572	1312	1316	1317	rBV2	264	163	0.01%	0.001%
33	5.620	1328	1331	1333	rBV	458	295	0.02%	0.002%
34	5.633	1333	1335	1338	rVB	168	80	0.00%	0.001%
35	5.723	1342	1363	1393	rBV2	598416	1625199	100.00%	13.385%
36	6.012	1451	1453	1454	rBV	252	127	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052145.D
 Acq On : 28 Nov 2022 14:10
 Operator : JC/MD
 Sample : N5785-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COL72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

37	6.025	1454	1457	1459	rVV3	396	278	0.02%	0.002%
38	6.044	1461	1463	1465	rBV	318	176	0.01%	0.001%
39	6.121	1485	1487	1489	rBV	314	192	0.01%	0.002%
40	6.166	1499	1501	1506	rVB2	641	443	0.03%	0.004%
41	6.192	1506	1509	1512	rBV	521	425	0.03%	0.004%
42	6.247	1512	1526	1555	rBV	510437	976130	60.06%	8.039%
43	6.498	1600	1604	1608	rBV2	757	634	0.04%	0.005%
44	6.530	1609	1614	1615	rBV3	957	753	0.05%	0.006%
45	6.687	1648	1663	1693	rBV	371769	736006	45.29%	6.062%
46	6.922	1734	1736	1742	rVB2	708	510	0.03%	0.004%
47	7.256	1837	1840	1843	rVB2	274	187	0.01%	0.002%
48	7.276	1843	1846	1847	rBV	167	82	0.01%	0.001%
49	7.330	1858	1863	1866	rBV	618	513	0.03%	0.004%
50	7.379	1872	1878	1880	rBV3	407	392	0.02%	0.003%
51	7.565	1923	1936	1955	rBV2	185067	324971	20.00%	2.676%
52	7.723	1982	1985	1989	rBB2	800	441	0.03%	0.004%
53	7.896	2025	2039	2062	rBV	687796	1192408	73.37%	9.820%
54	8.176	2115	2126	2146	rBV	130243	220288	13.55%	1.814%
55	8.559	2240	2245	2251	rBV5	774	855	0.05%	0.007%
56	8.629	2255	2267	2301	rBV	445350	825099	50.77%	6.795%
57	8.877	2342	2344	2348	rVB2	663	406	0.02%	0.003%
58	9.028	2387	2391	2393	rBV	472	356	0.02%	0.003%
59	9.112	2411	2417	2421	rBV3	574	698	0.04%	0.006%
60	9.166	2431	2434	2439	rBV2	647	489	0.03%	0.004%
61	9.301	2472	2476	2480	rBV2	582	643	0.04%	0.005%
62	9.350	2489	2491	2494	rBV2	342	220	0.01%	0.002%
63	9.414	2498	2511	2543	rBV	719917	1204550	74.12%	9.920%
64	9.639	2578	2581	2584	rBV2	589	347	0.02%	0.003%
65	9.671	2589	2591	2594	rVB	358	161	0.01%	0.001%
66	9.700	2594	2600	2603	rBV4	1004	972	0.06%	0.008%
67	9.761	2616	2619	2621	rBV	323	201	0.01%	0.002%
68	9.787	2625	2627	2629	rBV	453	266	0.02%	0.002%
69	9.983	2686	2688	2691	rBV	292	233	0.01%	0.002%
70	10.523	2854	2856	2859	rBV	305	195	0.01%	0.002%
71	10.575	2867	2872	2875	rBV	500	521	0.03%	0.004%
72	10.755	2913	2928	2947	rBV	554387	897793	55.24%	7.394%
73	11.382	3120	3123	3125	rBV2	512	392	0.02%	0.003%
74	11.809	3244	3256	3282	rBV	561645	910393	56.02%	7.498%
75	12.066	3328	3336	3350	rBV5	5177	10207	0.63%	0.084%
76	12.192	3361	3375	3402	rBV	584809	970754	59.73%	7.995%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052145.D
Acq On : 28 Nov 2022 14:10
Operator : JC/MD
Sample : N5785-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L72

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Title : VOC Analysis

77	12.520	3474	3477	3480	rBV2	660	607	0.04%	0.005%
78	13.841	3882	3888	3903	rVB2	10916	17489	1.08%	0.144%


Sum of corrected areas: 12142206

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052145.D
Acq On : 28 Nov 2022 14:10
Operator : JC/MD
Sample : N5785-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COL72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

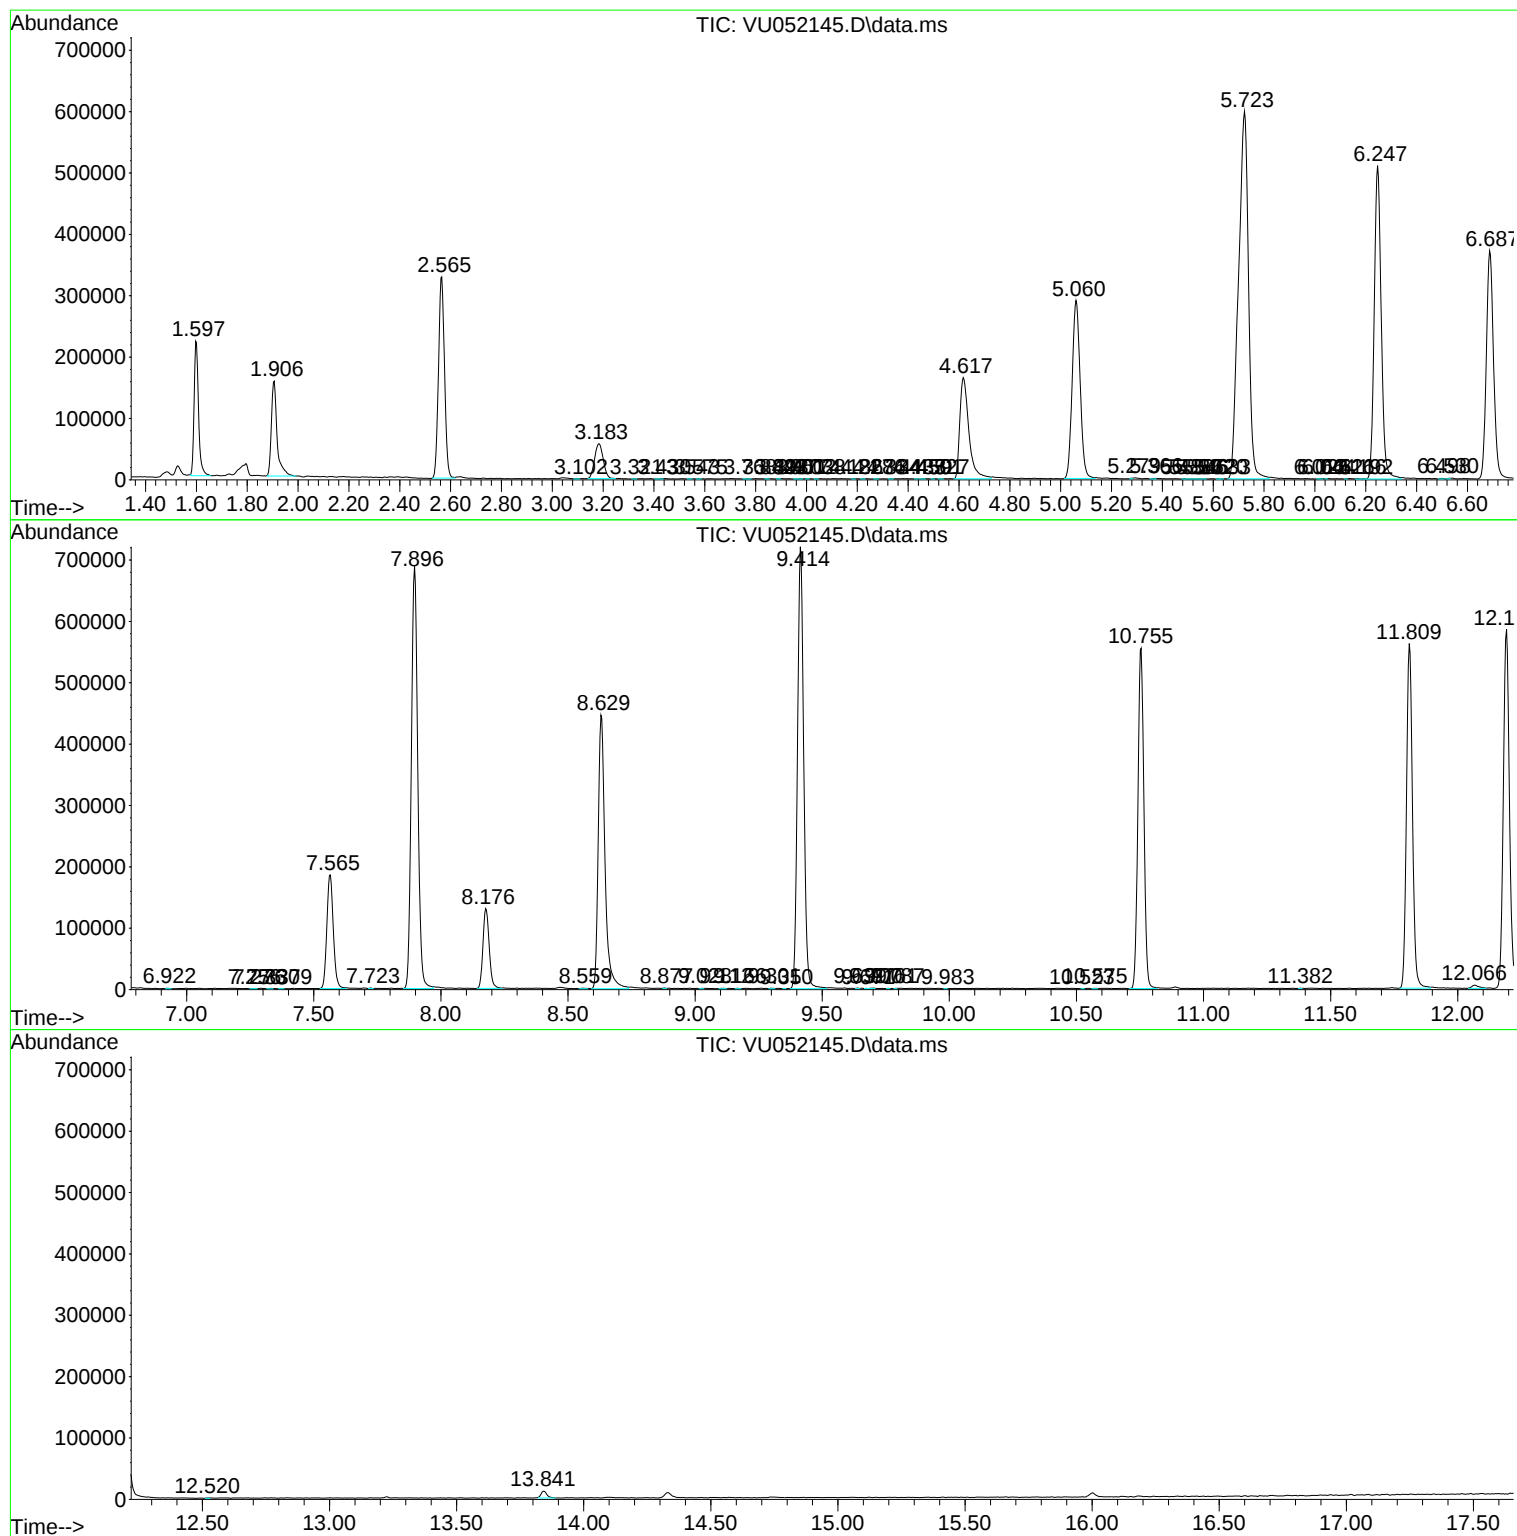

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052145.D
Acq On : 28 Nov 2022 14:10
Operator : JC/MD
Sample : N5785-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052145.D
Acq On : 28 Nov 2022 14:10
Operator : JC/MD
Sample : N5785-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------