

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052146.D
 Acq On : 28 Nov 2022 14:35
 Operator : JC/MD
 Sample : N5785-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COL73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

Signal : TIC: VU052146.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.524	52	57	68	rBV	7126	10388	0.63%	0.085%
2	1.597	73	80	100	rVB	224263	265412	16.18%	2.177%
3	1.903	167	175	203	rVB	158901	242840	14.81%	1.992%
4	2.562	368	380	396	rBV	331764	542712	33.09%	4.452%
5	2.636	399	403	413	rVB3	3416	4949	0.30%	0.041%
6	2.745	435	437	443	rVB3	580	389	0.02%	0.003%
7	2.958	496	503	507	rVB4	817	1071	0.07%	0.009%
8	3.044	522	530	541	rVV6	1684	3583	0.22%	0.029%
9	3.183	557	573	590	rBV	58478	136096	8.30%	1.117%
10	3.266	595	599	601	rBV	538	429	0.03%	0.004%
11	3.324	612	617	622	rBV2	362	391	0.02%	0.003%
12	3.430	646	650	656	rVB2	818	985	0.06%	0.008%
13	3.475	656	664	667	rBV3	498	523	0.03%	0.004%
14	3.604	700	704	710	rVB3	458	468	0.03%	0.004%
15	3.646	714	717	721	rVB	497	353	0.02%	0.003%
16	3.765	749	754	758	rBV3	412	418	0.03%	0.003%
17	3.903	791	797	801	rBV2	565	522	0.03%	0.004%
18	3.990	817	824	826	rBV2	353	437	0.03%	0.004%
19	4.112	857	862	866	rBV	631	578	0.04%	0.005%
20	4.134	866	869	874	rVB2	382	354	0.02%	0.003%
21	4.202	886	890	893	rBV2	395	329	0.02%	0.003%
22	4.330	927	930	938	rVB3	485	536	0.03%	0.004%
23	4.453	963	968	971	rVB2	671	593	0.04%	0.005%
24	4.617	1007	1019	1055	rBV	164837	413849	25.23%	3.395%
25	4.832	1083	1086	1089	rBV2	515	397	0.02%	0.003%
26	5.060	1137	1157	1179	rBV	293917	644553	39.30%	5.288%
27	5.253	1209	1217	1219	rBV2	600	575	0.04%	0.005%
28	5.285	1223	1227	1233	rVV5	1260	1518	0.09%	0.012%
29	5.366	1248	1252	1254	rBV3	407	334	0.02%	0.003%
30	5.379	1254	1256	1262	rVV3	962	711	0.04%	0.006%
31	5.414	1264	1267	1271	rVB	496	336	0.02%	0.003%
32	5.443	1272	1276	1280	rVB	998	777	0.05%	0.006%
33	5.482	1285	1288	1295	rBV3	502	517	0.03%	0.004%
34	5.568	1313	1315	1322	rVB2	705	715	0.04%	0.006%
35	5.604	1322	1326	1330	rBV2	437	406	0.02%	0.003%
36	5.642	1333	1338	1341	rVB	483	351	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052146.D
 Acq On : 28 Nov 2022 14:35
 Operator : JC/MD
 Sample : N5785-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COL73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

37	5.723	1341	1363	1396	rBV2	602594	1640052	100.00%	13.455%
38	5.993	1445	1447	1453	rVB	527	327	0.02%	0.003%
39	6.038	1453	1461	1464	rBV	923	894	0.05%	0.007%
40	6.247	1511	1526	1568	rBV	503011	970959	59.20%	7.966%
41	6.449	1586	1589	1595	rVB3	775	813	0.05%	0.007%
42	6.491	1597	1602	1607	rBV3	678	778	0.05%	0.006%
43	6.520	1607	1611	1613	rBV2	1117	932	0.06%	0.008%
44	6.578	1625	1629	1631	rBV2	517	343	0.02%	0.003%
45	6.636	1642	1647	1649	rBV2	506	461	0.03%	0.004%
46	6.687	1649	1663	1693	rVV	376236	739189	45.07%	6.064%
47	7.035	1765	1771	1775	rBV2	559	580	0.04%	0.005%
48	7.253	1835	1839	1843	rBV	528	479	0.03%	0.004%
49	7.295	1848	1852	1857	rVB2	411	448	0.03%	0.004%
50	7.562	1923	1935	1959	rVV	181523	328413	20.02%	2.694%
51	7.674	1966	1970	1972	rBV2	424	350	0.02%	0.003%
52	7.835	2016	2020	2025	rBV3	336	393	0.02%	0.003%
53	7.896	2025	2039	2066	rBV	701199	1203998	73.41%	9.878%
54	8.176	2114	2126	2143	rVV	129885	219509	13.38%	1.801%
55	8.295	2159	2163	2165	rBV2	757	551	0.03%	0.005%
56	8.472	2212	2218	2227	rVB5	2196	3245	0.20%	0.027%
57	8.526	2231	2235	2239	rBV4	663	521	0.03%	0.004%
58	8.552	2241	2243	2247	rVB2	593	360	0.02%	0.003%
59	8.629	2252	2267	2298	rBV	454585	838449	51.12%	6.879%
60	8.780	2311	2314	2320	rVB6	766	734	0.04%	0.006%
61	8.883	2341	2346	2349	rBV3	622	667	0.04%	0.005%
62	8.928	2357	2360	2370	rBV4	698	1050	0.06%	0.009%
63	9.038	2392	2394	2397	rVV	586	369	0.02%	0.003%
64	9.115	2414	2418	2421	rBV3	487	469	0.03%	0.004%
65	9.179	2435	2438	2446	rVB2	557	803	0.05%	0.007%
66	9.221	2446	2451	2453	rBV	330	326	0.02%	0.003%
67	9.414	2498	2511	2535	rBV	713065	1191721	72.66%	9.777%
68	9.633	2577	2579	2584	rVB4	576	427	0.03%	0.004%
69	9.674	2590	2592	2596	rBV2	506	376	0.02%	0.003%
70	10.102	2722	2725	2730	rVV2	620	610	0.04%	0.005%
71	10.250	2768	2771	2775	rVB3	575	458	0.03%	0.004%
72	10.414	2818	2822	2828	rVV2	390	531	0.03%	0.004%
73	10.462	2835	2837	2841	rVB2	536	324	0.02%	0.003%
74	10.491	2842	2846	2849	rVV3	597	424	0.03%	0.003%
75	10.571	2868	2871	2877	rVB	426	392	0.02%	0.003%
76	10.751	2913	2927	2948	rBV	547452	883871	53.89%	7.251%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052146.D
 Acq On : 28 Nov 2022 14:35
 Operator : JC/MD
 Sample : N5785-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

77	10.890	2964	2970	2979	rVB4	1823	2866	0.17%	0.024%
78	10.960	2988	2992	2996	rBV3	662	582	0.04%	0.005%
79	11.012	3005	3008	3012	rBV2	612	558	0.03%	0.005%
80	11.102	3033	3036	3040	rVV2	488	429	0.03%	0.004%
81	11.407	3128	3131	3134	rVB2	561	356	0.02%	0.003%
82	11.472	3147	3151	3153	rBV3	480	342	0.02%	0.003%
83	11.591	3182	3188	3191	rBV3	668	677	0.04%	0.006%
84	11.610	3191	3194	3197	rVV	581	368	0.02%	0.003%
85	11.809	3243	3256	3279	rBV	553337	888029	54.15%	7.285%
86	11.989	3308	3312	3317	rBV3	679	588	0.04%	0.005%
87	12.038	3323	3327	3328	rBV	612	437	0.03%	0.004%
88	12.063	3328	3335	3356	rVB4	7578	15582	0.95%	0.128%
89	12.189	3362	3374	3402	rBV	570897	947982	57.80%	7.777%
90	12.452	3451	3456	3459	rBV3	535	600	0.04%	0.005%
91	12.504	3469	3472	3473	rBV2	648	330	0.02%	0.003%
92	12.755	3543	3550	3552	rBV	524	542	0.03%	0.004%
93	13.092	3652	3655	3657	rBV2	620	427	0.03%	0.004%
94	13.214	3686	3693	3695	rBV4	601	809	0.05%	0.007%
95	13.311	3720	3723	3729	rBV2	657	690	0.04%	0.006%
96	13.607	3812	3815	3817	rBV2	504	347	0.02%	0.003%
97	13.848	3884	3890	3899	rVB5	2542	3823	0.23%	0.031%
98	14.173	3988	3991	3997	rVB	504	445	0.03%	0.004%
99	14.333	4034	4041	4056	rVB9	3259	6932	0.42%	0.057%
100	14.394	4056	4060	4062	rBV	555	457	0.03%	0.004%




Sum of corrected areas: 12189189

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052146.D
Acq On : 28 Nov 2022 14:35
Operator : JC/MD
Sample : N5785-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COL73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

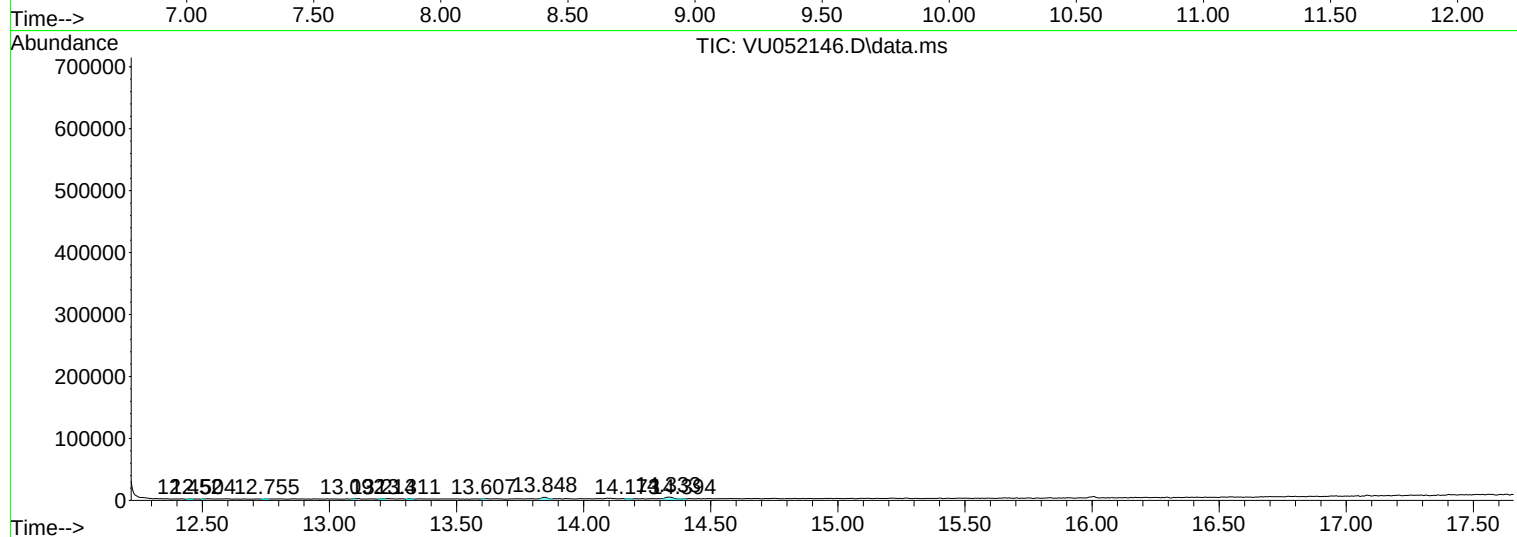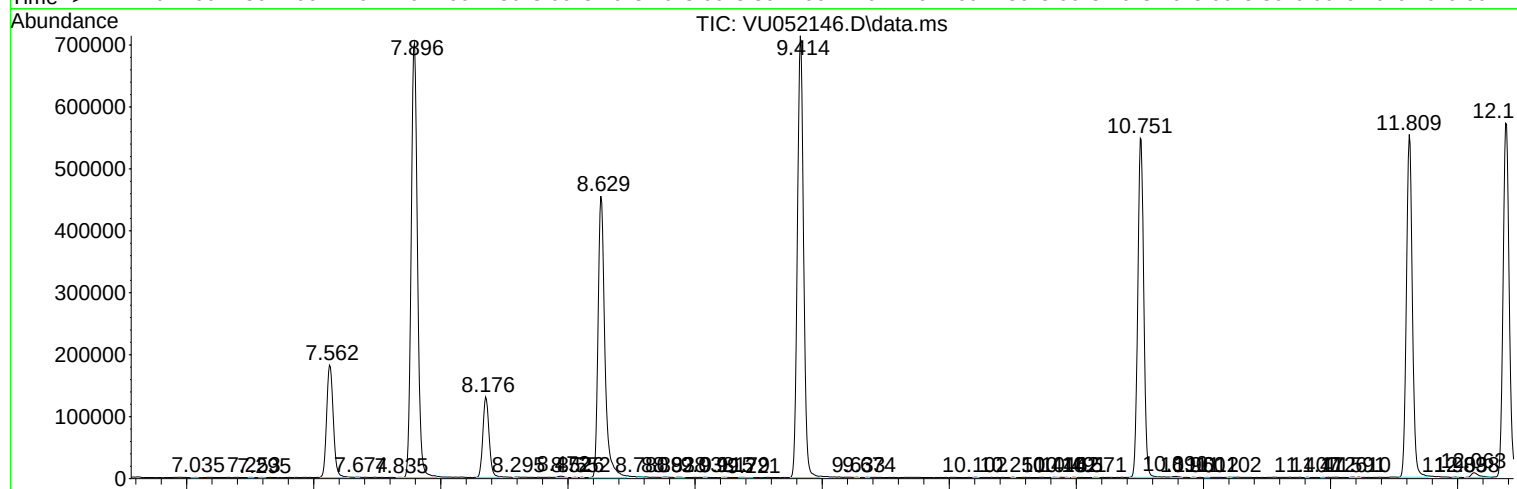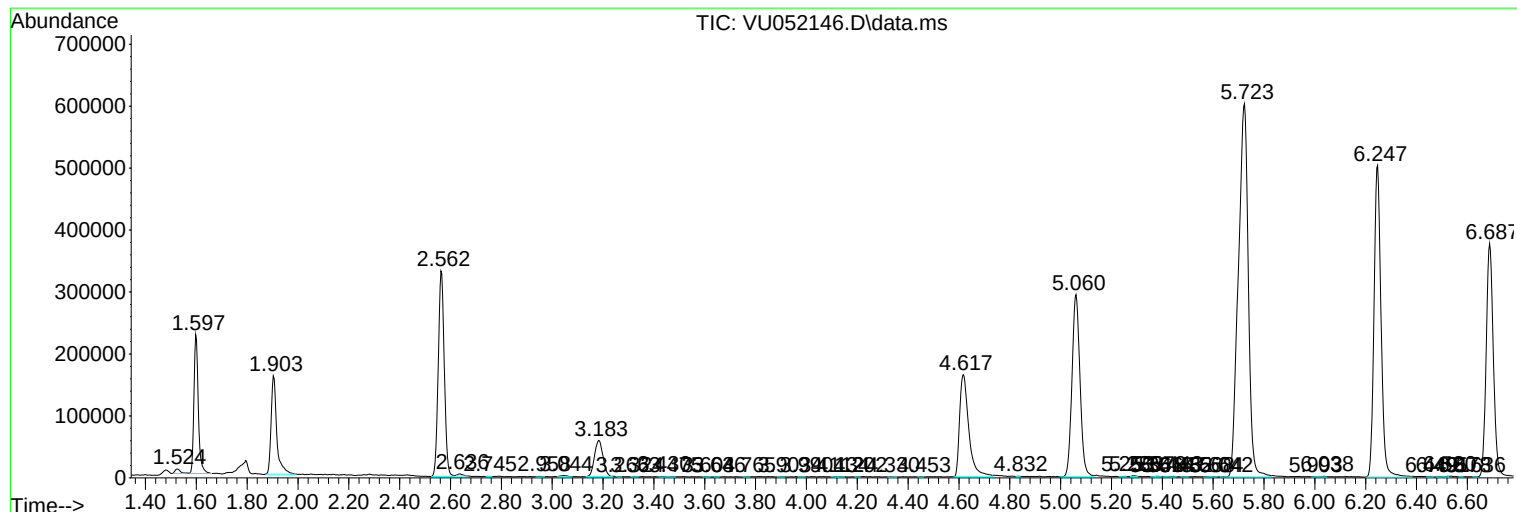

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052146.D
Acq On : 28 Nov 2022 14:35
Operator : JC/MD
Sample : N5785-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052146.D
Acq On : 28 Nov 2022 14:35
Operator : JC/MD
Sample : N5785-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L73

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------