

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052148.D
 Acq On : 28 Nov 2022 15:24
 Operator : JC/MD
 Sample : N5785-05DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L75DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

Signal : TIC: VU052148.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	100	rVB	244314	290916	16.55%	2.072%
2	1.906	167	176	198	rBV	173022	256735	14.61%	1.829%
3	2.565	368	381	396	rBV	368273	605065	34.42%	4.310%
4	2.720	427	429	431	rBV	592	306	0.02%	0.002%
5	2.774	442	446	449	rBV2	819	750	0.04%	0.005%
6	3.048	521	531	538	rBV6	3760	7106	0.40%	0.051%
7	3.109	546	550	553	rBV3	487	471	0.03%	0.003%
8	3.141	557	560	561	rBV3	441	285	0.02%	0.002%
9	3.183	561	573	593	rVB	9210	20911	1.19%	0.149%
10	3.295	603	608	614	rBV2	621	557	0.03%	0.004%
11	3.321	614	616	619	rVB2	494	296	0.02%	0.002%
12	3.356	619	627	629	rBV2	591	809	0.05%	0.006%
13	3.427	645	649	651	rBV	487	302	0.02%	0.002%
14	3.504	670	673	677	rBV2	343	288	0.02%	0.002%
15	3.549	682	687	691	rBV2	366	355	0.02%	0.003%
16	3.919	799	802	809	rVB	533	618	0.04%	0.004%
17	3.974	816	819	822	rBV2	439	389	0.02%	0.003%
18	3.990	822	824	829	rVB2	579	378	0.02%	0.003%
19	4.041	836	840	843	rBV2	332	334	0.02%	0.002%
20	4.102	856	859	863	rBV2	422	370	0.02%	0.003%
21	4.163	875	878	885	rVB2	339	326	0.02%	0.002%
22	4.199	885	889	892	rBV2	552	436	0.02%	0.003%
23	4.279	907	914	920	rBV3	429	723	0.04%	0.005%
24	4.369	939	942	946	rVB	529	366	0.02%	0.003%
25	4.392	946	949	957	rBV2	468	430	0.02%	0.003%
26	4.456	966	969	972	rBV	477	291	0.02%	0.002%
27	4.617	1007	1019	1049	rBV	167622	407974	23.21%	2.906%
28	4.864	1092	1096	1098	rVV2	716	402	0.02%	0.003%
29	5.060	1141	1157	1180	rBV	311612	683867	38.91%	4.872%
30	5.240	1210	1213	1219	rVB3	482	402	0.02%	0.003%
31	5.295	1220	1230	1233	rBV4	1462	1933	0.11%	0.014%
32	5.369	1249	1253	1256	rVB5	751	575	0.03%	0.004%
33	5.527	1300	1302	1308	rVB4	705	674	0.04%	0.005%
34	5.556	1308	1311	1317	rVB	385	357	0.02%	0.003%
35	5.604	1322	1326	1329	rVB	349	293	0.02%	0.002%
36	5.723	1341	1363	1375	rBV2	643373	1757704	100.00%	12.522%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052148.D
 Acq On : 28 Nov 2022 15:24
 Operator : JC/MD
 Sample : N5785-05DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COL75DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

37	6.031	1458	1459	1465	rBV2	452	446	0.03%	0.003%
38	6.057	1465	1467	1473	rVB	514	347	0.02%	0.002%
39	6.176	1500	1504	1507	rBV2	491	454	0.03%	0.003%
40	6.247	1511	1526	1560	rBV	537737	1050206	59.75%	7.482%
41	6.482	1597	1599	1602	rVB3	544	309	0.02%	0.002%
42	6.501	1602	1605	1607	rBV	740	501	0.03%	0.004%
43	6.527	1608	1613	1615	rBV4	1499	1406	0.08%	0.010%
44	6.597	1630	1635	1639	rBV3	775	702	0.04%	0.005%
45	6.687	1648	1663	1690	rBV	399208	785336	44.68%	5.595%
46	6.970	1747	1751	1753	rBV	425	323	0.02%	0.002%
47	6.983	1753	1755	1759	rVB2	427	308	0.02%	0.002%
48	7.420	1888	1891	1895	rVB2	467	406	0.02%	0.003%
49	7.562	1923	1935	1958	rBV	196191	348006	19.80%	2.479%
50	7.716	1979	1983	1988	rBV4	305	337	0.02%	0.002%
51	7.797	2002	2008	2013	rBV4	658	808	0.05%	0.006%
52	7.826	2013	2017	2019	rBV	507	315	0.02%	0.002%
53	7.896	2025	2039	2066	rBV	754700	1311390	74.61%	9.342%
54	8.105	2100	2104	2107	rBV3	409	370	0.02%	0.003%
55	8.176	2114	2126	2155	rBV	139761	236739	13.47%	1.687%
56	8.346	2177	2179	2185	rVB3	561	396	0.02%	0.003%
57	8.382	2187	2190	2193	rBV3	638	466	0.03%	0.003%
58	8.469	2214	2217	2224	rVB5	1308	1548	0.09%	0.011%
59	8.504	2224	2228	2230	rBV2	443	321	0.02%	0.002%
60	8.546	2239	2241	2245	rBV2	455	320	0.02%	0.002%
61	8.629	2255	2267	2301	rBV	480947	890432	50.66%	6.343%
62	8.832	2328	2330	2334	rVB3	461	311	0.02%	0.002%
63	8.896	2346	2350	2354	rBV3	543	414	0.02%	0.003%
64	8.932	2356	2361	2365	rVB3	744	668	0.04%	0.005%
65	8.993	2377	2380	2383	rBV2	466	319	0.02%	0.002%
66	9.108	2413	2416	2419	rBV2	713	507	0.03%	0.004%
67	9.215	2447	2449	2453	rVB	632	395	0.02%	0.003%
68	9.414	2498	2511	2517	rBV	798910	1415395	80.53%	10.083%
69	9.687	2593	2596	2599	rBV2	619	464	0.03%	0.003%
70	9.845	2640	2645	2648	rBV2	402	396	0.02%	0.003%
71	9.912	2662	2666	2669	rBV2	452	360	0.02%	0.003%
72	9.993	2687	2691	2696	rBV2	336	397	0.02%	0.003%
73	10.124	2729	2732	2736	rVB2	538	390	0.02%	0.003%
74	10.176	2746	2748	2755	rVB2	615	575	0.03%	0.004%
75	10.214	2755	2760	2761	rBV	482	385	0.02%	0.003%
76	10.420	2821	2824	2829	rVB2	618	489	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052148.D
 Acq On : 28 Nov 2022 15:24
 Operator : JC/MD
 Sample : N5785-05DL 500X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L75DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

77	10.610	2880	2883	2886	rBV3	554	452	0.03%	0.003%
78	10.658	2895	2898	2905	rVB2	445	393	0.02%	0.003%
79	10.751	2914	2927	2949	rBV	587846	948733	53.98%	6.759%
80	10.928	2978	2982	2985	rVB3	599	443	0.03%	0.003%
81	11.076	3026	3028	3032	rBV	441	293	0.02%	0.002%
82	11.301	3096	3098	3102	rVB2	538	315	0.02%	0.002%
83	11.401	3123	3129	3132	rVB2	416	402	0.02%	0.003%
84	11.507	3159	3162	3166	rVB3	682	538	0.03%	0.004%
85	11.597	3187	3190	3194	rVB2	609	375	0.02%	0.003%
86	11.623	3195	3198	3202	rVB	673	430	0.02%	0.003%
87	11.745	3226	3236	3244	rVV2	24203	36633	2.08%	0.261%
88	11.809	3244	3256	3289	rVB2	645398	1327310	75.51%	9.456%
89	12.192	3361	3375	3400	rVV3	725370	1551821	88.29%	11.055%
90	12.645	3513	3516	3520	rVB2	957	702	0.04%	0.005%
91	12.677	3524	3526	3533	rVB2	543	559	0.03%	0.004%
92	12.742	3541	3546	3550	rBV3	657	745	0.04%	0.005%
93	12.790	3558	3561	3564	rBV2	458	397	0.02%	0.003%
94	13.124	3662	3665	3668	rBV	507	341	0.02%	0.002%
95	13.713	3845	3848	3851	rBV3	723	543	0.03%	0.004%
96	13.841	3878	3888	3902	rBV3	33443	55029	3.13%	0.392%
97	14.240	4009	4012	4015	rVB4	689	461	0.03%	0.003%
98	14.259	4015	4018	4020	rBV2	668	458	0.03%	0.003%
99	14.330	4032	4040	4048	rBV6	7535	11755	0.67%	0.084%
100	14.671	4144	4146	4151	rVB3	682	393	0.02%	0.003%




Sum of corrected areas: 14037172

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052148.D
Acq On : 28 Nov 2022 15:24
Operator : JC/MD
Sample : N5785-05DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COL75DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

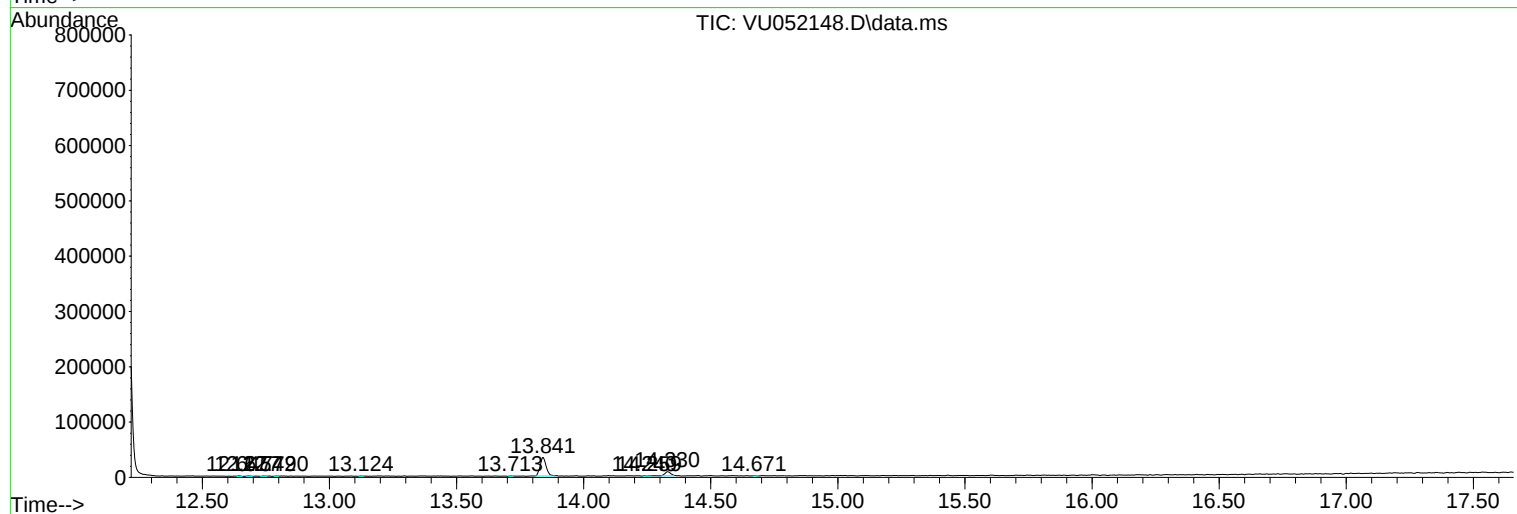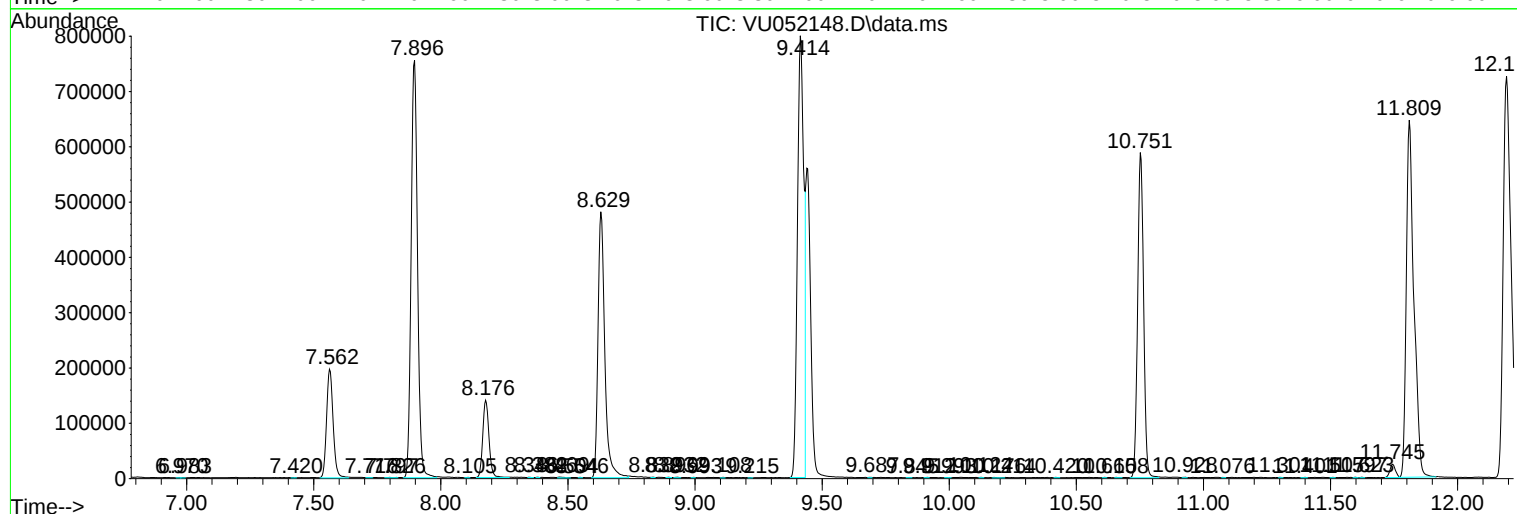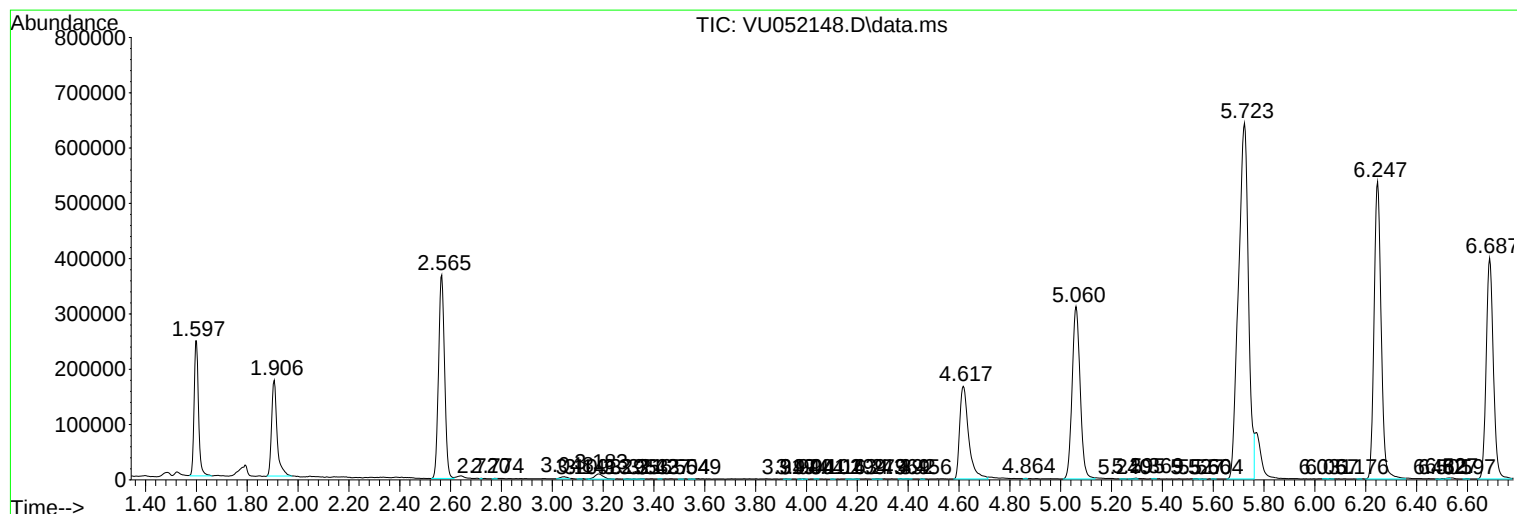

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052148.D
Acq On : 28 Nov 2022 15:24
Operator : JC/MD
Sample : N5785-05DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L75DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052148.D
Acq On : 28 Nov 2022 15:24
Operator : JC/MD
Sample : N5785-05DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L75DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc