

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052149.D
 Acq On : 28 Nov 2022 15:48
 Operator : JC/MD
 Sample : N5785-05 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COL75

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

Signal : TIC: VU052149.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.523	53	57	72	rVB2	6473	8748	0.15%	0.038%
2	1.600	73	81	97	rVB	248526	290830	4.98%	1.276%
3	1.793	125	141	148	rVB6	17638	39584	0.68%	0.174%
4	1.906	167	176	203	rVB	172153	267339	4.58%	1.173%
5	2.565	368	381	396	rBV	376422	611737	10.48%	2.684%
6	2.977	506	509	512	rBV2	601	367	0.01%	0.002%
7	3.044	521	530	542	rBV2	4562	8285	0.14%	0.036%
8	3.115	548	552	555	rBV2	418	388	0.01%	0.002%
9	3.182	560	573	586	rVV	8065	18390	0.32%	0.081%
10	3.372	630	632	637	rVV2	444	348	0.01%	0.002%
11	3.472	658	663	666	rBV	392	403	0.01%	0.002%
12	3.523	675	679	681	rBV	457	314	0.01%	0.001%
13	3.735	741	745	752	rBV3	515	609	0.01%	0.003%
14	3.809	764	768	775	rVB2	608	721	0.01%	0.003%
15	3.861	780	784	791	rVB3	283	313	0.01%	0.001%
16	3.903	791	797	804	rVB2	408	502	0.01%	0.002%
17	3.989	819	824	831	rBV2	412	529	0.01%	0.002%
18	4.067	844	848	854	rVV	483	598	0.01%	0.003%
19	4.259	905	908	916	rVB2	493	642	0.01%	0.003%
20	4.301	916	921	922	rBV	578	520	0.01%	0.002%
21	4.346	928	935	940	rBV2	618	800	0.01%	0.004%
22	4.475	969	975	979	rBV2	668	582	0.01%	0.003%
23	4.526	984	991	997	rBV4	538	823	0.01%	0.004%
24	4.616	1008	1019	1048	rBV	166976	399985	6.86%	1.755%
25	4.935	1116	1118	1125	rVV2	492	491	0.01%	0.002%
26	4.970	1125	1129	1133	rVV3	390	334	0.01%	0.001%
27	5.060	1140	1157	1184	rBV	310165	689171	11.81%	3.024%
28	5.292	1225	1229	1231	rVV4	617	454	0.01%	0.002%
29	5.375	1250	1255	1259	rBV2	741	819	0.01%	0.004%
30	5.520	1290	1300	1312	rBV5	1988	4236	0.07%	0.019%
31	5.591	1319	1322	1326	rBV	617	413	0.01%	0.002%
32	5.722	1342	1363	1372	rBV2	653093	1777693	30.47%	7.799%
33	5.944	1430	1432	1439	rVB4	684	574	0.01%	0.003%
34	6.018	1451	1455	1457	rBV3	579	407	0.01%	0.002%
35	6.105	1477	1482	1483	rBV	734	456	0.01%	0.002%
36	6.247	1512	1526	1553	rBV	562181	1076821	18.46%	4.724%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052149.D
 Acq On : 28 Nov 2022 15:48
 Operator : JC/MD
 Sample : N5785-05 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 COL75

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

37	6.529	1607	1614	1619	rBV4	2036	2740	0.05%	0.012%
38	6.687	1647	1663	1692	rBV	405980	797411	13.67%	3.498%
39	6.883	1721	1724	1727	rBV2	609	340	0.01%	0.001%
40	6.902	1727	1730	1735	rVB3	619	494	0.01%	0.002%
41	6.989	1751	1757	1758	rBV	590	463	0.01%	0.002%
42	7.060	1776	1779	1781	rBV	463	320	0.01%	0.001%
43	7.073	1781	1783	1788	rVV2	416	335	0.01%	0.001%
44	7.115	1793	1796	1804	rVB2	710	949	0.02%	0.004%
45	7.163	1804	1811	1814	rBV3	647	886	0.02%	0.004%
46	7.372	1871	1876	1880	rBV	345	361	0.01%	0.002%
47	7.465	1900	1905	1910	rBV2	449	537	0.01%	0.002%
48	7.562	1923	1935	1959	rBV	197197	352057	6.03%	1.545%
49	7.722	1982	1985	1989	rVB3	421	303	0.01%	0.001%
50	7.748	1989	1993	1995	rBV3	376	326	0.01%	0.001%
51	7.764	1995	1998	2002	rVB3	714	591	0.01%	0.003%
52	7.803	2006	2010	2014	rVB2	615	525	0.01%	0.002%
53	7.896	2021	2039	2066	rBV	778485	1340460	22.97%	5.881%
54	8.176	2114	2126	2144	rBV	137963	238346	4.08%	1.046%
55	8.420	2197	2202	2206	rVB4	729	682	0.01%	0.003%
56	8.459	2211	2214	2217	rBV2	450	350	0.01%	0.002%
57	8.549	2240	2242	2247	rVB2	517	414	0.01%	0.002%
58	8.629	2256	2267	2298	rBV	475908	870613	14.92%	3.820%
59	9.105	2411	2415	2422	rVB3	514	587	0.01%	0.003%
60	9.163	2430	2433	2437	rVV4	466	346	0.01%	0.002%
61	9.208	2441	2447	2455	rVB2	600	820	0.01%	0.004%
62	9.243	2455	2458	2461	rBV2	504	348	0.01%	0.002%
63	9.269	2462	2466	2472	rVB	548	626	0.01%	0.003%
64	9.317	2477	2481	2485	rBV3	603	617	0.01%	0.003%
65	9.443	2498	2520	2569	rBV2	2798888	5834743	100.00%	25.598%
66	9.629	2573	2578	2582	rBV6	1165	1353	0.02%	0.006%
67	9.787	2625	2627	2630	rVB3	650	361	0.01%	0.002%
68	9.803	2630	2632	2638	rVB4	819	725	0.01%	0.003%
69	9.832	2638	2641	2643	rBV2	610	457	0.01%	0.002%
70	10.041	2703	2706	2709	rBV	508	354	0.01%	0.002%
71	10.095	2721	2723	2727	rBV2	712	426	0.01%	0.002%
72	10.127	2727	2733	2735	rVV3	309	328	0.01%	0.001%
73	10.208	2754	2758	2763	rVB	342	344	0.01%	0.002%
74	10.234	2763	2766	2771	rVB3	475	428	0.01%	0.002%
75	10.343	2792	2800	2805	rBV2	610	783	0.01%	0.003%
76	10.533	2856	2859	2865	rVV2	322	388	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052149.D
 Acq On : 28 Nov 2022 15:48
 Operator : JC/MD
 Sample : N5785-05 100X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0L75

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

77	10.632	2887	2890	2895	rVB2	933	696	0.01%	0.003%
78	10.674	2895	2903	2909	rBV	580	852	0.01%	0.004%
79	10.751	2914	2927	2952	rBV	575998	944000	16.18%	4.142%
80	10.931	2980	2983	2988	rVB3	608	493	0.01%	0.002%
81	11.050	3018	3020	3024	rVB2	476	313	0.01%	0.001%
82	11.095	3030	3034	3036	rBV2	373	322	0.01%	0.001%
83	11.375	3116	3121	3124	rVB2	458	389	0.01%	0.002%
84	11.623	3195	3198	3203	rVB	573	414	0.01%	0.002%
85	11.655	3203	3208	3211	rBV3	589	521	0.01%	0.002%
86	11.742	3224	3235	3245	rBV	125991	202244	3.47%	0.887%
87	11.832	3245	3263	3284	rVV2	1172965	2866409	49.13%	12.576%
88	12.037	3324	3327	3329	rBV4	448	304	0.01%	0.001%
89	12.208	3361	3380	3415	rBV2	1742709	3703662	63.48%	16.249%
90	12.516	3473	3476	3479	rBV4	608	342	0.01%	0.002%
91	12.886	3588	3591	3596	rBV2	529	459	0.01%	0.002%
92	12.973	3614	3618	3628	rVB5	1373	1554	0.03%	0.007%
93	13.298	3715	3719	3721	rBV	473	433	0.01%	0.002%
94	13.545	3793	3796	3800	rBV2	636	438	0.01%	0.002%
95	13.838	3875	3887	3908	rBV	199149	332675	5.70%	1.460%
96	14.130	3976	3978	3984	rVB3	726	581	0.01%	0.003%
97	14.169	3987	3990	3994	rBV	587	498	0.01%	0.002%
98	14.330	4029	4040	4062	rBV2	45362	75959	1.30%	0.333%
99	14.876	4207	4210	4213	rBV2	838	685	0.01%	0.003%
100	14.966	4235	4238	4243	rVB3	779	558	0.01%	0.002%




Sum of corrected areas: 22793564

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052149.D
Acq On : 28 Nov 2022 15:48
Operator : JC/MD
Sample : N5785-05 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COL75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

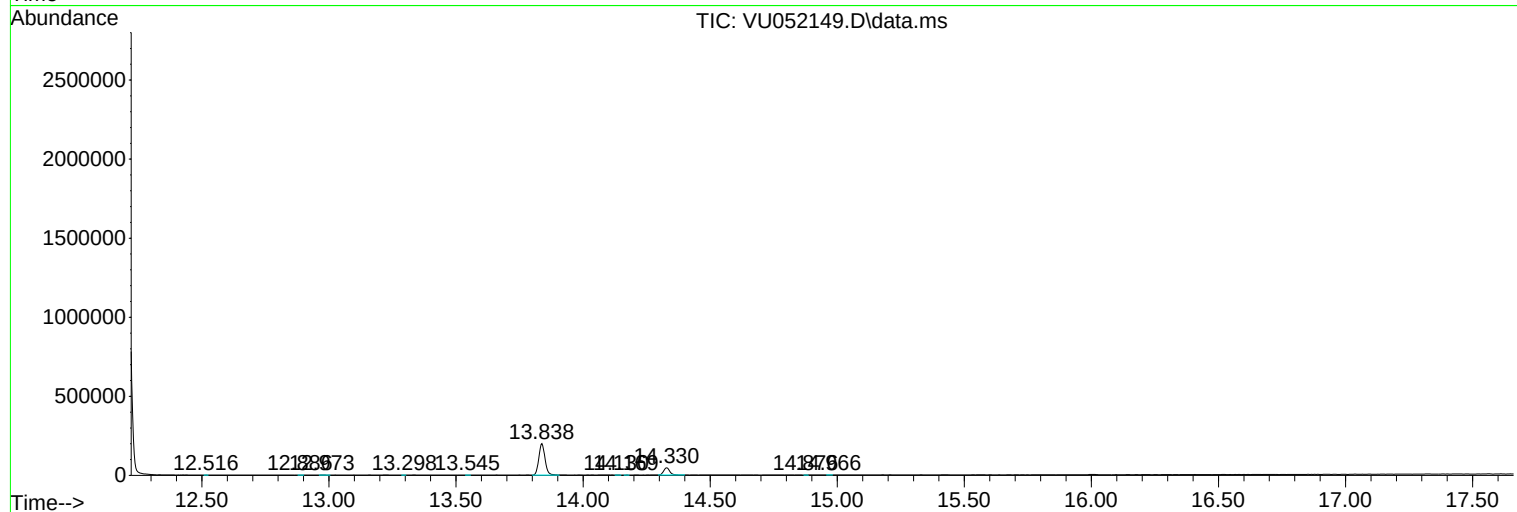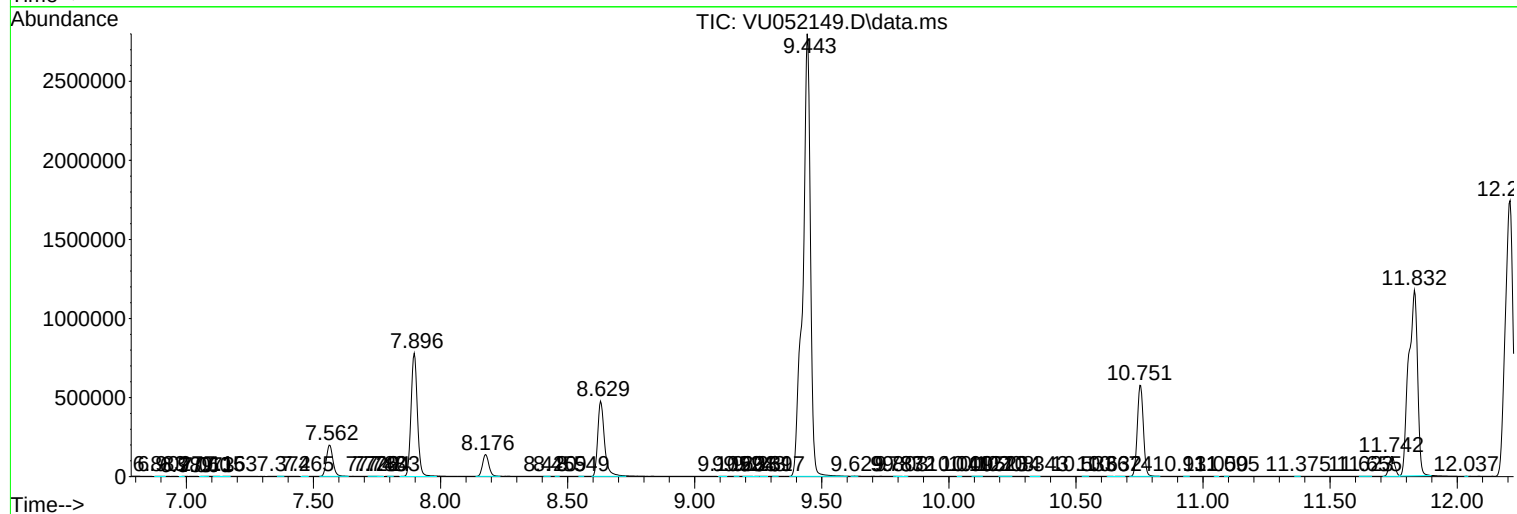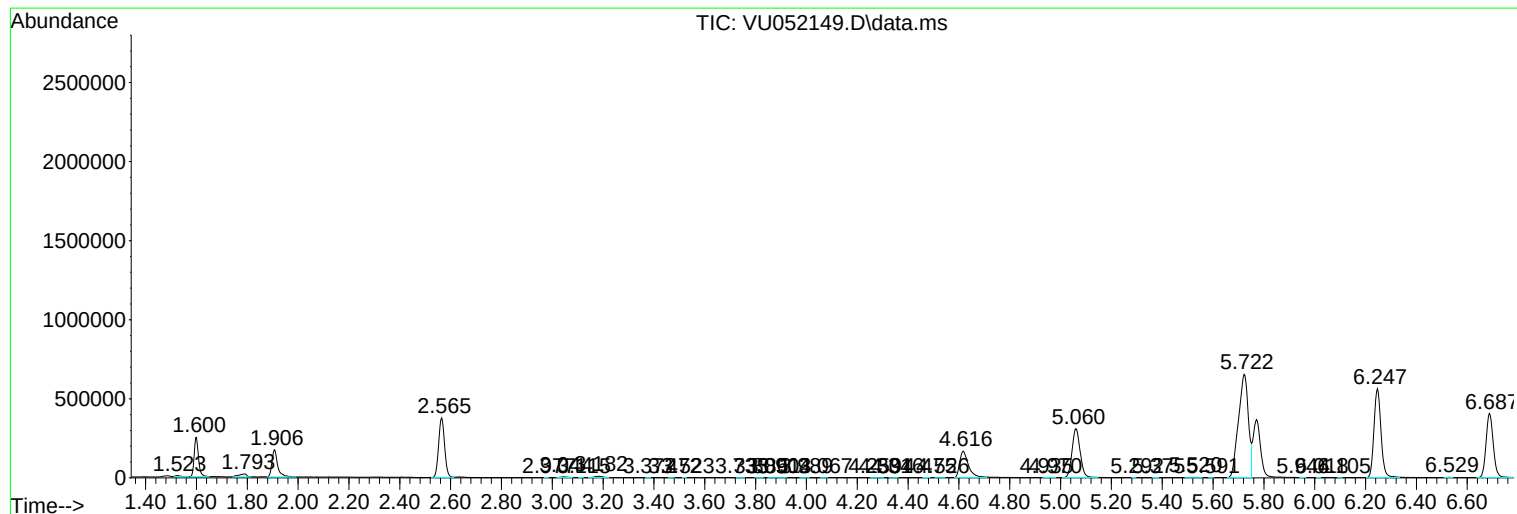

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052149.D
Acq On : 28 Nov 2022 15:48
Operator : JC/MD
Sample : N5785-05 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052149.D
Acq On : 28 Nov 2022 15:48
Operator : JC/MD
Sample : N5785-05 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0L75

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
