

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052150.D
 Acq On : 28 Nov 2022 16:12
 Operator : JC/MD
 Sample : N5785-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

Signal : TIC: VU052150.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.523	53	57	67	rBV	4913	6757	0.39%	0.054%
2	1.597	73	80	101	rVB	236828	283843	16.51%	2.255%
3	1.906	167	176	200	rVB	165999	248282	14.44%	1.973%
4	2.565	368	381	396	rBV	355276	583785	33.95%	4.639%
5	2.874	470	477	479	rBV3	336	375	0.02%	0.003%
6	2.915	486	490	493	rBV2	519	551	0.03%	0.004%
7	3.044	516	530	543	rBV3	8456	16420	0.95%	0.130%
8	3.173	566	570	571	rBV2	921	560	0.03%	0.004%
9	3.288	602	606	611	rBV3	372	462	0.03%	0.004%
10	3.311	611	613	621	rVB2	502	561	0.03%	0.004%
11	3.356	621	627	630	rBV2	688	684	0.04%	0.005%
12	3.459	655	659	664	rVB3	362	363	0.02%	0.003%
13	3.639	708	715	717	rBV2	571	663	0.04%	0.005%
14	3.841	769	778	782	rBV2	485	590	0.03%	0.005%
15	3.912	797	800	805	rBV2	384	353	0.02%	0.003%
16	4.163	872	878	879	rBV3	409	415	0.02%	0.003%
17	4.224	893	897	900	rVB2	423	324	0.02%	0.003%
18	4.272	906	912	915	rBV3	349	391	0.02%	0.003%
19	4.382	938	946	949	rBV3	353	367	0.02%	0.003%
20	4.433	955	962	964	rBV2	426	382	0.02%	0.003%
21	4.533	989	993	994	rBV	456	325	0.02%	0.003%
22	4.616	1007	1019	1047	rBV	162265	390223	22.69%	3.101%
23	4.951	1121	1123	1128	rVB2	452	326	0.02%	0.003%
24	5.060	1140	1157	1180	rBV	303220	669238	38.92%	5.318%
25	5.227	1206	1209	1212	rVB2	490	374	0.02%	0.003%
26	5.279	1219	1225	1226	rBV3	549	503	0.03%	0.004%
27	5.366	1249	1252	1256	rVV	496	357	0.02%	0.003%
28	5.488	1286	1290	1292	rBV2	426	363	0.02%	0.003%
29	5.610	1326	1328	1332	rVB2	566	331	0.02%	0.003%
30	5.632	1332	1335	1342	rBV2	430	484	0.03%	0.004%
31	5.722	1342	1363	1400	rBV2	633589	1719463	100.00%	13.663%
32	5.848	1400	1402	1406	rVV3	1561	1171	0.07%	0.009%
33	5.957	1433	1436	1442	rVB	768	585	0.03%	0.005%
34	5.989	1442	1446	1449	rVB2	452	412	0.02%	0.003%
35	6.015	1449	1454	1457	rBV3	568	488	0.03%	0.004%
36	6.095	1476	1479	1482	rVV3	416	359	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052150.D
 Acq On : 28 Nov 2022 16:12
 Operator : JC/MD
 Sample : N5785-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

37	6.189	1504	1508	1512	rBV2	562	605	0.04%	0.005%
38	6.247	1512	1526	1560	rBV	522043	1005122	58.46%	7.987%
39	6.526	1602	1613	1617	rBV6	2489	3526	0.21%	0.028%
40	6.600	1631	1636	1638	rBV2	446	373	0.02%	0.003%
41	6.687	1648	1663	1694	rBV	399545	783761	45.58%	6.228%
42	6.806	1694	1700	1703	rBV6	1088	1198	0.07%	0.010%
43	6.986	1754	1756	1763	rVB2	411	430	0.03%	0.003%
44	7.108	1788	1794	1799	rBV2	487	557	0.03%	0.004%
45	7.356	1867	1871	1874	rBV	433	361	0.02%	0.003%
46	7.439	1888	1897	1900	rBV2	467	577	0.03%	0.005%
47	7.565	1923	1936	1958	rBV	189455	340549	19.81%	2.706%
48	7.835	2015	2020	2023	rVB2	351	335	0.02%	0.003%
49	7.896	2023	2039	2064	rBV	730790	1278694	74.37%	10.160%
50	8.127	2106	2111	2114	rBV3	567	560	0.03%	0.004%
51	8.176	2115	2126	2142	rBV	139748	230682	13.42%	1.833%
52	8.410	2196	2199	2203	rBV	421	357	0.02%	0.003%
53	8.459	2208	2214	2218	rBV4	612	694	0.04%	0.006%
54	8.507	2224	2229	2231	rBV	504	472	0.03%	0.004%
55	8.571	2246	2249	2251	rBV2	437	339	0.02%	0.003%
56	8.629	2255	2267	2294	rBV	461381	851212	49.50%	6.764%
57	8.867	2336	2341	2343	rBV	595	582	0.03%	0.005%
58	8.909	2347	2354	2358	rBV4	777	749	0.04%	0.006%
59	9.002	2379	2383	2387	rVB2	513	563	0.03%	0.004%
60	9.076	2403	2406	2412	rBV2	379	377	0.02%	0.003%
61	9.169	2432	2435	2443	rVB3	556	610	0.04%	0.005%
62	9.208	2443	2447	2449	rBV	654	426	0.02%	0.003%
63	9.311	2476	2479	2482	rBV	591	424	0.02%	0.003%
64	9.414	2497	2511	2536	rBV	743793	1247971	72.58%	9.916%
65	9.787	2625	2627	2633	rVB3	474	427	0.02%	0.003%
66	9.851	2639	2647	2652	rBV2	622	916	0.05%	0.007%
67	9.889	2657	2659	2665	rVB3	518	362	0.02%	0.003%
68	9.922	2665	2669	2675	rBV2	390	472	0.03%	0.004%
69	10.044	2701	2707	2709	rBV2	322	371	0.02%	0.003%
70	10.063	2710	2713	2716	rVV	579	413	0.02%	0.003%
71	10.079	2716	2718	2723	rVV2	479	348	0.02%	0.003%
72	10.111	2723	2728	2731	rVB3	568	482	0.03%	0.004%
73	10.275	2776	2779	2784	rVB2	616	537	0.03%	0.004%
74	10.301	2784	2787	2791	rBV2	410	449	0.03%	0.004%
75	10.475	2837	2841	2843	rVV4	637	536	0.03%	0.004%
76	10.545	2860	2863	2870	rVB	632	587	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
 Data File : VU052150.D
 Acq On : 28 Nov 2022 16:12
 Operator : JC/MD
 Sample : N5785-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
 Title : VOC Analysis

77	10.751	2915	2927	2950	rBV	567170	912933	53.09%	7.254%
78	11.108	3035	3038	3041	rBV2	476	372	0.02%	0.003%
79	11.298	3093	3097	3099	rBV2	430	357	0.02%	0.003%
80	11.362	3110	3117	3118	rBV2	463	476	0.03%	0.004%
81	11.436	3135	3140	3143	rVB2	520	431	0.03%	0.003%
82	11.651	3204	3207	3211	rBV2	472	394	0.02%	0.003%
83	11.745	3232	3236	3238	rBV2	1136	1029	0.06%	0.008%
84	11.809	3244	3256	3284	rBV	554561	932940	54.26%	7.413%
85	12.060	3331	3334	3337	rBV2	390	326	0.02%	0.003%
86	12.192	3361	3375	3396	rBV	589243	1018631	59.24%	8.094%
87	12.426	3443	3448	3453	rBV2	550	741	0.04%	0.006%
88	12.539	3479	3483	3486	rBV	415	422	0.02%	0.003%
89	12.796	3559	3563	3566	rBV2	537	512	0.03%	0.004%
90	12.844	3574	3578	3581	rBV2	549	497	0.03%	0.004%
91	12.893	3590	3593	3597	rVB2	628	440	0.03%	0.003%
92	13.118	3660	3663	3666	rVB3	626	378	0.02%	0.003%
93	13.147	3666	3672	3674	rBV2	370	402	0.02%	0.003%
94	13.587	3805	3809	3811	rVV3	462	327	0.02%	0.003%
95	13.732	3851	3854	3859	rBV	727	734	0.04%	0.006%
96	13.841	3880	3888	3903	rBV4	9448	16221	0.94%	0.129%
97	13.979	3927	3931	3934	rBV3	692	583	0.03%	0.005%
98	14.182	3992	3994	3997	rBV2	599	377	0.02%	0.003%
99	14.330	4032	4040	4053	rVB5	3529	6177	0.36%	0.049%
100	14.680	4147	4149	4152	rBV2	619	399	0.02%	0.003%




Sum of corrected areas: 12585235

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052150.D
Acq On : 28 Nov 2022 16:12
Operator : JC/MD
Sample : N5785-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

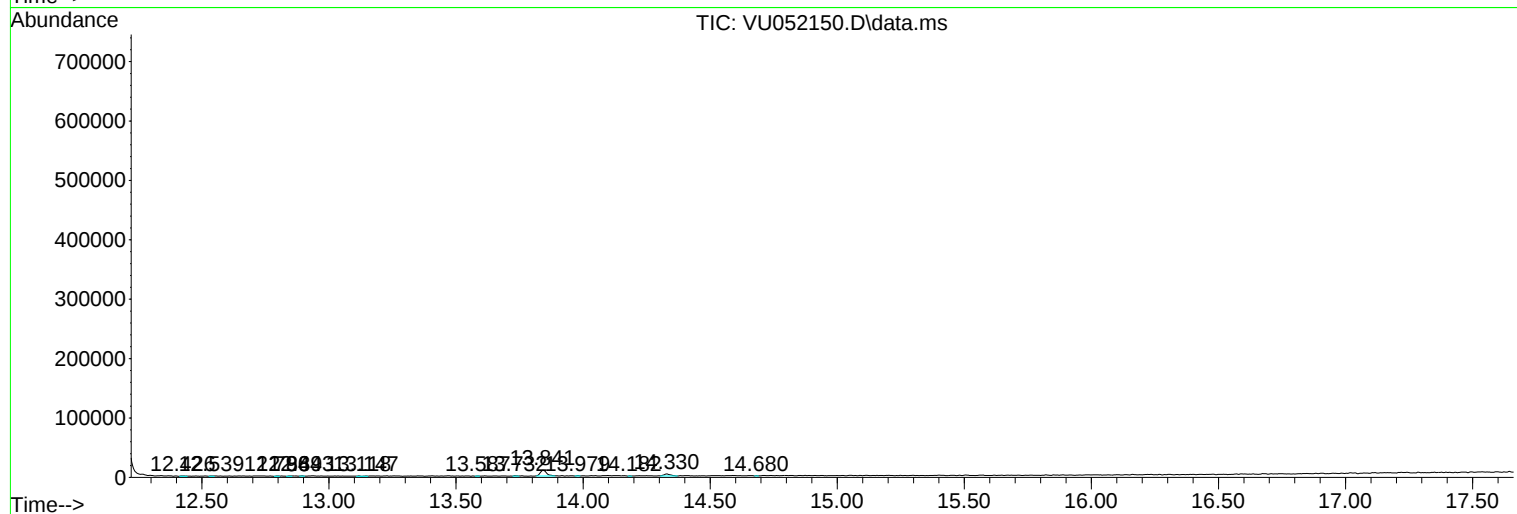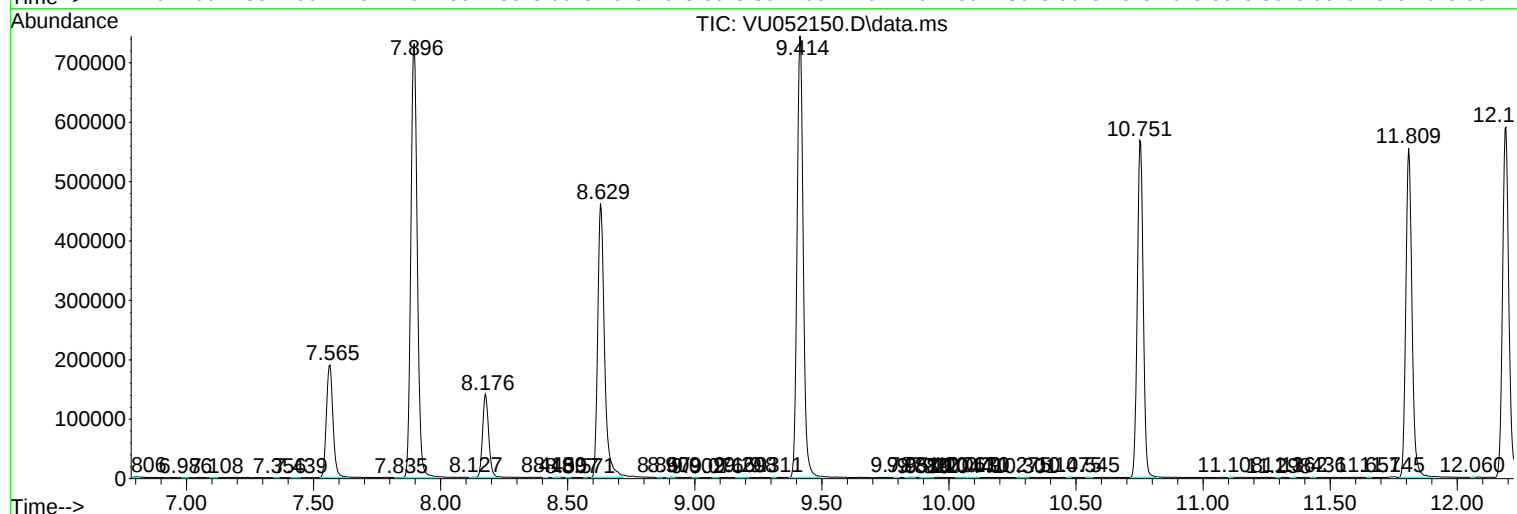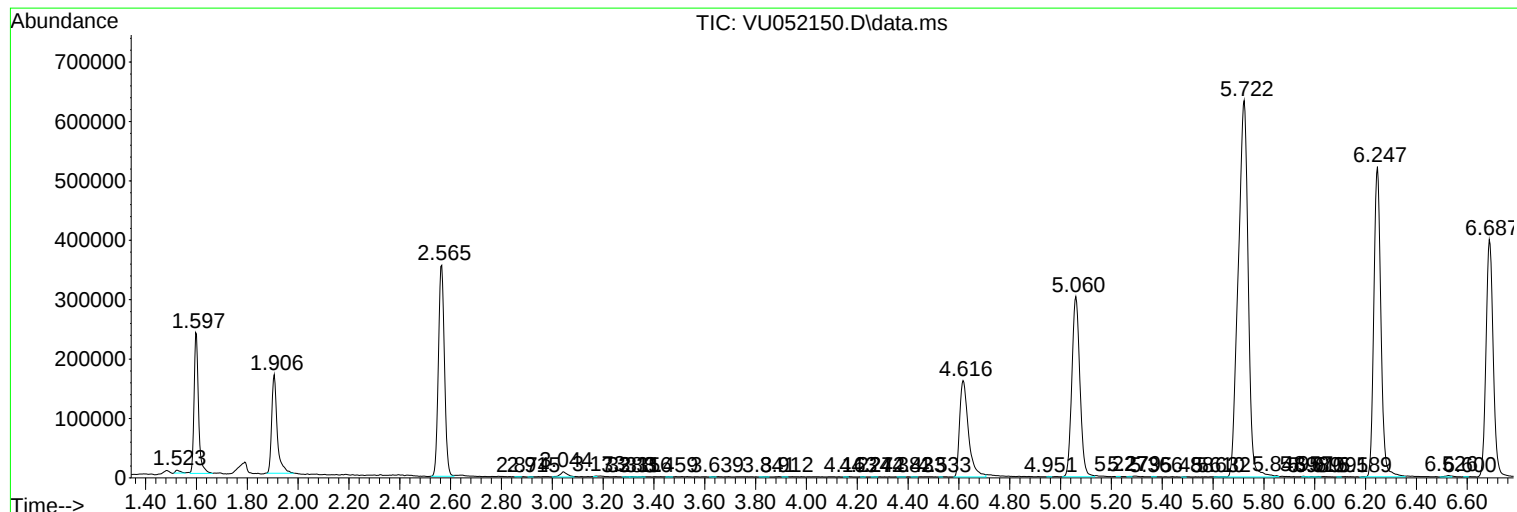

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052150.D
Acq On : 28 Nov 2022 16:12
Operator : JC/MD
Sample : N5785-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052150.D
Acq On : 28 Nov 2022 16:12
Operator : JC/MD
Sample : N5785-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------