


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112822\
Data File : VU052139.D
Acq On : 28 Nov 2022 08:55
Operator : JC/MD
Sample : BFB149
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB149

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM112122WMA.M
Title : VOC Analysis
Last Update : Mon Nov 28 21:44:47 2022

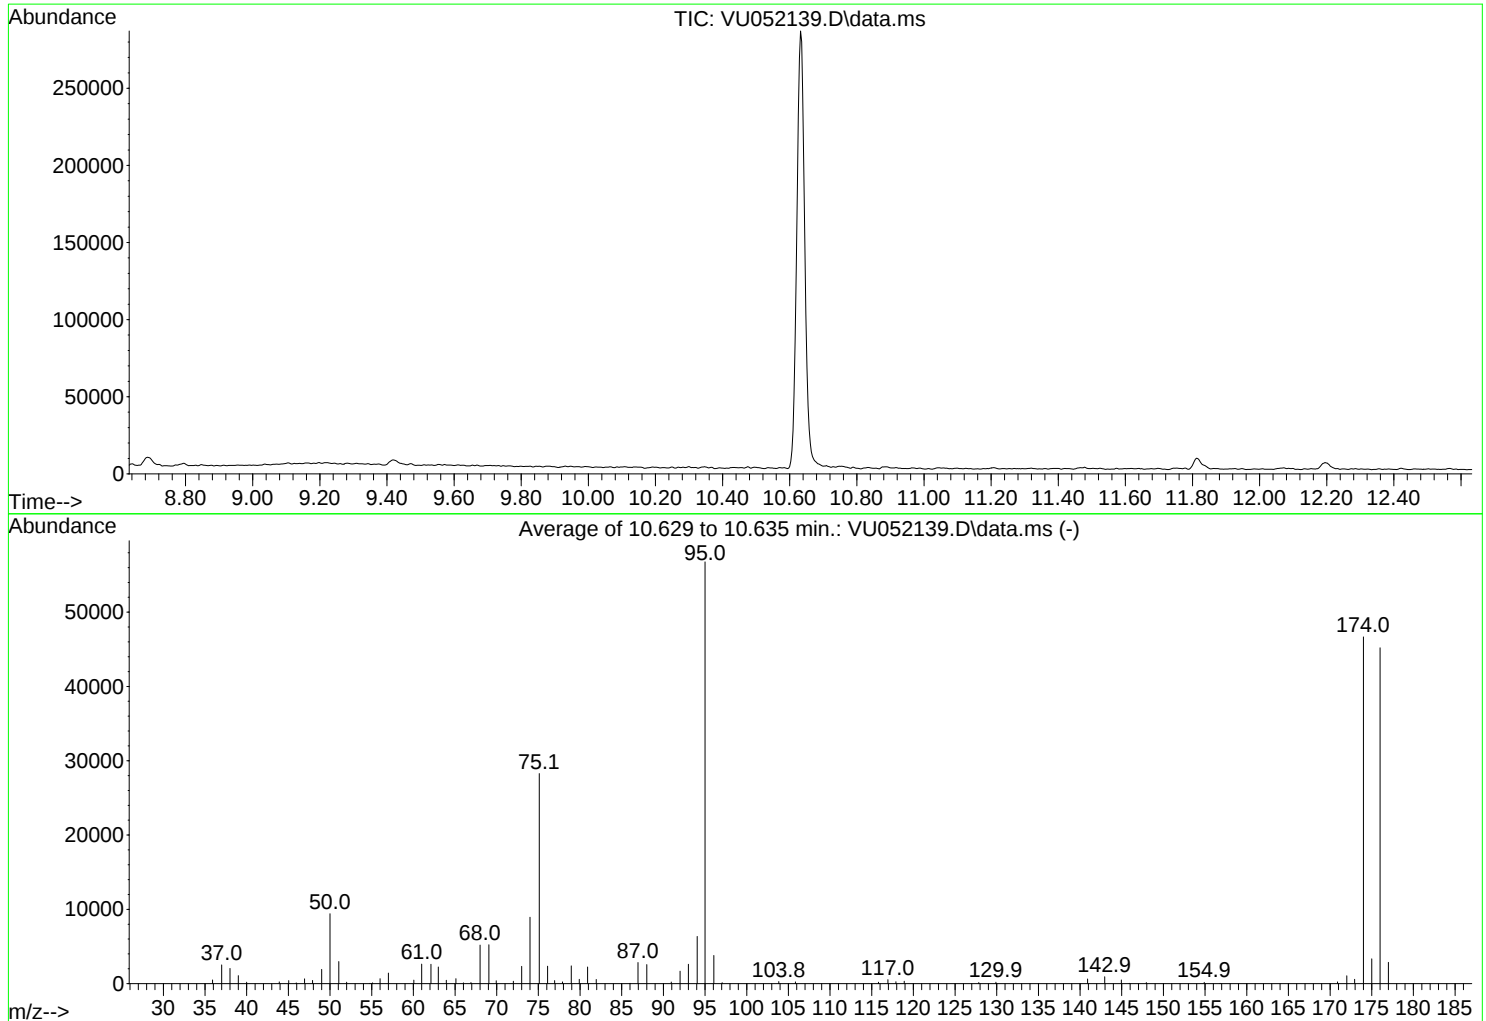

AutoFind: Scans 2889, 2890, 2891; Background Corrected with Scan 2877

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.6	9416	PASS
75	95	30	80	49.8	28275	PASS
95	95	100	100	100.0	56771	PASS
96	95	5	9	6.7	3782	PASS
173	174	0.00	2	1.2	576	PASS
174	95	50	120	82.2	46675	PASS
175	174	5	9	7.1	3329	PASS
176	174	95	101	96.9	45211	PASS
177	176	5	9	6.3	2869	PASS

m/z	Abundance
35.90	1308.0
38.00	532.0
40.00	1406.0
43.90	387.0

Instrument :
MSVOA_U
ClientSampleId :
BFB149

m/z	Abundance
36.00	1781.0
37.00	2347.0
38.00	2538.0
39.00	1105.0
40.00	1497.0
44.00	696.0
45.00	430.0
46.10	118.0
47.00	708.0
47.90	437.0
49.00	1892.0
50.00	9186.0
51.00	3121.0
52.00	214.0
55.10	194.0
56.00	704.0
57.00	1446.0
60.10	513.0
61.00	2751.0
62.10	2583.0
63.00	2236.0
63.90	445.0
65.10	681.0
66.00	106.0
67.00	173.0
68.00	4796.0
69.10	5112.0
69.90	406.0
72.00	341.0
73.00	2404.0
74.00	8732.0
75.10	27880.0
76.10	2285.0
77.00	444.0
77.90	236.0
79.00	2381.0
79.90	585.0
80.90	2227.0
81.90	566.0
86.90	2675.0
88.00	2475.0
91.00	212.0
92.00	1709.0
93.00	2470.0
94.10	6170.0
95.00	54096.0
96.00	3863.0
97.10	147.0
103.80	281.0
105.80	247.0
115.80	172.0
117.00	532.0
117.90	267.0
118.90	316.0
127.80	151.0
129.90	212.0
140.90	660.0
143.00	890.0
145.00	466.0
148.00	135.0
154.90	171.0
170.90	177.0
172.00	943.0
173.00	513.0
174.00	44280.0
175.00	3332.0
176.00	42864.0
177.00	2892.0

Instrument :
MSVOA_U
ClientSampleId :
BFB149

m/z	Abundance
36.00	1822.0
37.00	2637.0
38.00	2634.0
39.00	1123.0
40.00	1614.0
44.00	643.0
45.10	441.0
45.90	114.0
47.00	682.0
47.90	460.0
49.00	1997.0
50.00	9616.0
51.00	2981.0
52.00	187.0
55.10	122.0
56.00	675.0
57.00	1466.0
60.10	478.0
61.00	2705.0
62.10	2648.0
63.00	2272.0
64.00	480.0
65.10	673.0
66.00	109.0
66.90	156.0
68.00	5356.0
69.00	5385.0
69.90	414.0
72.00	343.0
73.00	2367.0
74.00	9284.0
75.10	29352.0
76.10	2415.0
77.00	436.0
77.90	244.0
79.00	2498.0
79.90	576.0
80.90	2296.0
81.90	578.0
87.00	2906.0
88.00	2629.0
91.00	219.0
92.00	1764.0
93.00	2673.0
94.10	6566.0
95.00	58552.0
96.00	3896.0
97.00	144.0
103.80	273.0
105.80	258.0
115.80	202.0
117.00	557.0
117.90	278.0
118.90	327.0
127.90	156.0
129.90	213.0
140.90	647.0
143.00	960.0
145.00	513.0
147.90	148.0
154.90	193.0
170.90	254.0
172.00	1098.0
173.00	599.0
174.00	47904.0
175.00	3448.0
176.00	46504.0
177.00	2931.0

Instrument :
MSVOA_U
ClientSampleId :
BFB149

m/z	Abundance
36.00	1784.0
37.00	2554.0
38.00	2590.0
39.00	994.0
40.00	1714.0
43.90	566.0
45.00	386.0
45.80	116.0
46.90	567.0
47.90	405.0
49.00	1888.0
50.00	9445.0
51.10	2803.0
52.00	161.0
54.80	111.0
56.00	649.0
57.00	1323.0
60.00	404.0
61.00	2409.0
62.10	2581.0
63.00	2235.0
64.00	454.0
65.10	622.0
66.00	112.0
66.80	120.0
68.00	5439.0
69.00	5218.0
70.00	362.0
72.00	286.0
73.00	2205.0
74.00	8830.0
75.10	27592.0
76.10	2361.0
76.90	376.0
77.90	221.0
78.90	2318.0
79.90	592.0
80.90	2187.0
82.00	541.0
86.00	111.0
87.00	2945.0
88.00	2582.0
90.90	195.0
92.00	1579.0
93.00	2681.0
94.00	6319.0
95.00	57664.0
96.10	3586.0
97.00	133.0
103.90	257.0
105.90	237.0
115.80	212.0
116.90	514.0
117.90	246.0
118.90	333.0
127.90	144.0
129.90	178.0
140.90	554.0
142.90	962.0
144.90	490.0
145.90	109.0
148.00	147.0
154.90	181.0
156.80	130.0
170.90	304.0
172.00	1155.0
172.90	616.0
174.00	47840.0
175.00	3206.0
176.00	46264.0
177.00	2784.0

Instrument :
MSVOA_U
ClientSampleId :
BFB149