

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112823\
 Data File : VU056624.D
 Acq On : 28 Nov 2023 12:53
 Operator : MD/SY
 Sample : 05554-04
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B29

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU056624.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	106	rVB	115714	131733	12.42%	1.478%
2	1.908	184	192	207	rVB	93421	129379	12.20%	1.451%
3	2.563	382	396	409	rBV	204025	330592	31.17%	3.708%
4	4.615	1024	1034	1072	rBV	138174	371530	35.04%	4.167%
5	5.055	1154	1171	1198	rBV	204273	470515	44.37%	5.278%
6	5.721	1356	1378	1401	rBV2	404201	1060447	100.00%	11.895%
7	6.242	1524	1540	1562	rBV	346820	682801	64.39%	7.659%
8	6.685	1664	1678	1700	rBV	262716	518945	48.94%	5.821%
9	7.107	1797	1809	1823	rBV3	6708	12880	1.21%	0.144%
10	7.560	1937	1950	1973	rBV	132149	240203	22.65%	2.694%
11	7.894	2041	2054	2071	rBV	503591	911409	85.95%	10.223%
12	8.177	2130	2142	2160	rBV2	79130	139948	13.20%	1.570%
13	8.547	2247	2257	2272	rBV3	52300	93324	8.80%	1.047%
14	8.628	2272	2282	2321	rBV2	536937	1042808	98.34%	11.697%
15	8.804	2326	2337	2350	rVB6	17004	37691	3.55%	0.423%
16	9.412	2514	2526	2558	rBV	501152	889327	83.86%	9.976%
17	10.750	2927	2942	2967	rBV	186579	307019	28.95%	3.444%
18	11.807	3259	3271	3303	rBV	463729	765320	72.17%	8.585%
19	12.187	3376	3389	3410	rBV	461502	779226	73.48%	8.741%




Sum of corrected areas: 8915097

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112823\
Data File : VU056624.D
Acq On : 28 Nov 2023 12:53
Operator : MD/SY
Sample : 05554-04
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

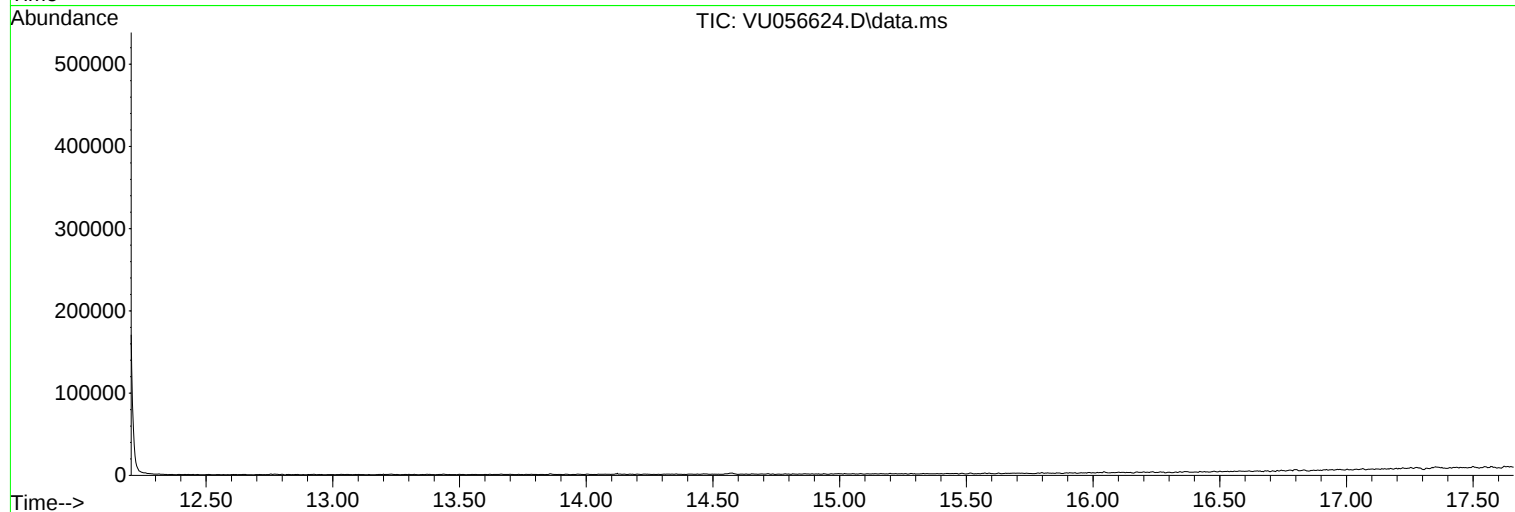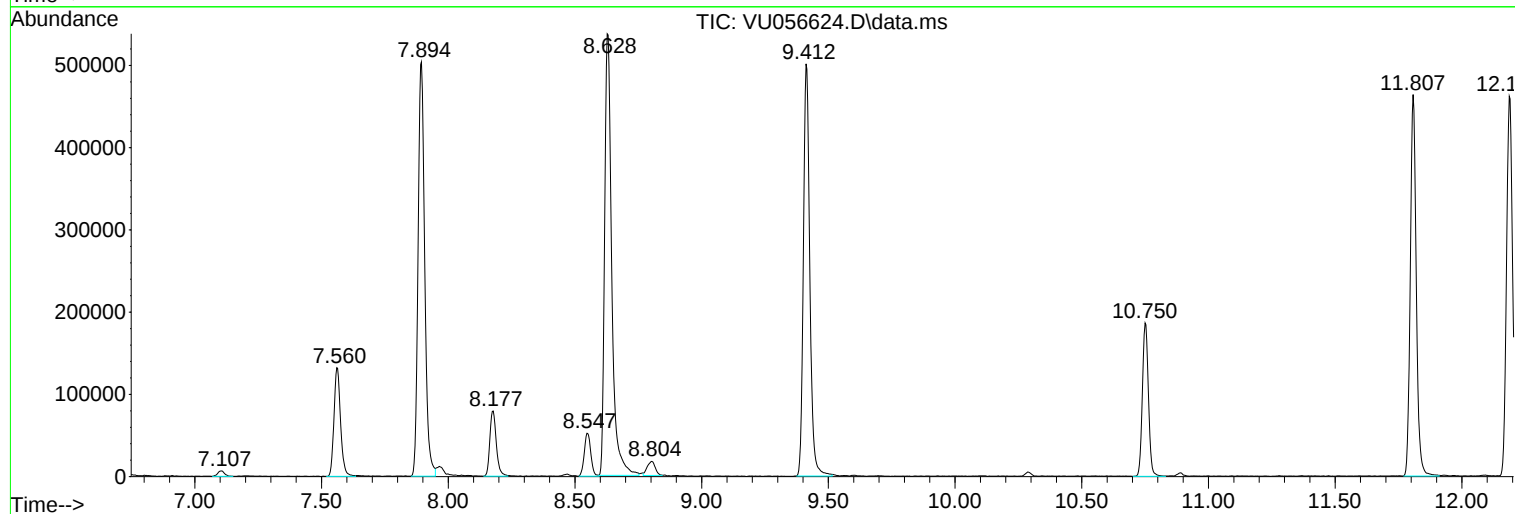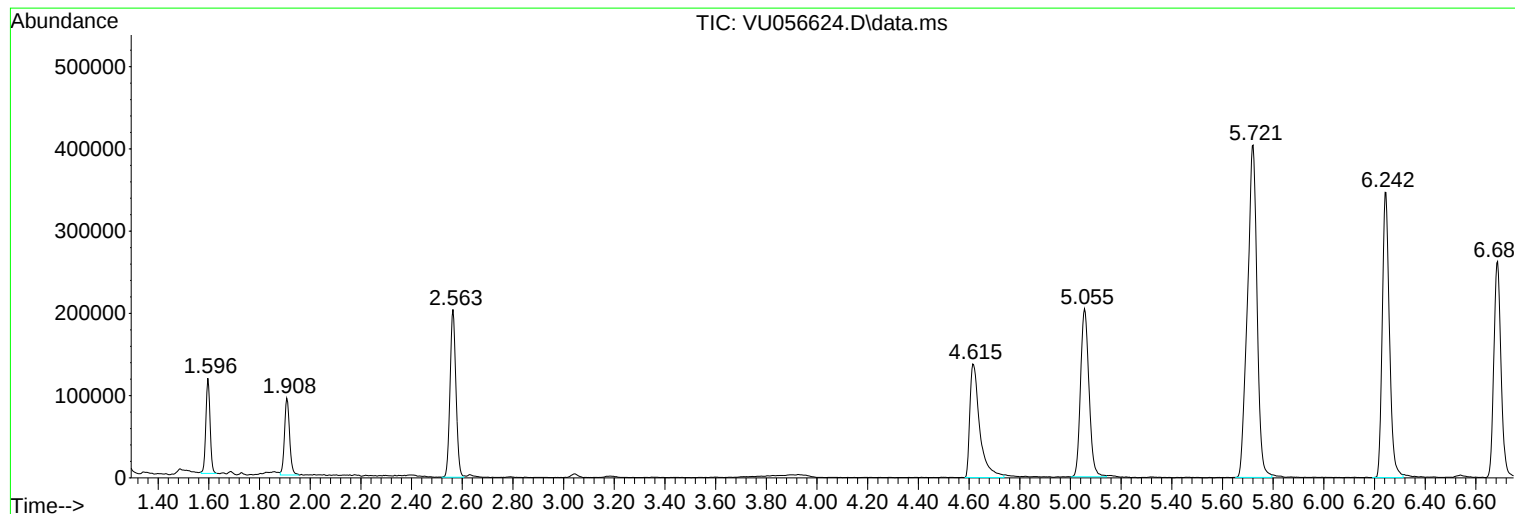

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112823\
Data File : VU056624.D
Acq On : 28 Nov 2023 12:53
Operator : MD/SY
Sample : 05554-04
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112823\
Data File : VU056624.D
Acq On : 28 Nov 2023 12:53
Operator : MD/SY
Sample : 05554-04
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc