

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112823\
 Data File : VU056627.D
 Acq On : 28 Nov 2023 14:18
 Operator : MD/SY
 Sample : 05554-04
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B29

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056627.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	111	rVB	103704	121818	12.10%	1.407%
2	1.907	184	192	205	rVB	88667	118766	11.79%	1.371%
3	2.563	384	396	410	rBV	193081	317986	31.58%	3.672%
4	4.618	1024	1035	1078	rBV2	130340	354621	35.22%	4.095%
5	5.055	1156	1171	1194	rBV	194283	438369	43.53%	5.062%
6	5.721	1355	1378	1409	rBV2	372020	988582	98.17%	11.415%
7	6.245	1528	1541	1571	rBV	405726	792799	78.73%	9.154%
8	6.685	1665	1678	1704	rBV	230262	461112	45.79%	5.324%
9	7.103	1797	1808	1820	rVB	6318	11999	1.19%	0.139%
10	7.560	1936	1950	1969	rBV	118471	213429	21.19%	2.464%
11	7.894	2041	2054	2071	rBV	447574	811286	80.56%	9.368%
12	8.177	2131	2142	2164	rBV	68684	125122	12.43%	1.445%
13	8.550	2244	2258	2272	rBV2	50867	88124	8.75%	1.018%
14	8.631	2272	2283	2318	rBV2	470752	921777	91.54%	10.644%
15	8.804	2326	2337	2351	rVB6	17420	38493	3.82%	0.444%
16	9.412	2511	2526	2564	rBV	561426	1007006	100.00%	11.628%
17	10.753	2930	2943	2961	rBV	163072	270012	26.81%	3.118%
18	11.807	3257	3271	3301	rBV	524428	879266	87.31%	10.153%
19	12.190	3375	3390	3411	rBV	407301	699760	69.49%	8.080%




Sum of corrected areas: 8660327

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112823\
Data File : VU056627.D
Acq On : 28 Nov 2023 14:18
Operator : MD/SY
Sample : 05554-04
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

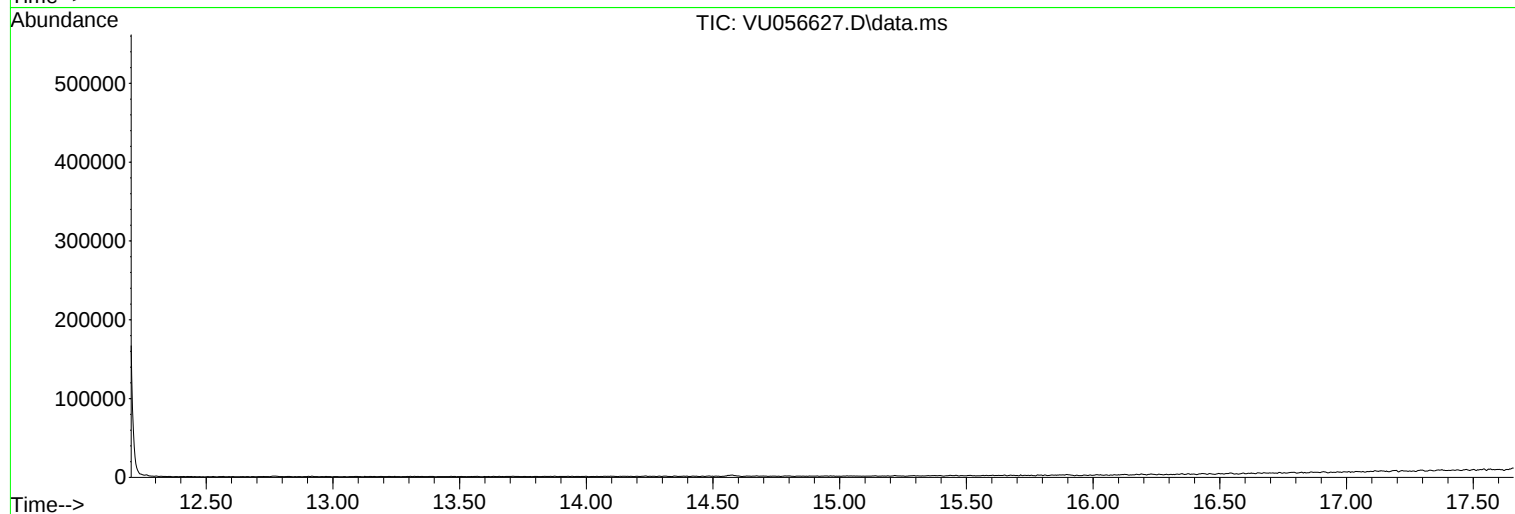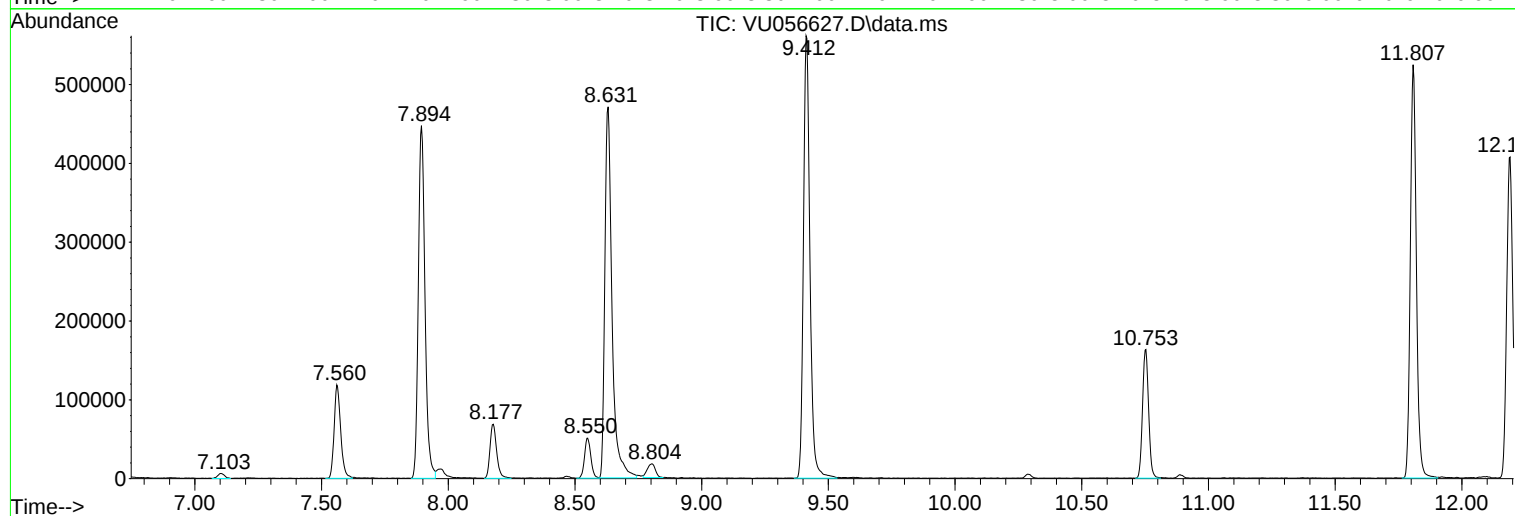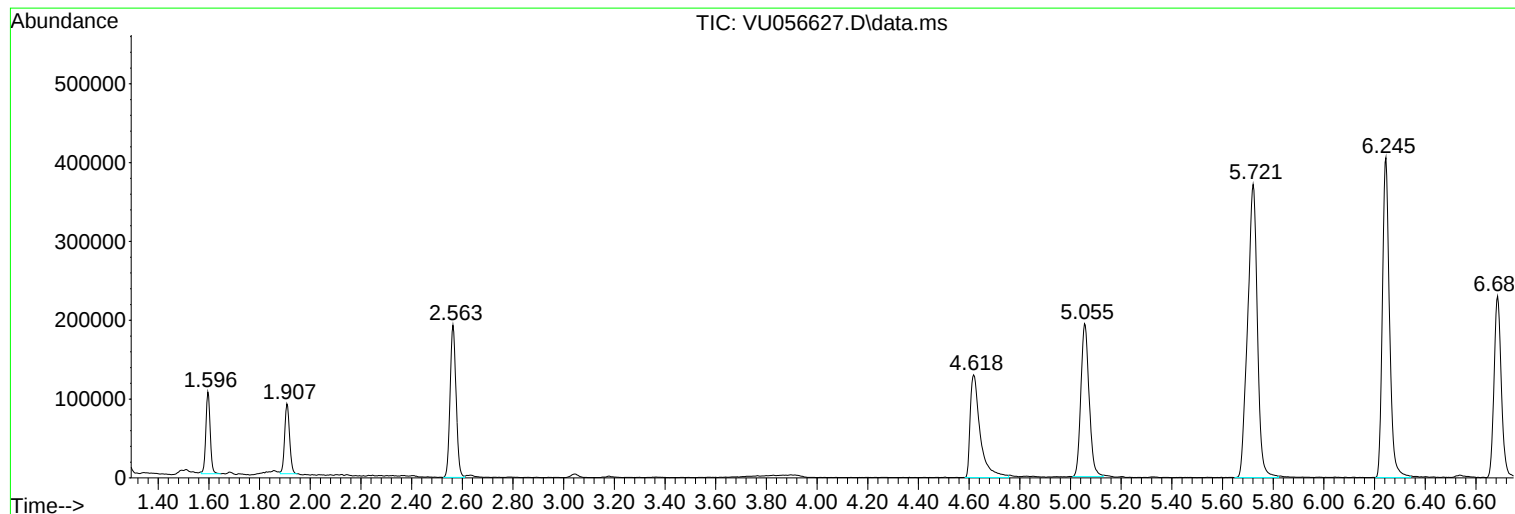

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112823\
Data File : VU056627.D
Acq On : 28 Nov 2023 14:18
Operator : MD/SY
Sample : 05554-04
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112823\
Data File : VU056627.D
Acq On : 28 Nov 2023 14:18
Operator : MD/SY
Sample : 05554-04
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc