

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112823\
 Data File : VU056629.D
 Acq On : 28 Nov 2023 15:07
 Operator : MD/SY
 Sample : 05554-03DL 4X
 Misc : 25mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0B28DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU056629.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.499	54	65	69	rBV3	5181	11104	1.04%	0.116%
2	1.596	87	95	109	rVB	113065	132253	12.41%	1.378%
3	1.907	184	192	212	rVB	93483	133827	12.56%	1.394%
4	2.563	383	396	411	rBV	205817	339182	31.83%	3.534%
5	3.039	529	544	558	rBV2	16593	32761	3.07%	0.341%
6	3.181	576	588	601	rBV2	6404	14090	1.32%	0.147%
7	4.618	1022	1035	1074	rBV	141572	393883	36.96%	4.104%
8	5.055	1151	1171	1199	rBV	208580	477993	44.85%	4.980%
9	5.718	1355	1377	1402	rBV2	405008	1065738	100.00%	11.104%
10	6.242	1527	1540	1571	rBV2	364329	723546	67.89%	7.539%
11	6.685	1662	1678	1700	rBV	251044	501148	47.02%	5.222%
12	7.560	1938	1950	1967	rBV	127021	232956	21.86%	2.427%
13	7.894	2041	2054	2089	rBV	482643	894805	83.96%	9.323%
14	8.177	2131	2142	2163	rBV	76931	135578	12.72%	1.413%
15	8.547	2242	2257	2272	rBV	425360	730949	68.59%	7.616%
16	8.631	2272	2283	2316	rVB	528903	1010841	94.85%	10.532%
17	9.412	2513	2526	2557	rBV	503547	900954	84.54%	9.387%
18	10.753	2929	2943	2962	rBV	181600	300682	28.21%	3.133%
19	11.807	3258	3271	3294	rBV	486811	801836	75.24%	8.355%
20	12.187	3376	3389	3409	rBV	448979	763401	71.63%	7.954%




Sum of corrected areas: 9597527

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112823\
Data File : VU056629.D
Acq On : 28 Nov 2023 15:07
Operator : MD/SY
Sample : 05554-03DL 4X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B28DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

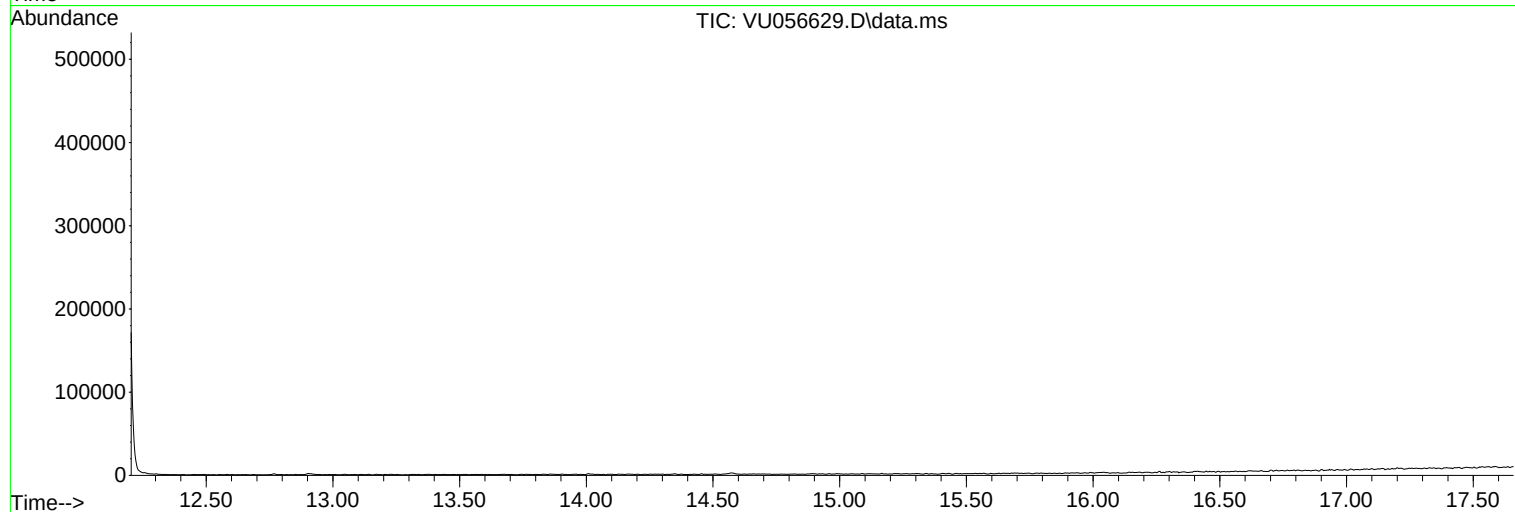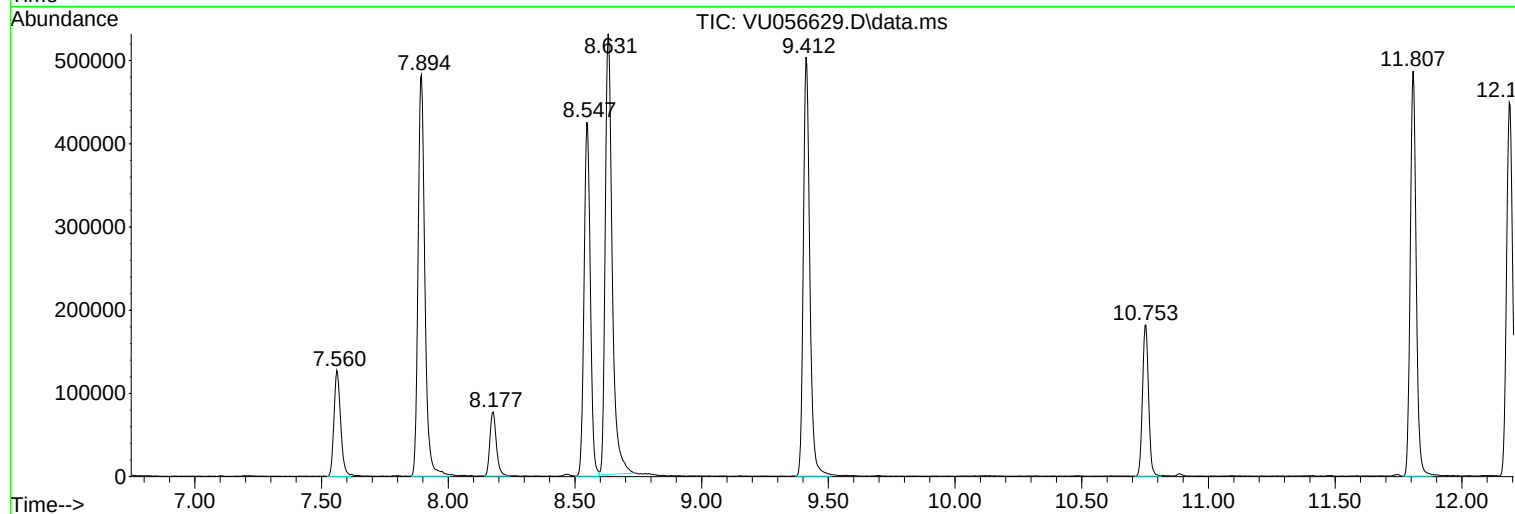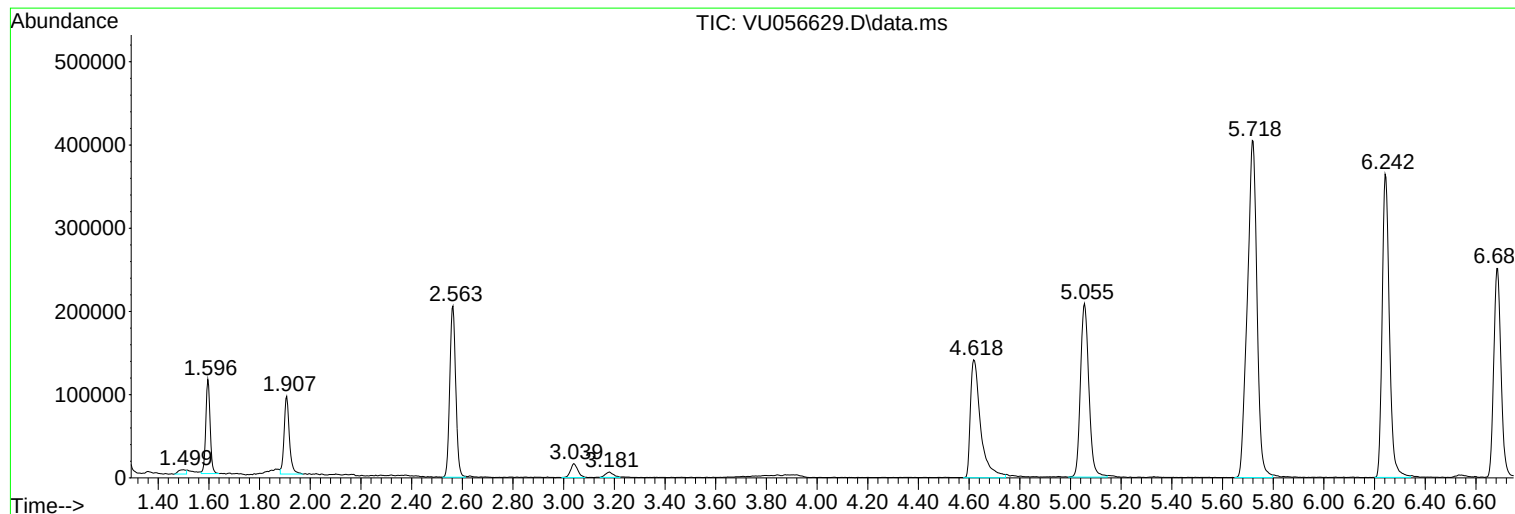

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112823\
Data File : VU056629.D
Acq On : 28 Nov 2023 15:07
Operator : MD/SY
Sample : 05554-03DL 4X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B28DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112823\
Data File : VU056629.D
Acq On : 28 Nov 2023 15:07
Operator : MD/SY
Sample : 05554-03DL 4X
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0B28DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc