
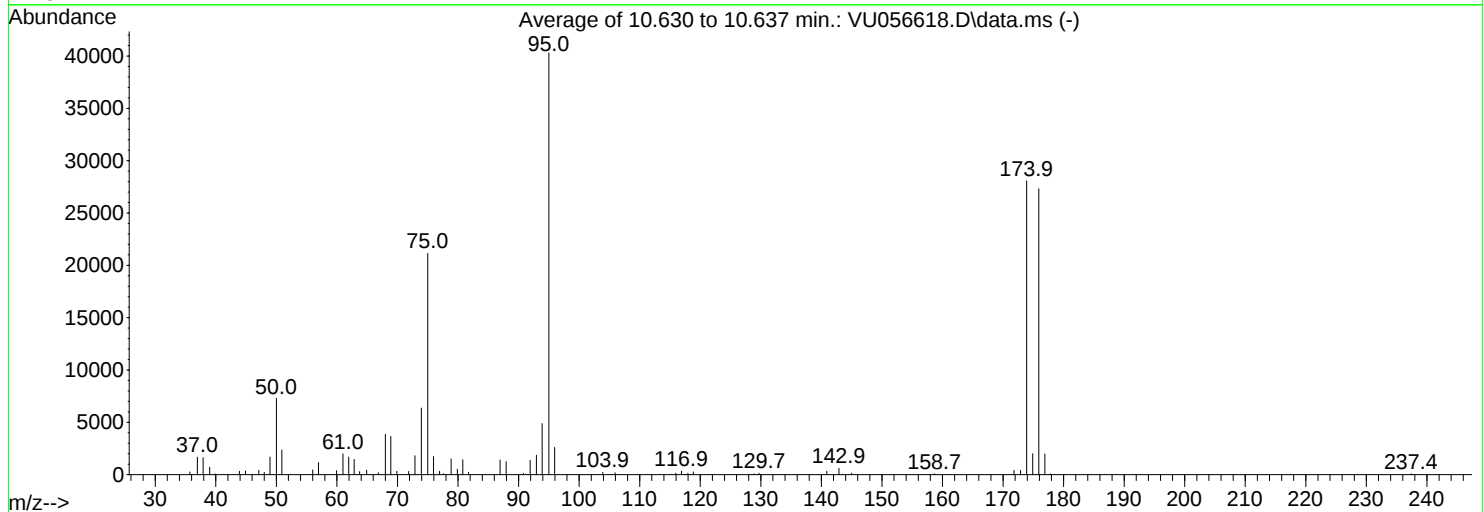


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU112823\
Data File : VU056618.D
Acq On : 28 Nov 2023 09:08
Operator : MD/SY
Sample : BFB083
Misc : 25mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB083

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR111323WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Nov 28 23:48:06 2023

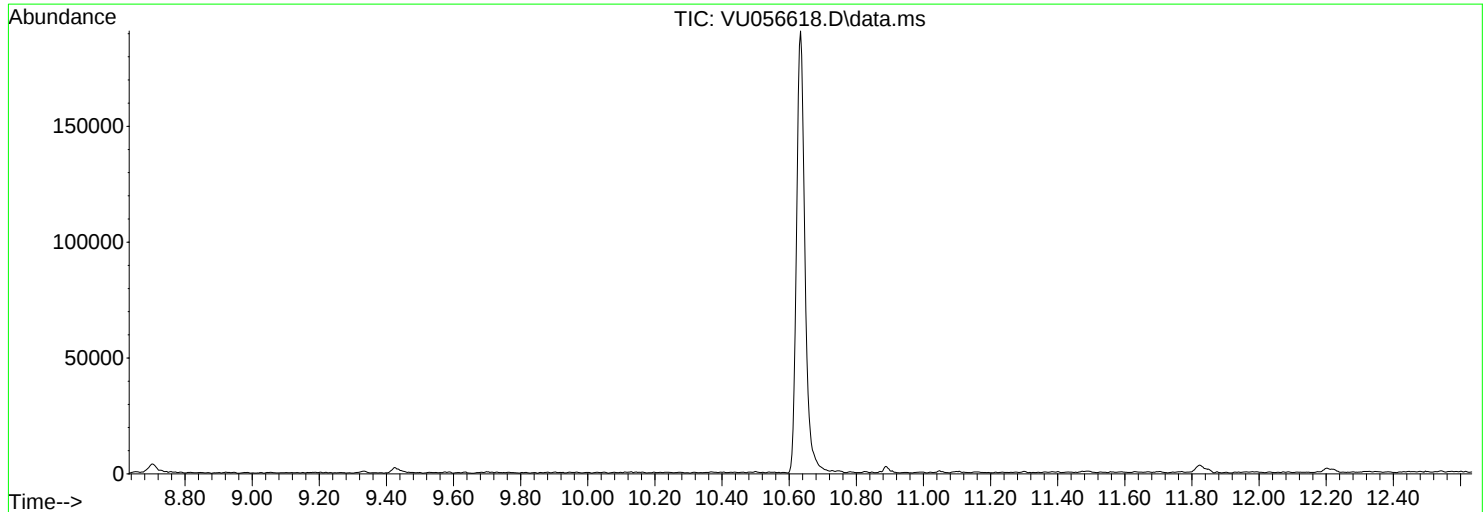

AutoFind: Scans 2905, 2906, 2907; Background Corrected with Scan 2893

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	7286	PASS
75	95	30	80	52.5	21147	PASS
95	95	100	100	100.0	40304	PASS
96	95	5	9	6.5	2605	PASS
173	174	0.00	2	1.5	412	PASS
174	95	50	120	69.6	28069	PASS
175	174	5	9	7.2	2008	PASS
176	174	95	101	97.4	27328	PASS
177	176	5	9	7.2	1970	PASS

m/z	Abundance
39.90	117.0
43.90	359.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

m/z	Abundance
35.70	275.0
37.00	1715.0
37.90	1668.0
39.00	786.0
40.00	228.0
44.00	660.0
45.00	395.0
47.10	343.0
48.00	205.0
48.90	1618.0
50.00	7098.0
50.90	2167.0
56.00	470.0
56.90	1094.0
59.90	382.0
61.00	2052.0
62.00	1725.0
62.90	1536.0
63.70	297.0
64.90	409.0
67.00	185.0
68.00	3851.0
68.90	3777.0
69.90	360.0
71.80	357.0
72.90	1958.0
73.90	6401.0
75.00	20928.0
75.90	1686.0
76.90	299.0
77.60	157.0
78.80	1473.0
79.90	418.0
80.80	1496.0
81.80	226.0
87.00	1220.0
87.90	1288.0
91.90	1549.0
92.90	1777.0
93.90	4775.0
95.00	40864.0
95.90	2679.0
103.90	242.0
106.00	195.0
115.90	121.0
116.90	266.0
117.90	163.0
118.90	273.0
127.90	112.0
128.90	120.0
129.70	133.0
141.00	331.0
142.90	579.0
145.00	148.0
171.90	463.0
172.90	347.0
173.90	27648.0
174.90	1843.0
175.90	26992.0
176.90	2023.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

m/z	Abundance
35.70	262.0
37.00	1707.0
37.90	1676.0
39.00	725.0
40.00	200.0
44.00	685.0
44.90	358.0
47.10	441.0
48.00	223.0
49.00	1735.0
50.00	7686.0
50.90	2524.0
56.00	515.0
57.00	1172.0
59.90	396.0
61.00	2056.0
62.00	1703.0
62.90	1454.0
63.80	306.0
64.90	429.0
66.80	185.0
68.00	3965.0
68.90	3704.0
69.90	336.0
71.80	327.0
72.90	1882.0
74.00	6507.0
75.00	21904.0
75.90	1744.0
77.00	364.0
77.60	134.0
78.80	1514.0
79.90	558.0
80.80	1450.0
81.70	202.0
86.90	1391.0
88.00	1198.0
90.80	150.0
91.90	1417.0
93.00	1920.0
93.90	4980.0
95.00	41536.0
95.90	2664.0
103.90	227.0
106.00	192.0
116.00	140.0
116.90	332.0
118.00	145.0
118.80	262.0
128.90	107.0
129.70	144.0
140.90	330.0
142.90	623.0
145.00	143.0
158.70	122.0
171.80	410.0
172.90	425.0
173.90	28856.0
174.90	2035.0
175.90	28080.0
176.90	2052.0
177.90	107.0
237.40	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083

m/z	Abundance
35.70	225.0
36.90	1603.0
37.90	1524.0
39.00	598.0
39.90	166.0
43.90	677.0
44.80	291.0
47.10	467.0
48.00	206.0
49.00	1674.0
50.00	7074.0
50.90	2387.0
56.00	404.0
57.00	1186.0
60.00	384.0
61.00	1853.0
61.90	1617.0
62.80	1387.0
63.80	257.0
64.90	436.0
66.80	185.0
68.00	3768.0
68.90	3481.0
69.90	273.0
71.90	243.0
72.90	1565.0
74.00	6186.0
75.00	20608.0
76.00	1739.0
76.90	317.0
78.90	1518.0
79.90	587.0
80.80	1323.0
81.70	230.0
86.90	1601.0
88.00	1256.0
90.80	204.0
91.90	1160.0
93.00	1880.0
93.90	4856.0
95.00	38512.0
96.00	2471.0
103.90	194.0
105.90	168.0
115.90	136.0
116.90	343.0
117.60	116.0
118.00	108.0
118.80	272.0
129.70	146.0
140.80	353.0
142.90	610.0
145.00	122.0
158.70	105.0
171.70	351.0
172.90	463.0
173.90	27704.0
174.90	2145.0
175.90	26912.0
176.90	1836.0
177.80	118.0
237.40	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB083